


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE101119\
 Data File : BE100632.D
 Acq On : 11 Oct 2019 8:35
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE101019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 10 14:01:52 2019

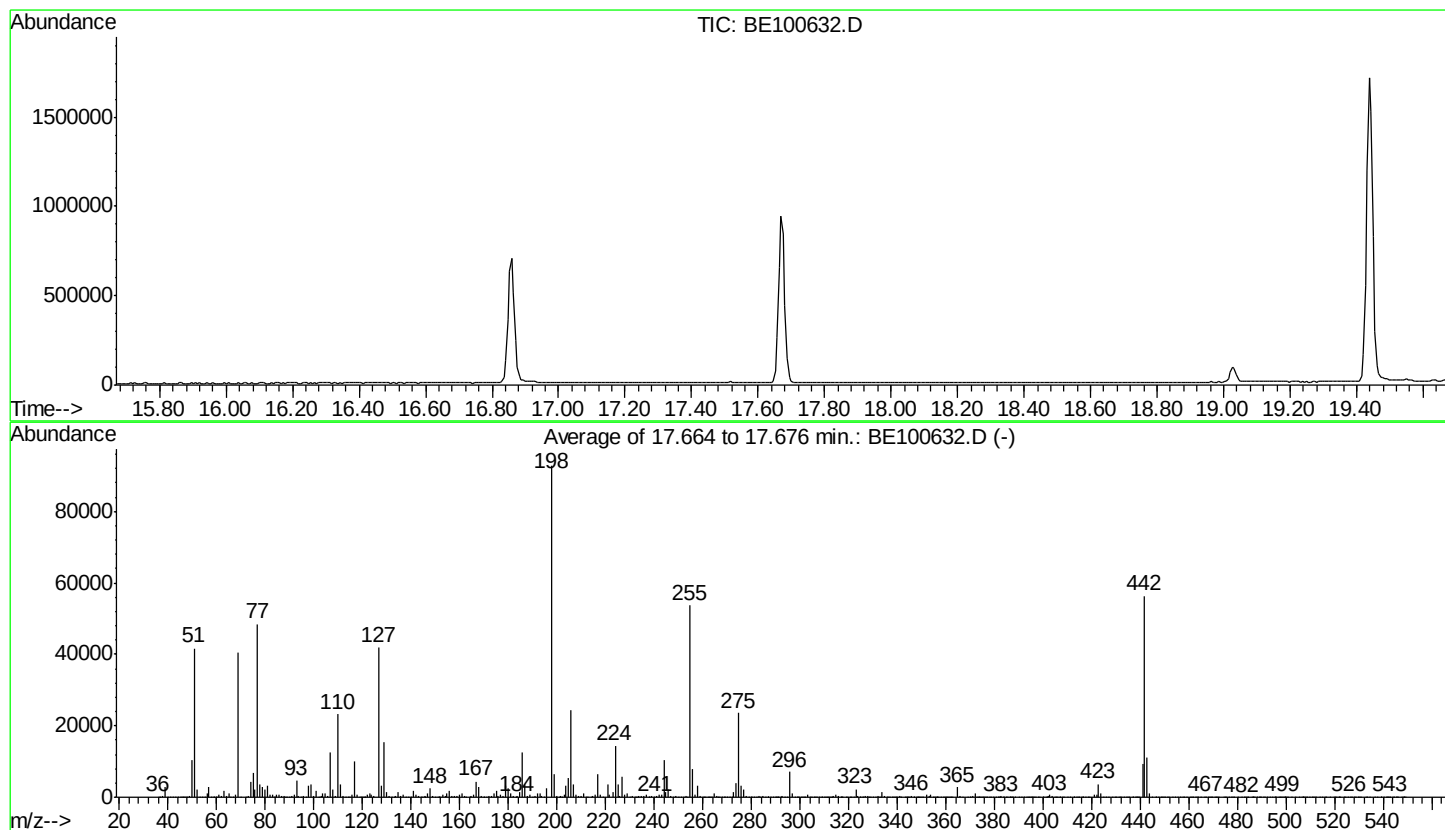

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2559

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.9	41711	PASS
68	69	0.00	2	2.0	805	PASS
69	198	0.00	100	43.5	40354	PASS
70	69	0.00	2	0.4	164	PASS
127	198	10	80	45.0	41771	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	92810	PASS
199	198	5	9	7.0	6475	PASS
275	198	10	60	25.4	23611	PASS
365	198	1	100	3.1	2833	PASS
441	198	0.01	100	10.0	9312	PASS
442	198	50	100	60.8	56402	PASS
443	442	15	24	19.7	11093	PASS