
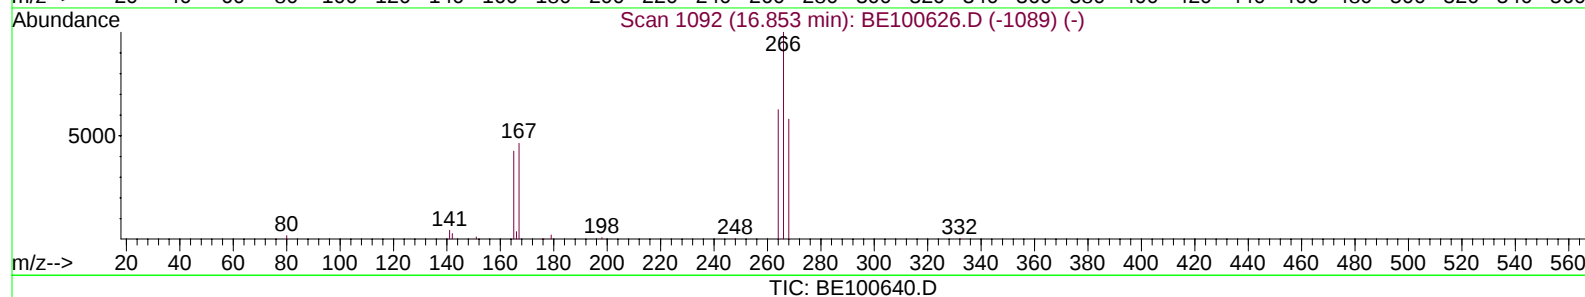
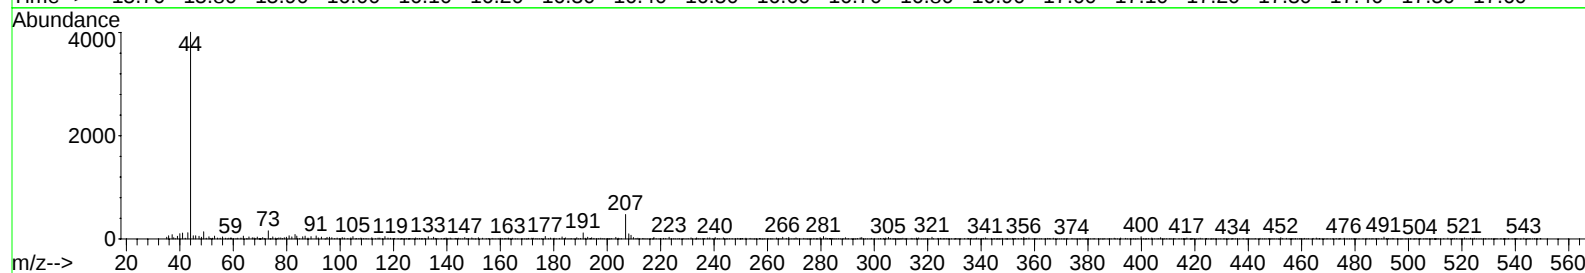


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE101519\
Data File : BE100640.D
Acq On : 15 Oct 2019 8:32
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 15 17:47:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 10 14:01:52 2019
Response via : Initial Calibration

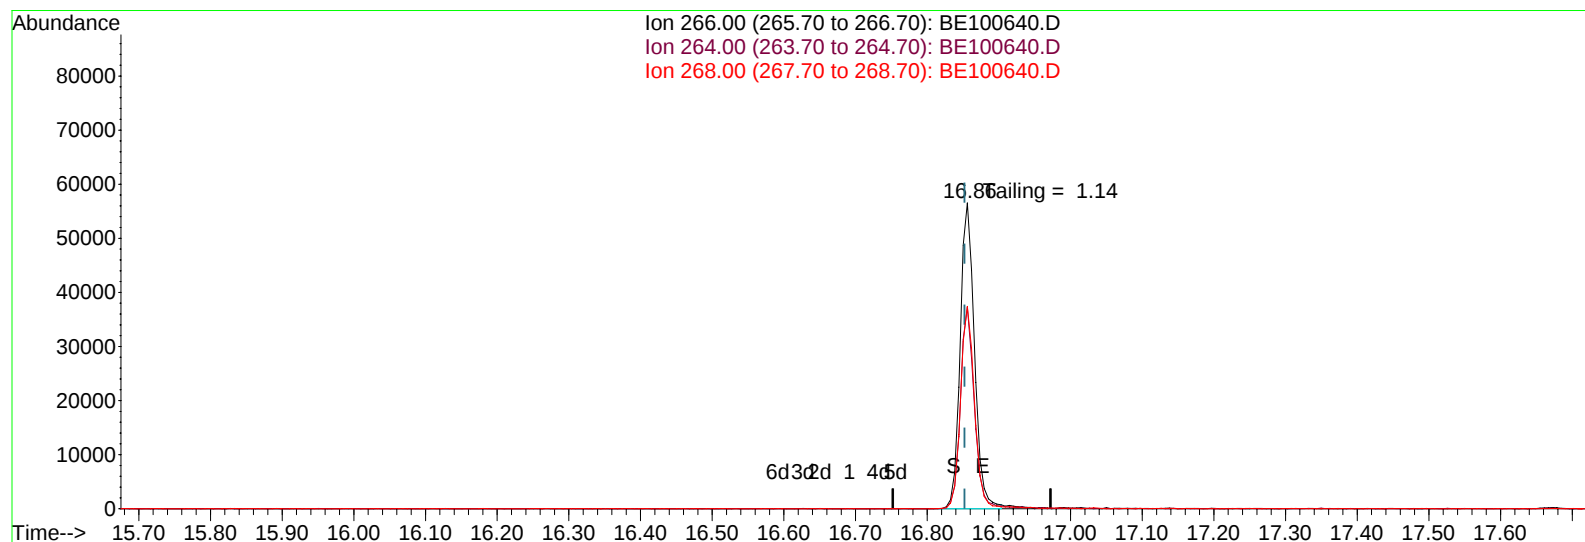

(22) Pentachlorophenol

16.692min (-0.160) 7.86ng

response 27

Ion	Exp%	Act%
266.00	100	100
264.00	63.40	22.86#
268.00	60.60	91.43#
0.00	0.00	0.00