


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE101519\
Data File : BE100640.D
Acq On : 15 Oct 2019 8:32
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE101019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 10 14:01:52 2019

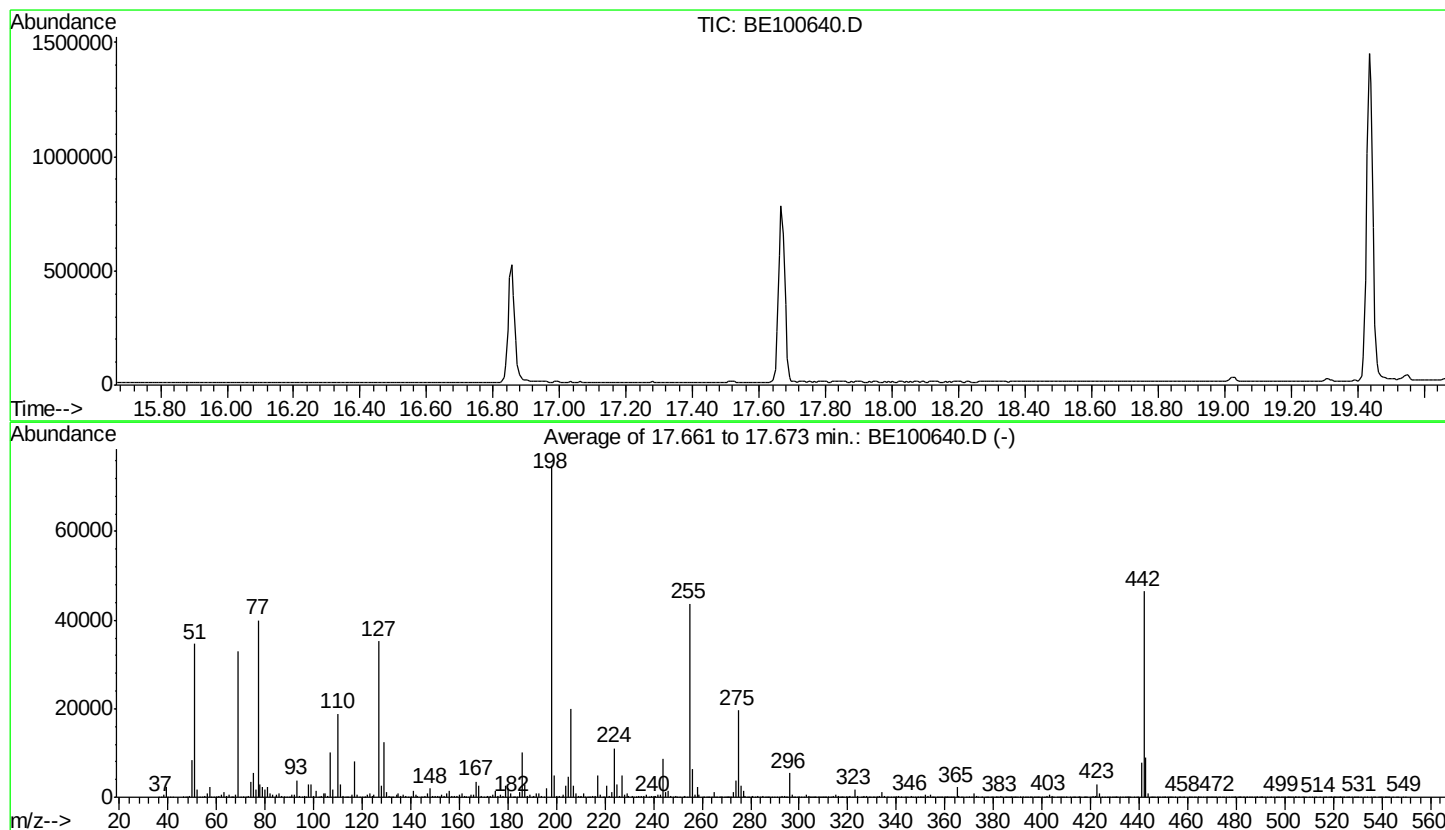

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	34668	PASS
68	69	0.00	2	2.0	647	PASS
69	198	0.00	100	43.9	32858	PASS
70	69	0.00	2	0.3	83	PASS
127	198	10	80	47.0	35205	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	74888	PASS
199	198	5	9	6.6	4918	PASS
275	198	10	60	26.1	19528	PASS
365	198	1	100	3.0	2216	PASS
441	198	0.01	100	10.4	7798	PASS
442	198	50	100	62.0	46454	PASS
443	442	15	24	19.4	9032	PASS