

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE101618\
 Data File : BE097925.D
 Acq On : 17 Oct 2018 00:23
 Operator : SJ/JU
 Sample : J5317-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 RE-122D3-20181004

Quant Time: Oct 17 08:00:17 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE101618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 16 15:36:44 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	1969	0.40	ng	0.00
7) Naphthalene-d8	10.69	136	8600	0.40	ng	0.00
13) Acenaphthene-d10	14.54	164	5928	0.40	ng	-0.01
19) Phenanthrene-d10	17.29	188	19205	0.40	ng	-0.01
27) Chrysene-d12	21.48	240	27690	0.40	ng	-0.01
34) Perylene-d12	24.03	264	22269	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.47	112	1228	0.20	ng	0.00
5) Phenol-d6	7.06	99	1086	0.12	ng	0.00
8) Nitrobenzene-d5	9.04	82	3151	0.39	ng	0.00
11) 2-Methylnaphthalene-d10	12.28	152	5487	0.38	ng	-0.01
14) 2,4,6-Tribromophenol	16.04	330	1258	0.39	ng	0.00
15) 2-Fluorobiphenyl	13.18	172	10495	0.43	ng	0.00
25) Fluoranthene-d10	19.33	212	116739	0.45	ng	0.00
29) Terphenyl-d14	19.92	244	32626	0.51	ng	0.00
Target Compounds						
22) Pentachlorophenol	16.95	266	3	0.031	ng	# 55
32) Bis(2-ethylhexyl)phthalate	21.39	149	15670	Below	Cal	99
33) Indeno(1,2,3-cd)pyrene	26.73	276	10	Below	Cal	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE101618\
Data File : BE097925.D
Acq On : 17 Oct 2018 00:23
Operator : SJ/JU
Sample : J5317-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
RE-122D3-20181004

Quant Time: Oct 17 08:00:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE101618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 16 15:36:44 2018
Response via : Initial Calibration

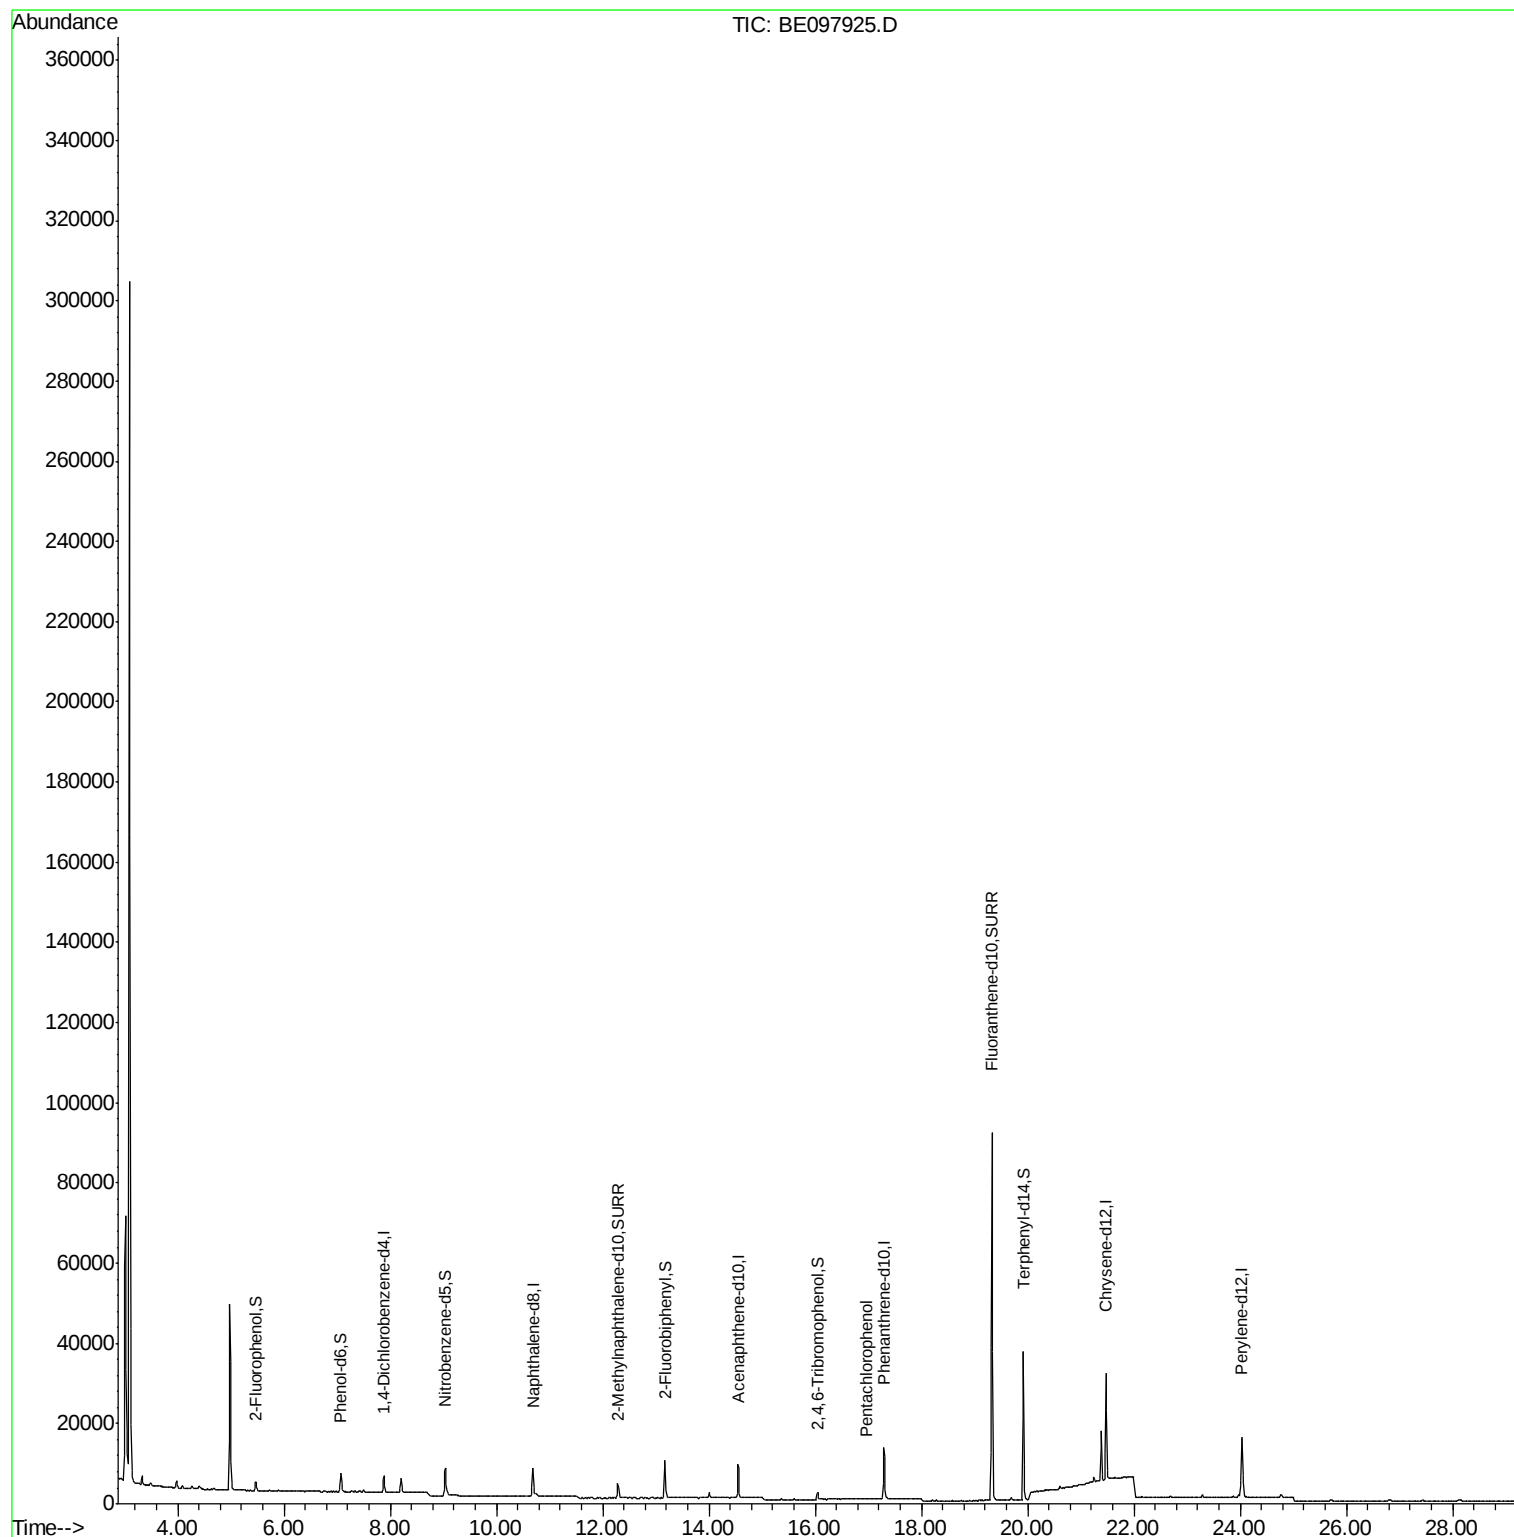




#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.88 min Scan# 436
Delta R.T. -0.00 min
Lab File: BE097925.D
Acq: 17 Oct 2018 00:23

Instrument :
BNA_E
ClientSampleId :
RE-122D3-20181004

Tot Ion:152 Resp: 1969
Ion Ratio Lower Upper
152 100
150 150.3 118.2 177.4
115 62.9 50.9 76.3

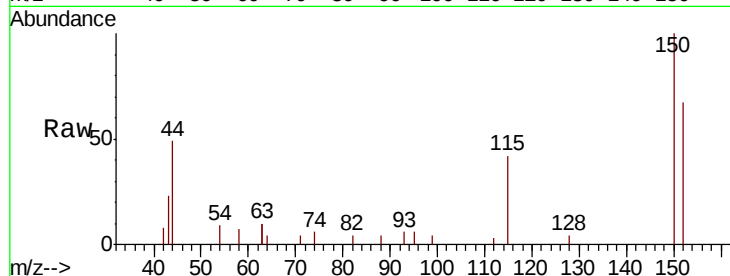


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

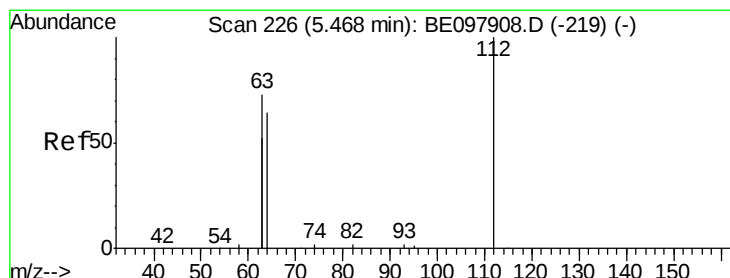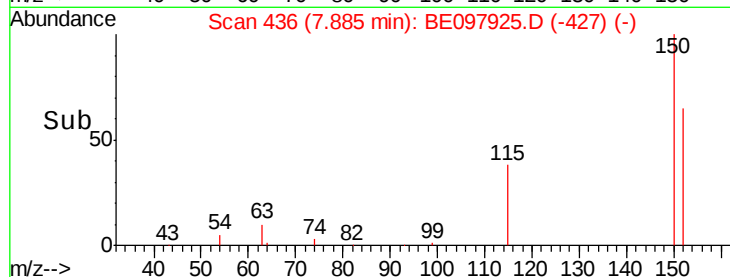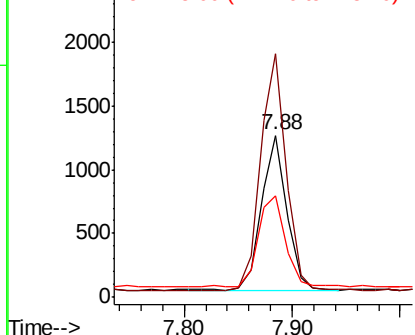



#4


2-Fluorophenol
Concen: 0.198 ng
RT: 5.47 min Scan# 226
Delta R.T. -0.00 min
Lab File: BE097925.D
Acq: 17 Oct 2018 00:23

Tgt Ion:112 Resp: 1228
Ion Ratio Lower Upper
112 100
64 70.3 58.9 88.3
63 143.9 120.3 180.5

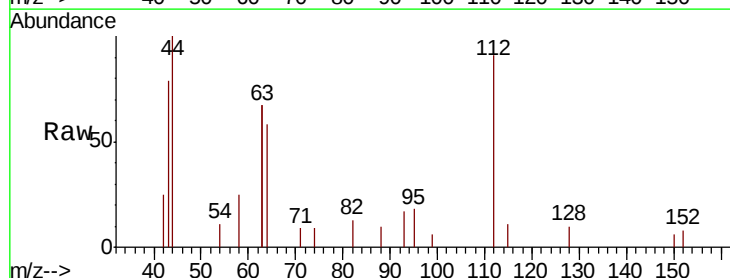

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BE0
Ion 63.00 (62.70 to 63.70): BE0

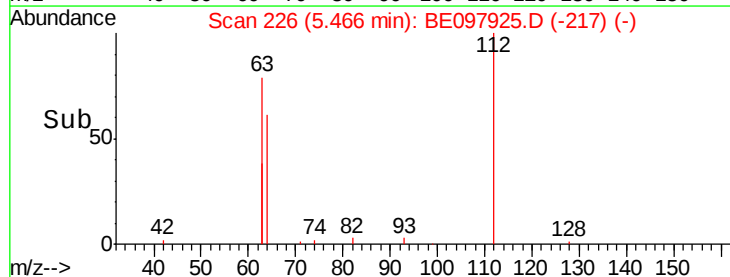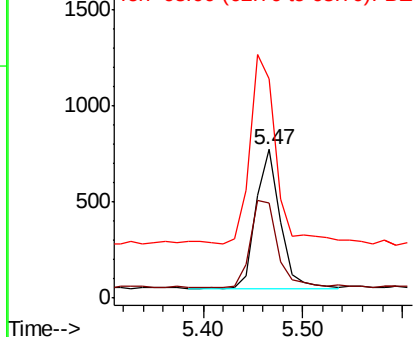



#5

Phenol-d6

Concen: 0.118 ng

RT: 7.06 min Scan# 364

Delta R.T. -0.00 min

Lab File: BE097925.D

Acq: 17 Oct 2018 00:23

Instrument :

BNA_E

ClientSampleId :

RE-122D3-20181004


Tot Ion: 99 Resp: 1086

Ion Ratio Lower Upper

99 100

42 46.7 19.9 29.9#




71 38.9 27.8 41.8

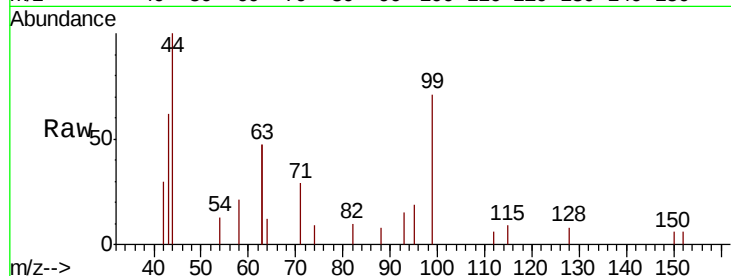

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

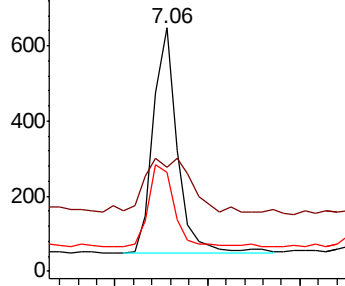

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.69 min Scan# 656

Delta R.T. -0.00 min

Lab File: BE097925.D

Acq: 17 Oct 2018 00:23

Tgt Ion: 136 Resp: 8600


Ion Ratio Lower Upper

136 100

137 12.2 9.6 14.4

54 33.7 27.7 41.5

68 6.4 5.3 7.9






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

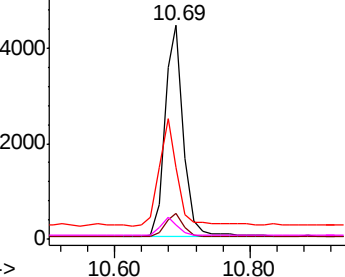


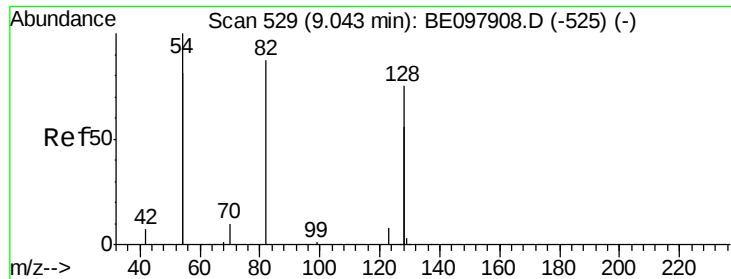




#8
 Nitrobenzene-d5
 Concen: 0.387 ng
 RT: 9.04 min Scan# 529
 Delta R.T. -0.00 min
 Lab File: BE097925.D
 Acq: 17 Oct 2018 00:23

Instrument :
 BNA_E
 ClientSampleId :
 RE-122D3-20181004

Tot Ion	Ratio	Lower	Upper
82	100		
128	168.8	129.9	194.9
54	221.1	174.0	261.0

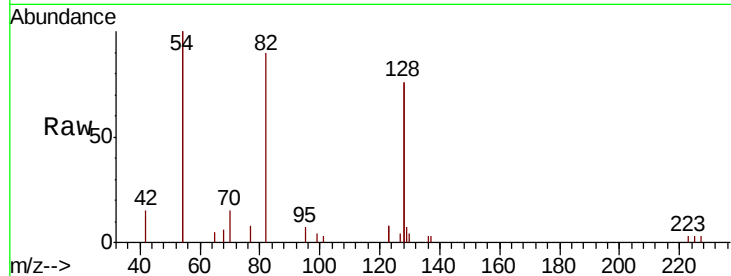


Abundance Ion 82.00 (81.70 to 82.70): BE0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BE0


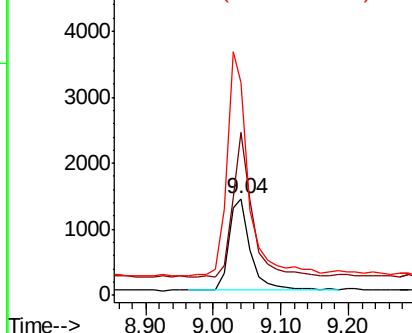



#11
 2-Methylnaphthalene-d10
 Concen: 0.384 ng
 RT: 12.28 min Scan# 768
 Delta R.T. -0.01 min
 Lab File: BE097925.D
 Acq: 17 Oct 2018 00:23

Tgt Ion	Ratio	Lower	Upper
152	100		
151	18.8	16.2	24.4



Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 151.00 (150.70 to 151.70): E

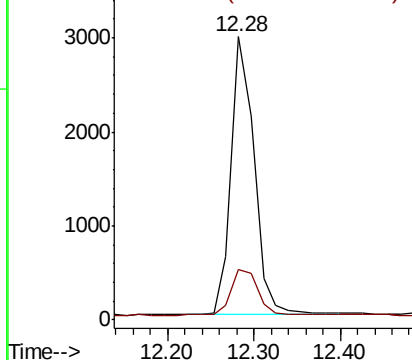



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.54 min Scan# 925

Delta R.T. -0.01 min

Lab File: BE097925.D

Acq: 17 Oct 2018 00:23

Instrument :

BNA_E

ClientSampleId :

RE-122D3-20181004


Tot Ion:164 Resp: 5928

Ion Ratio Lower Upper

164 100

162 104.0 77.4 116.2




160 49.4 36.5 54.7

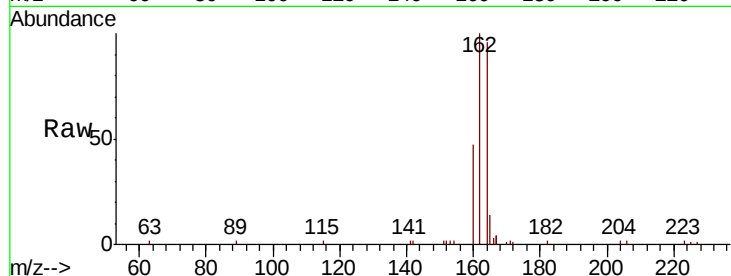

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

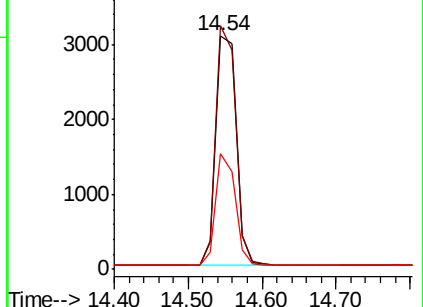

#14

2,4,6-Tribromophenol

Concen: 0.395 ng

RT: 16.04 min Scan# 1043

Delta R.T. -0.00 min

Lab File: BE097925.D

Acq: 17 Oct 2018 00:23


Tgt Ion:330 Resp: 1258

Ion Ratio Lower Upper

330 100

332 96.7 76.5 114.7



141 36.9 31.8 47.6




Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

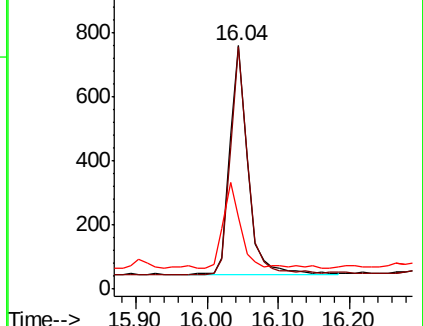

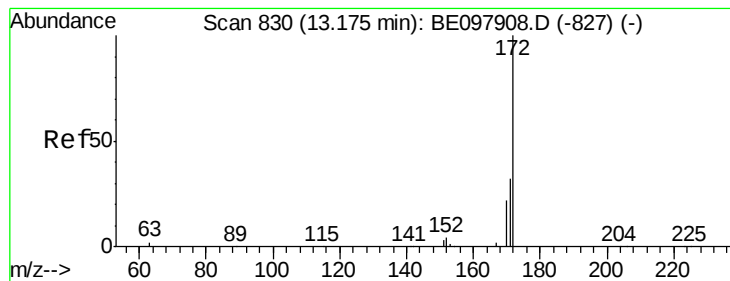

#15

2-Fluorobiphenyl

Concen: 0.433 ng

RT: 13.18 min Scan# 830

Delta R.T. 0.00 min

Lab File: BE097925.D

Acq: 17 Oct 2018 00:23

Instrument :

BNA_E

ClientSampleId :

RE-122D3-20181004


Tot Ion:172 Resp: 10495

Ion Ratio Lower Upper

172 100

171 31.9 26.0 39.0




170 20.8 18.0 27.0

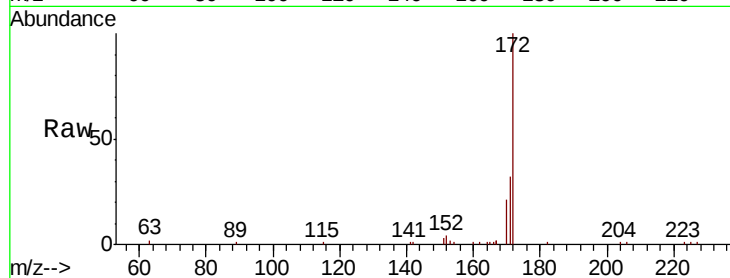

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

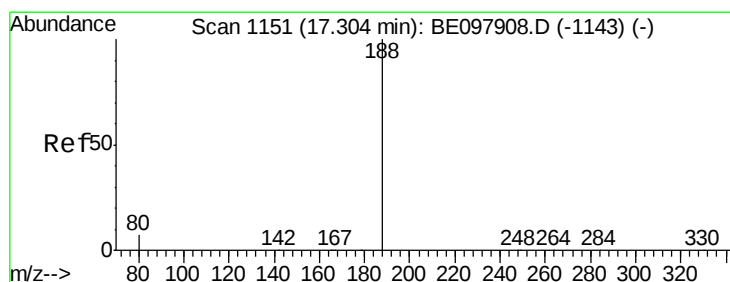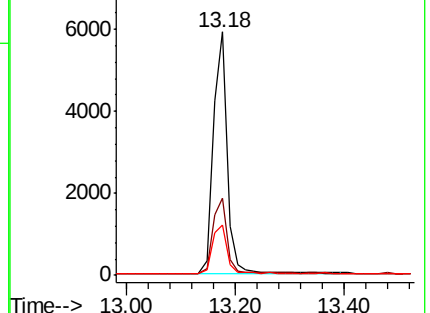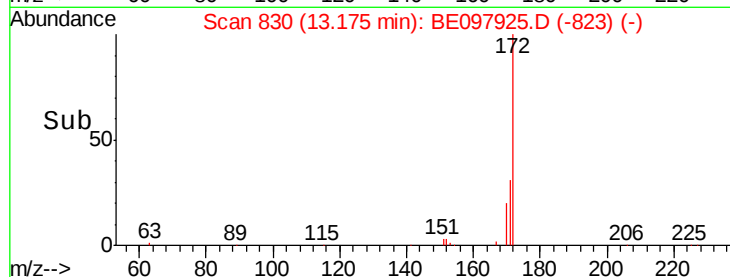

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.29 min Scan# 1150

Delta R.T. -0.01 min

Lab File: BE097925.D

Acq: 17 Oct 2018 00:23


Tgt Ion:188 Resp: 19205

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0



80 12.6 6.3 9.5#

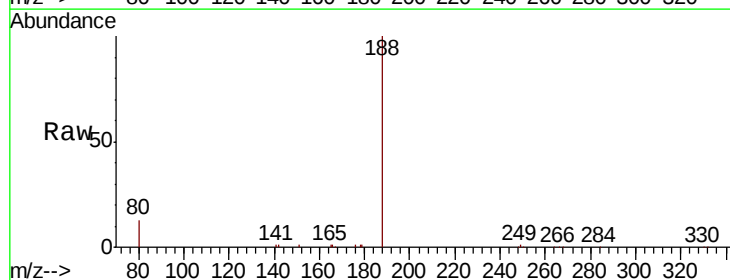


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

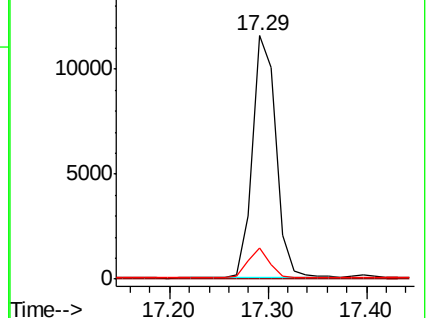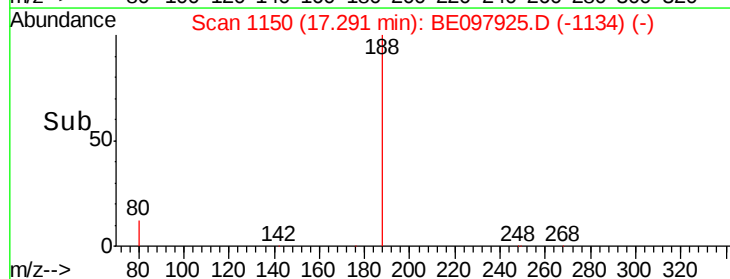



#22

Pentachlorophenol

Concen: 0.031 ng

RT: 16.95 min Scan# 1121

Delta R.T. -0.01 min

Lab File: BE097925.D

Acq: 17 Oct 2018 00:23





Instrument :

BNA_E

ClientSampleId :

RE-122D3-20181004

Tot	Ion:266	Resp:	3
Ion	Ratio	Lower	Upper
266	100		
264	92.3	51.3	76.9#
268	103.8	50.1	75.1#

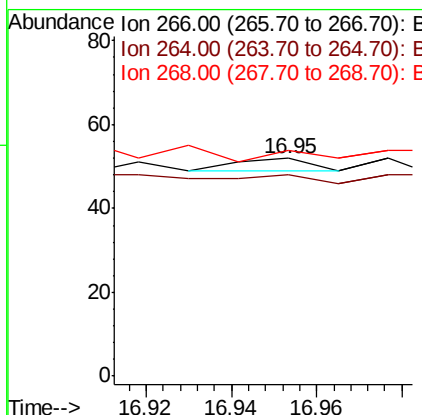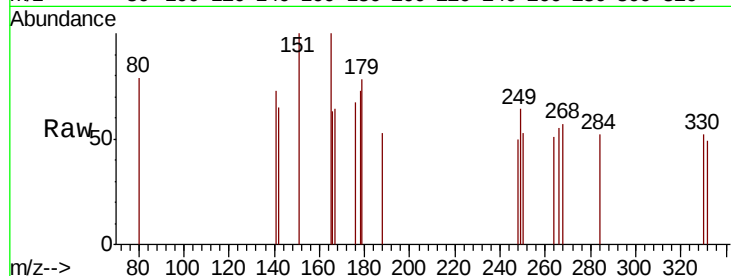

#25

Fluoranthene-d10

Concen: 0.449 ng




RT: 19.33 min Scan# 1436


Delta R.T. -0.01 min

Lab File: BE097925.D

Acq: 17 Oct 2018 00:23

Tgt Ion	212	Resp: Lower	116739 Upper
212	100		
106	3.0	2.3	3.5
104	1.6	1.3	1.9

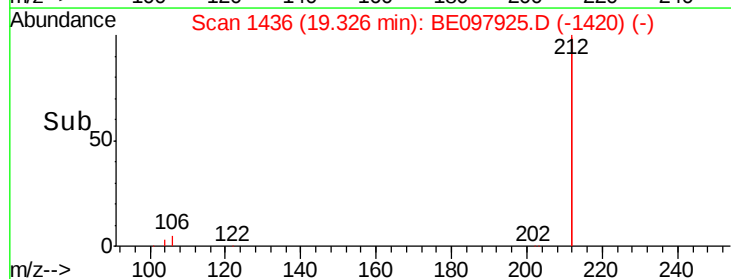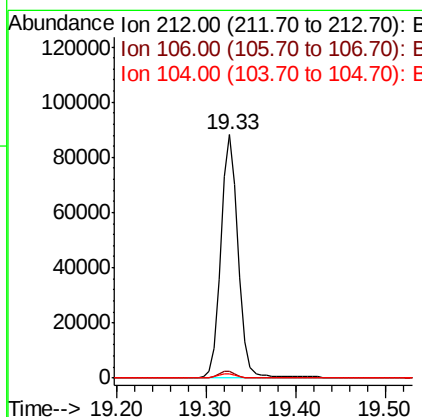



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.48 min Scan# 1672

Delta R.T. -0.01 min

Lab File: BE097925.D

Acq: 17 Oct 2018 00:23

Instrument :

BNA_E

ClientSampleId :

RE-122D3-20181004


Tot Ion:240 Resp: 27690

Ion Ratio Lower Upper

240 100

120 11.0 7.1 10.7#




236 27.0 21.3 31.9



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

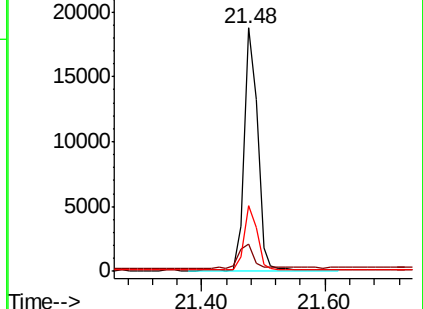

#29

Terphenyl-d14

Concen: 0.514 ng

RT: 19.92 min Scan# 1540

Delta R.T. -0.01 min

Lab File: BE097925.D

Acq: 17 Oct 2018 00:23


Tgt Ion:244 Resp: 32626

Ion Ratio Lower Upper

244 100

212 29.6 26.2 39.2



122 8.6 7.7 11.5




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

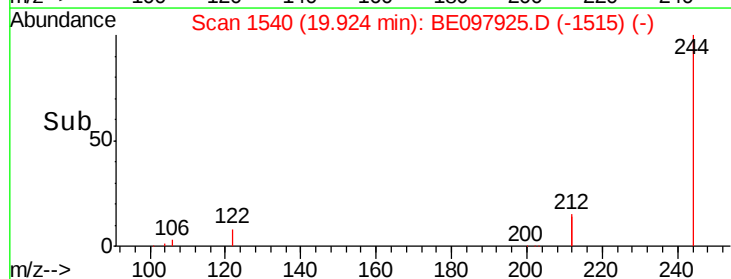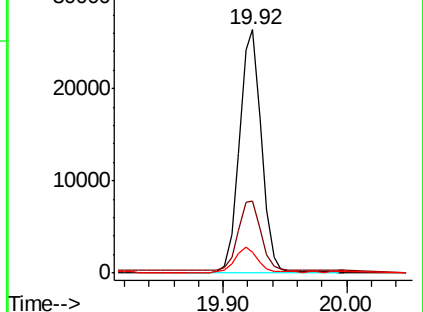

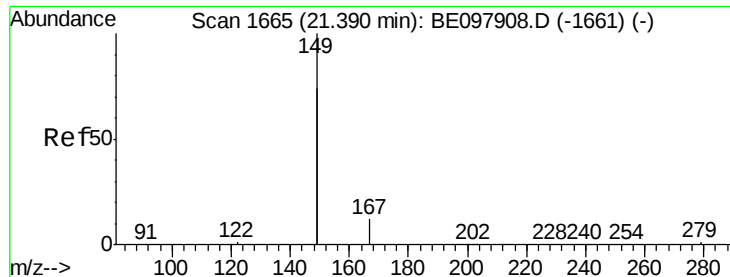

#32

Bis(2-ethylhexyl)phthalate

Concen: Below Cal

RT: 21.39 min Scan# 1665

Delta R.T. 0.00 min

Lab File: BE097925.D

Acq: 17 Oct 2018 00:23

Instrument :

BNA_E

ClientSampleId :

RE-122D3-20181004


Tot Ion:149 Resp: 15670

Ion Ratio Lower Upper

149 100

167 7.2 5.6 8.4




279 1.2 0.9 1.3

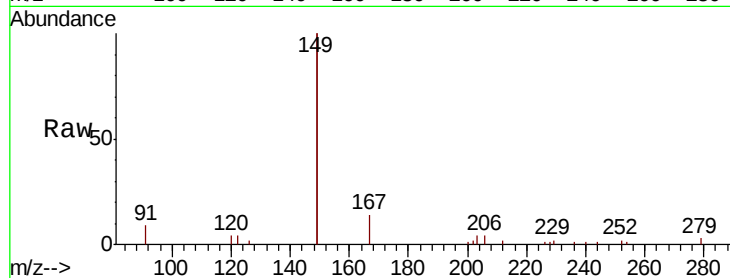

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

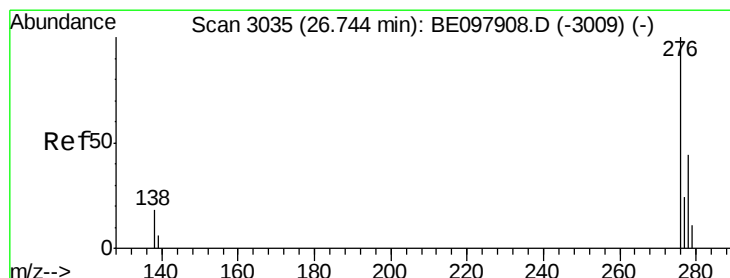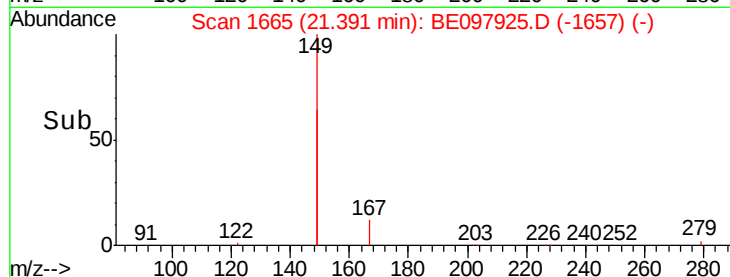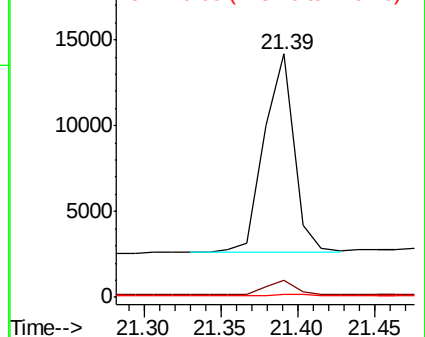

#33

Indeno(1,2,3-cd)pyrene

Concen: Below Cal

RT: 26.73 min Scan# 3032

Delta R.T. -0.01 min

Lab File: BE097925.D

Acq: 17 Oct 2018 00:23


Tgt Ion:276 Resp: 10

Ion Ratio Lower Upper

276 100

138 100.0 17.0 25.6#



277 50.0 20.5 30.7#



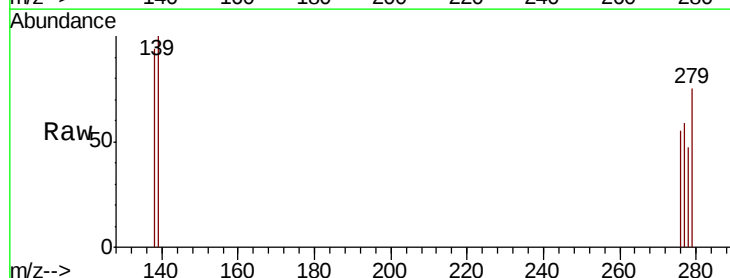


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

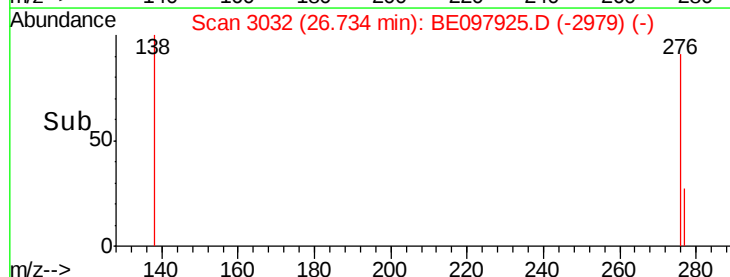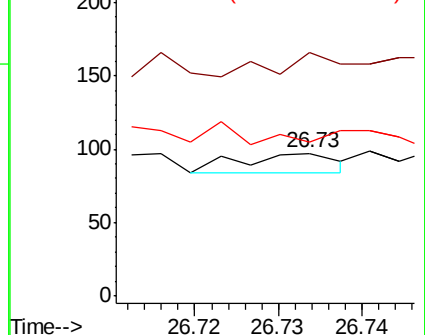

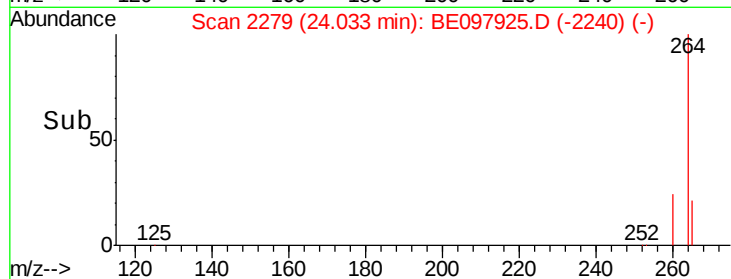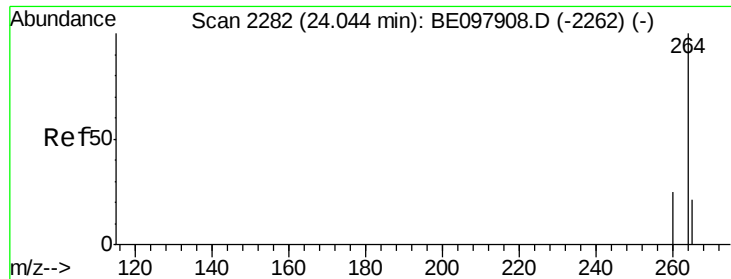

#34

Pervlene-d12

Concen: 0.400 ng

RT: 24.03 min Scan# 2279

Delta R.T. -0.01 min

Lab File: BE097925.D

Acq: 17 Oct 2018 00:23

Instrument :

BNA_E

ClientSampleId :

RE-122D3-20181004

Tot Ion:264 Resp: 22269

Ion Ratio Lower Upper

264 100

260 24.7 21.1 31.7

265 27.3 29.2 43.8#

