


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE101618\
 Data File : BE097904.D
 Acq On : 16 Oct 2018 10:40
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE101618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 16 15:36:44 2018

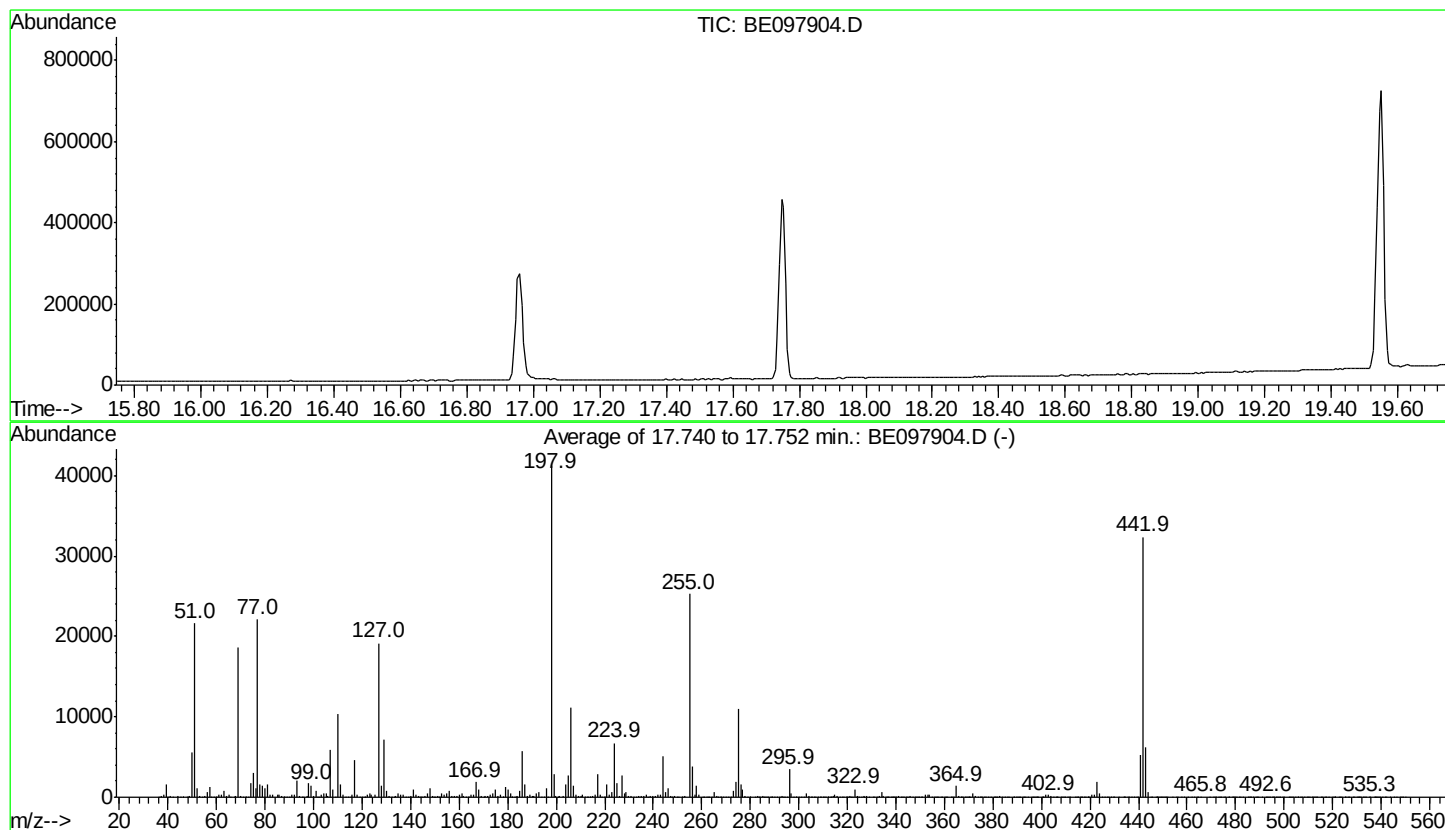

AutoFind: Scans 2579, 2580, 2581; Background Corrected with Scan 2572

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.3	21573	PASS
68	69	0.00	2	0.8	147	PASS
69	198	0.00	100	45.2	18639	PASS
70	69	0.00	2	0.6	110	PASS
127	198	10	80	46.4	19142	PASS
197	198	0.00	2	0.2	72	PASS
198	198	100	100	100.0	41224	PASS
199	198	5	9	6.8	2806	PASS
275	198	10	60	26.7	11021	PASS
365	198	1	100	3.3	1379	PASS
441	198	0.01	100	12.8	5289	PASS
442	198	50	100	78.5	32367	PASS
443	442	15	24	19.0	6148	PASS