


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE101718\
 Data File : BE097949.D
 Acq On : 17 Oct 2018 16:26
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE101618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 16 15:36:44 2018

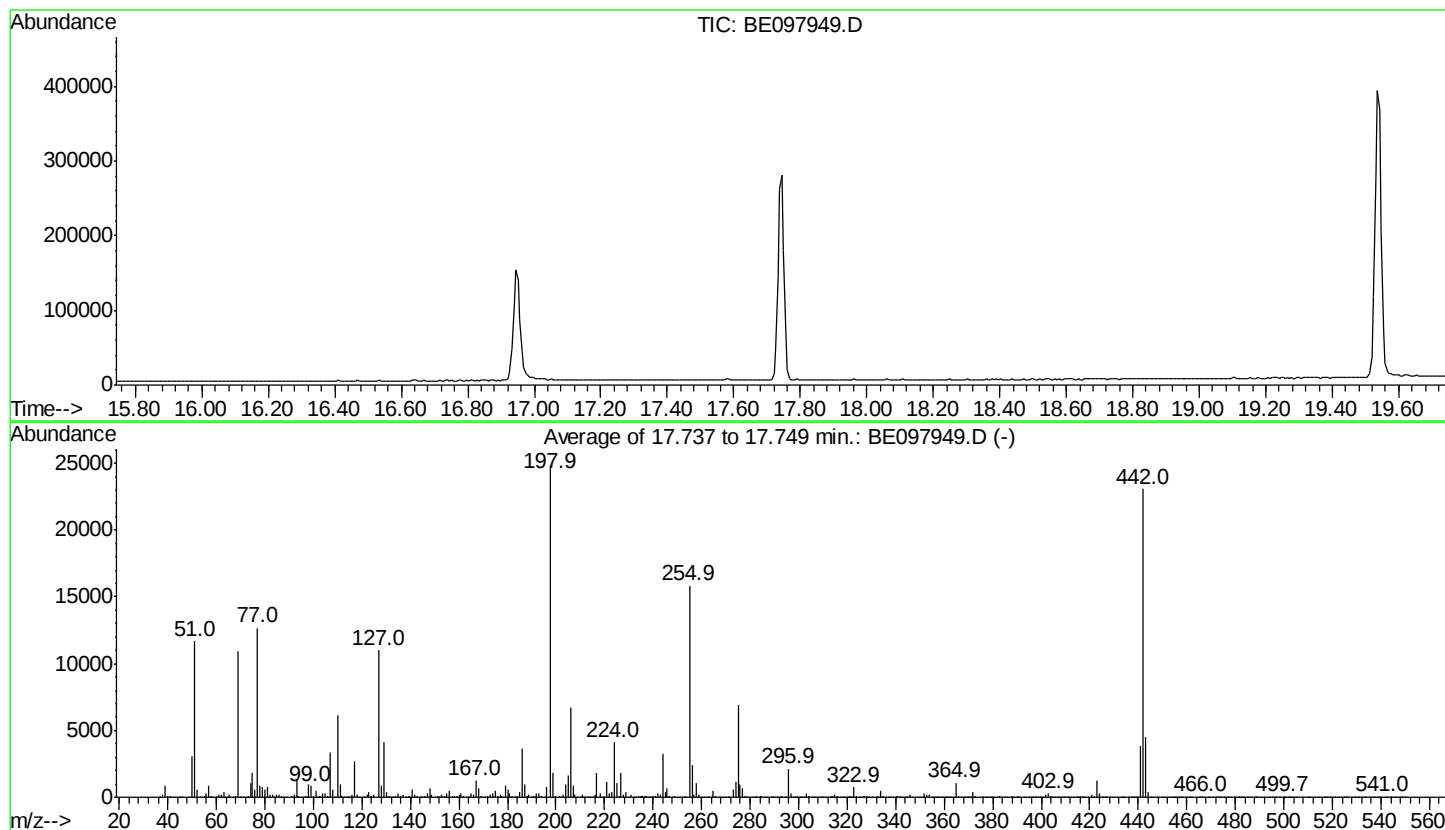

AutoFind: Scans 2578, 2579, 2580; Background Corrected with Scan 2570

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.9	11647	PASS
68	69	0.00	2	0.7	79	PASS
69	198	0.00	100	44.0	10932	PASS
70	69	0.00	2	0.1	15	PASS
127	198	10	80	44.4	11014	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	24824	PASS
199	198	5	9	7.2	1795	PASS
275	198	10	60	27.9	6936	PASS
365	198	1	100	4.3	1057	PASS
441	198	0.01	100	15.4	3822	PASS
442	198	50	100	93.0	23074	PASS
443	442	15	24	19.7	4554	PASS