


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE101818\
 Data File : BE097967.D
 Acq On : 18 Oct 2018 8:42
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE101618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 16 15:36:44 2018

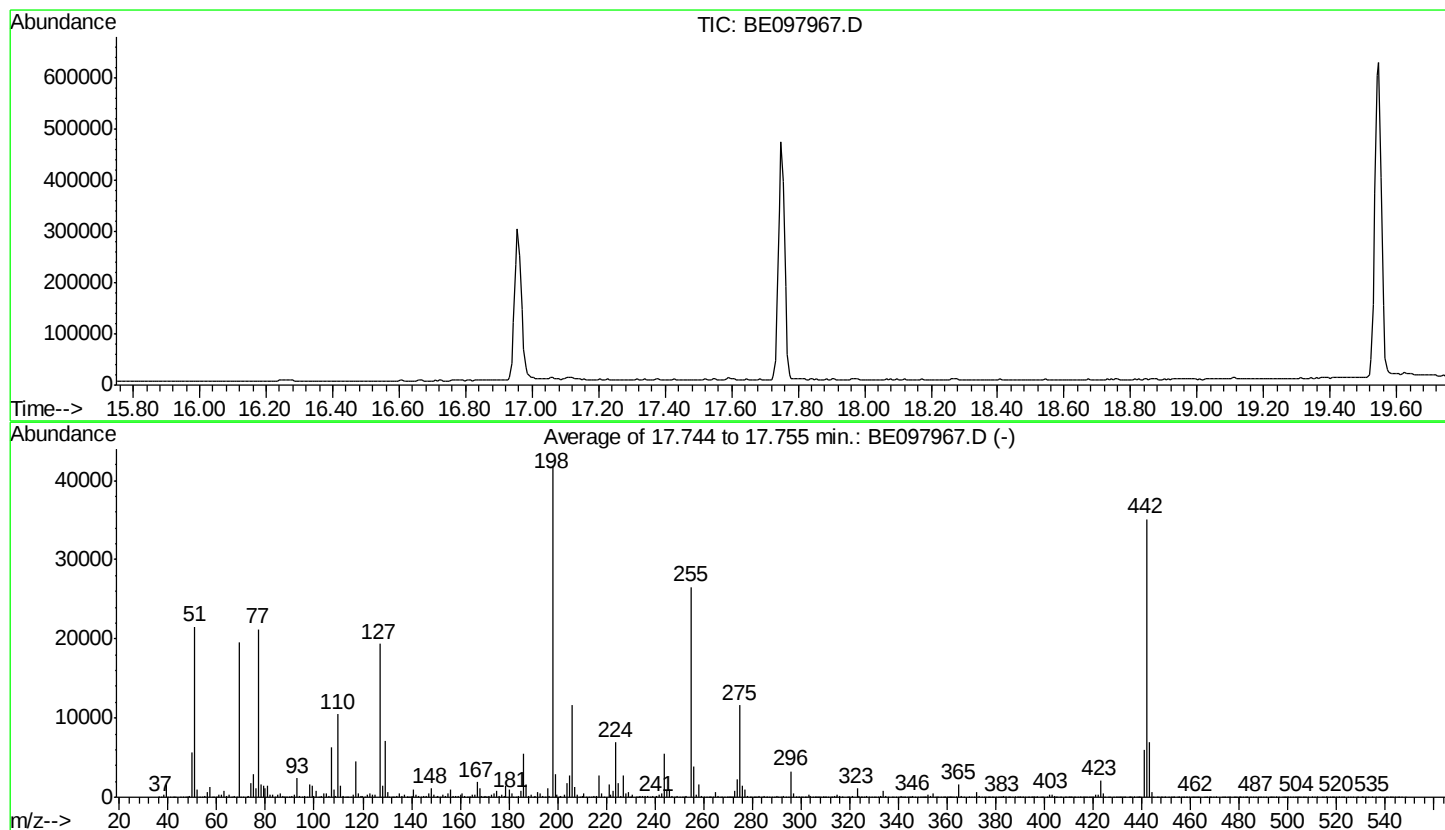

AutoFind: Scans 2579, 2580, 2581; Background Corrected with Scan 2568

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.5	21564	PASS
68	69	0.00	2	0.2	47	PASS
69	198	0.00	100	46.7	19559	PASS
70	69	0.00	2	0.3	56	PASS
127	198	10	80	46.3	19395	PASS
197	198	0.00	2	0.3	136	PASS
198	198	100	100	100.0	41870	PASS
199	198	5	9	6.9	2907	PASS
275	198	10	60	27.8	11637	PASS
365	198	1	100	3.7	1548	PASS
441	198	0.01	100	14.3	5967	PASS
442	198	50	100	83.9	35108	PASS
443	442	15	24	19.7	6907	PASS