


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE101819\
Data File : BE100652.D
Acq On : 18 Oct 2019 9:04
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE101019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 10 14:01:52 2019

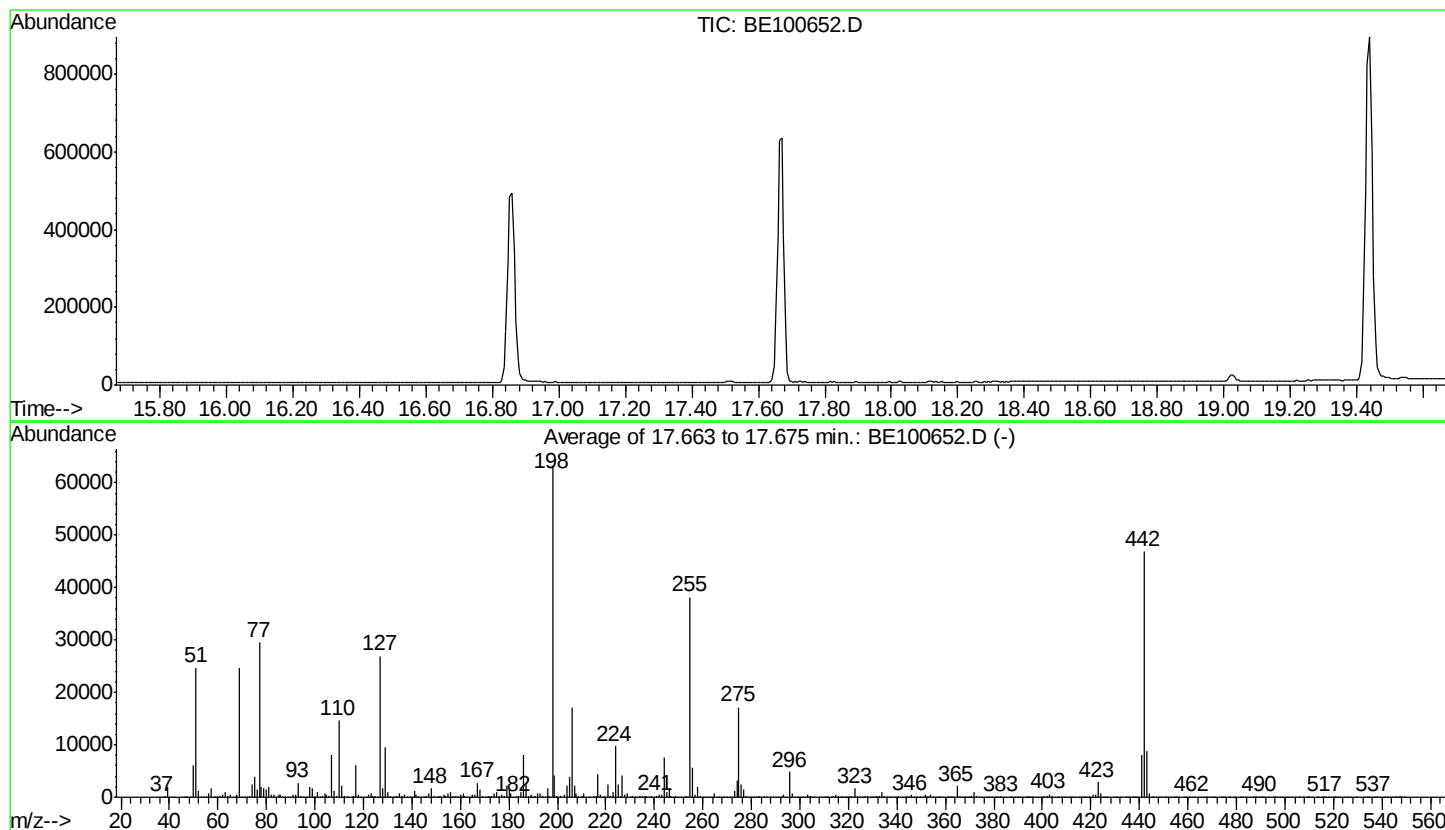

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	24795	PASS
68	69	0.00	2	1.9	474	PASS
69	198	0.00	100	38.8	24580	PASS
70	69	0.00	2	0.5	128	PASS
127	198	10	80	42.7	26985	PASS
197	198	0.00	2	0.3	212	PASS
198	198	100	100	100.0	63270	PASS
199	198	5	9	6.6	4199	PASS
275	198	10	60	27.2	17196	PASS
365	198	1	100	3.5	2199	PASS
441	198	0.01	100	12.7	8011	PASS
442	198	50	100	74.0	46838	PASS
443	442	15	24	19.0	8920	PASS