

Data File : BE098004.D
Acq On : 22 Oct 2018 11:00
Operator : SJ/JU
Sample : PB113933BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK33

Quant Time: Oct 23 01:27:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 23 01:24:18 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	2646	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	12860	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.54	164	9245	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.39	188	1255776	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.47
20) Perylene-d12	24.03	264	30156	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	7349	0.36	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.54	166	1974	0.060	ng/ul#	13
23) Benzo(a)pyrene	23.86	252	4923	0.069	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BE098004.D
Acq On : 22 Oct 2018 11:00
Operator : SJ/JU
Sample : PB113933BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK33

Quant Time: Oct 23 01:27:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 23 01:24:18 2018
Response via : Initial Calibration




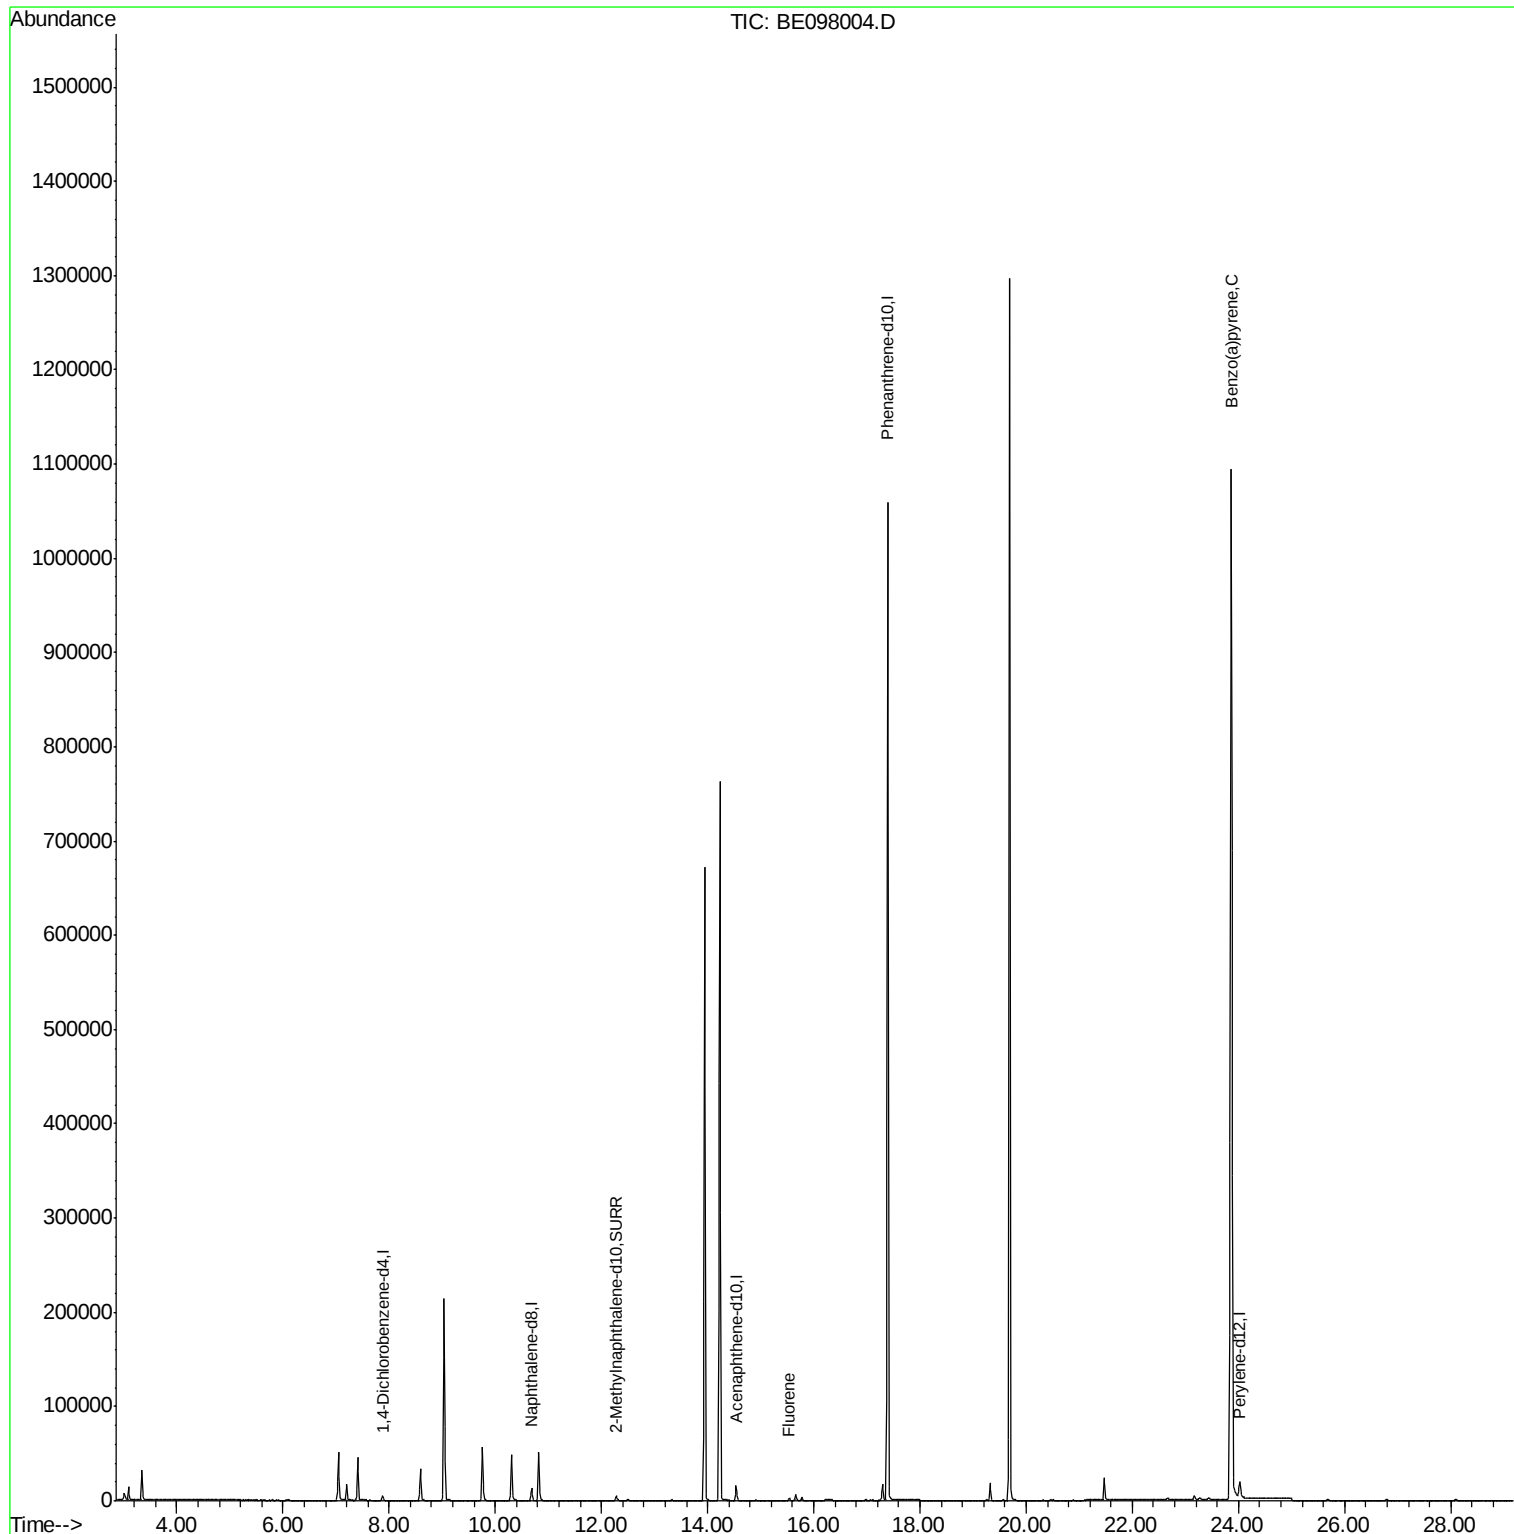


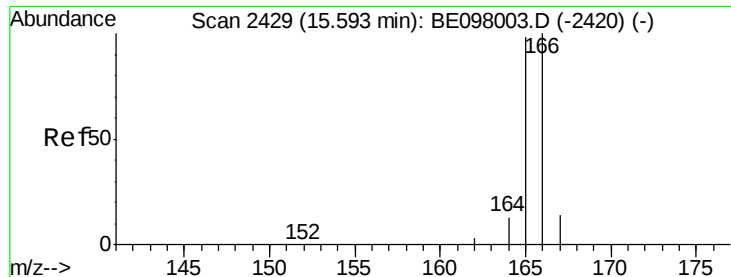

#9
Fluorene
 Concen: 0.060 ng/ul
 RT: 15.54 min Scan# 2420
 Delta R.T. -0.05 min
 Lab File: BE098004.D
 Acq: 22 Oct 2018 11:00

Instrument :
 BNA_E
 ClientSampleId :
 SBLK33

Tgt Ion:166 Resp: 1974
 Ion Ratio Lower Upper
 166 100
 165 8.4 79.2 118.8#
 167 36.7 11.3 16.9#

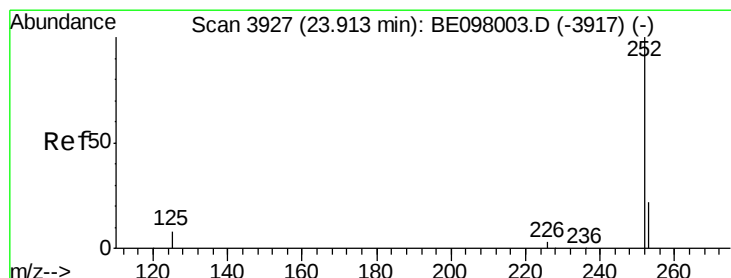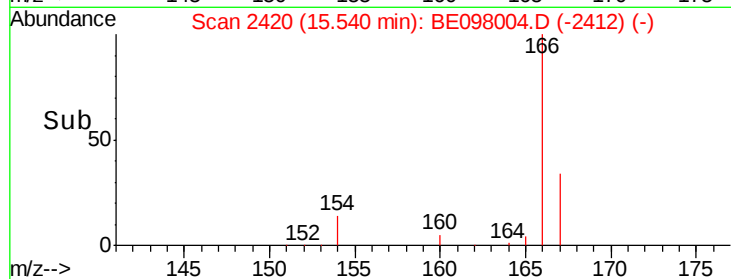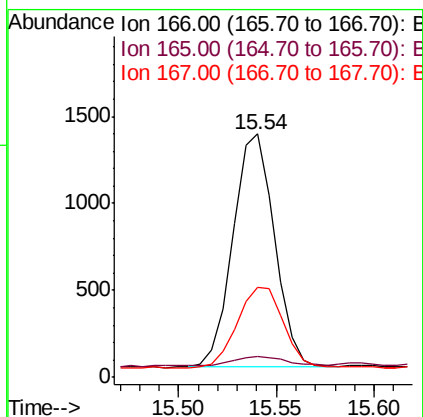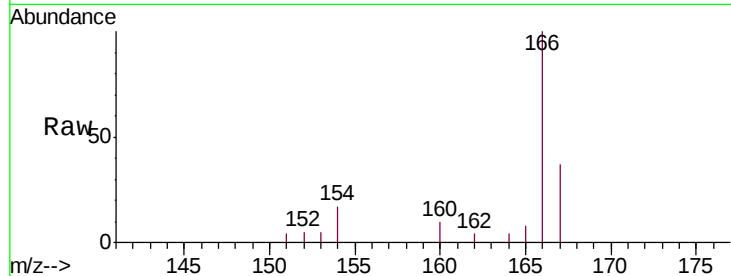

#23
Benzo(a)pyrene
 Concen: 0.069 ng/ul
 RT: 23.86 min Scan# 3920
 Delta R.T. -0.05 min
 Lab File: BE098004.D
 Acq: 22 Oct 2018 11:00

Tgt Ion:252 Resp: 4923
 Ion Ratio Lower Upper
 252 100
 253 34.1 18.2 27.4#
 125 25.2 8.3 12.5#

