

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102218\
Quantitation Report (QT Reviewed)


Data File : BE098019.D
Acq On : 22 Oct 2018 21:10
Operator : SJ/JU
Sample : J5567-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AJ1

Manual Integrations
APPROVED

Sohil
10/23/2018 5:34:41 PM

Quant Time: Oct 23 03:07:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 23 02:34:53 2018
Response via : Initial Calibration

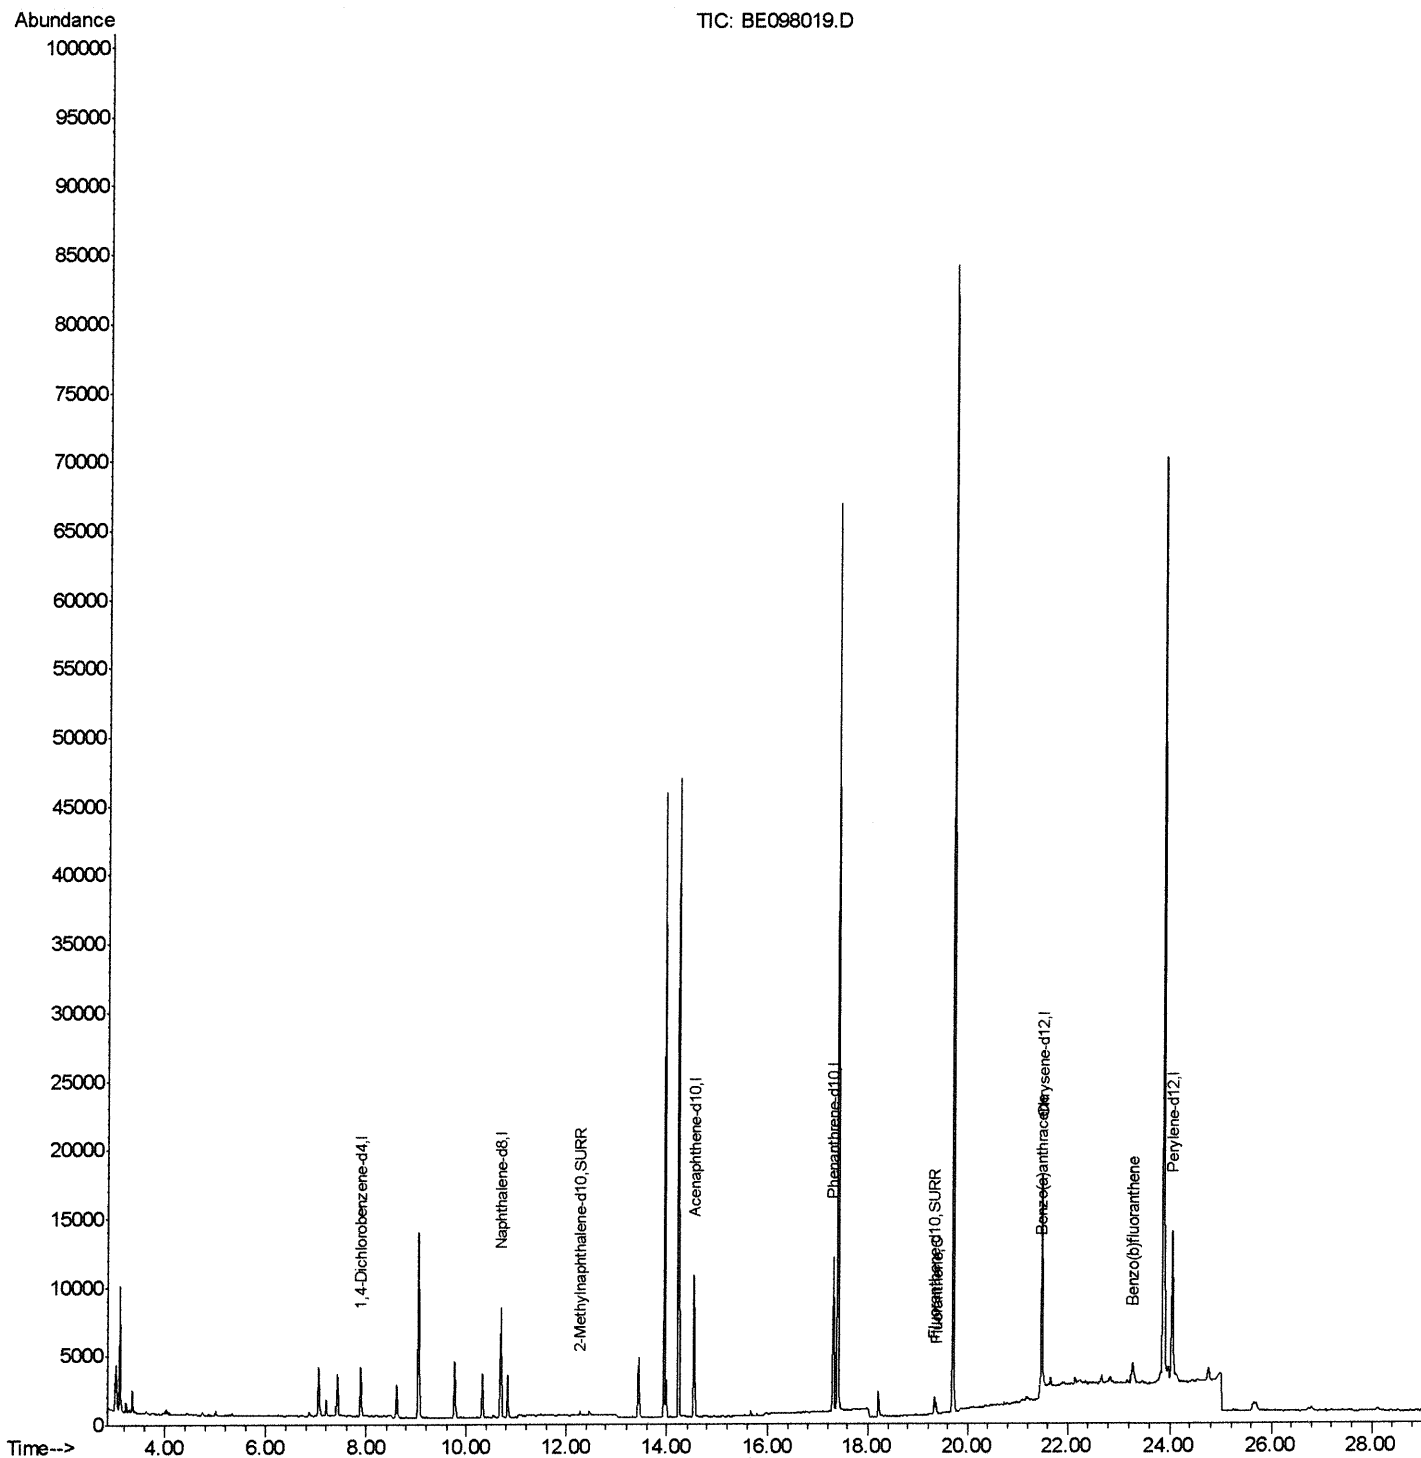

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102218\
Quantitation Report (Qedit)




Data File : BE098019.D
Acq On : 22 Oct 2018 21:10
Operator : SJ/JU
Sample : J5567-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AJ1

Manual Integrations
APPROVED

Sohil
10/23/2018 5:34:41 PM

Quant Time: Oct 23 02:38:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 23 02:34:53 2018
Response via : Initial Calibration

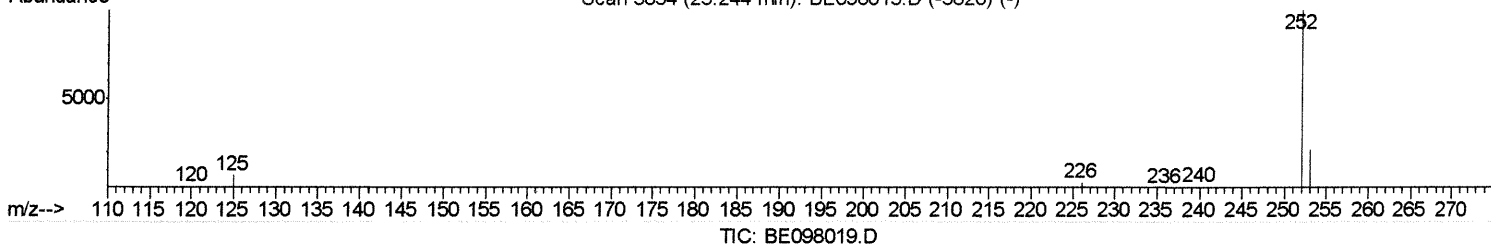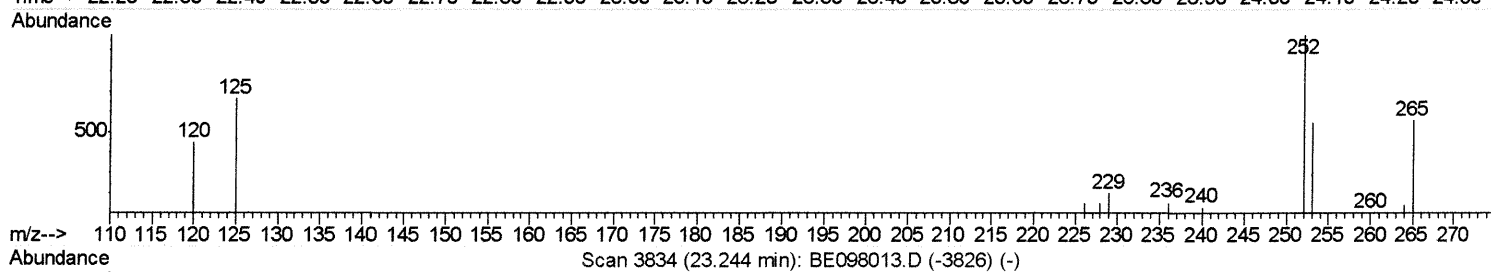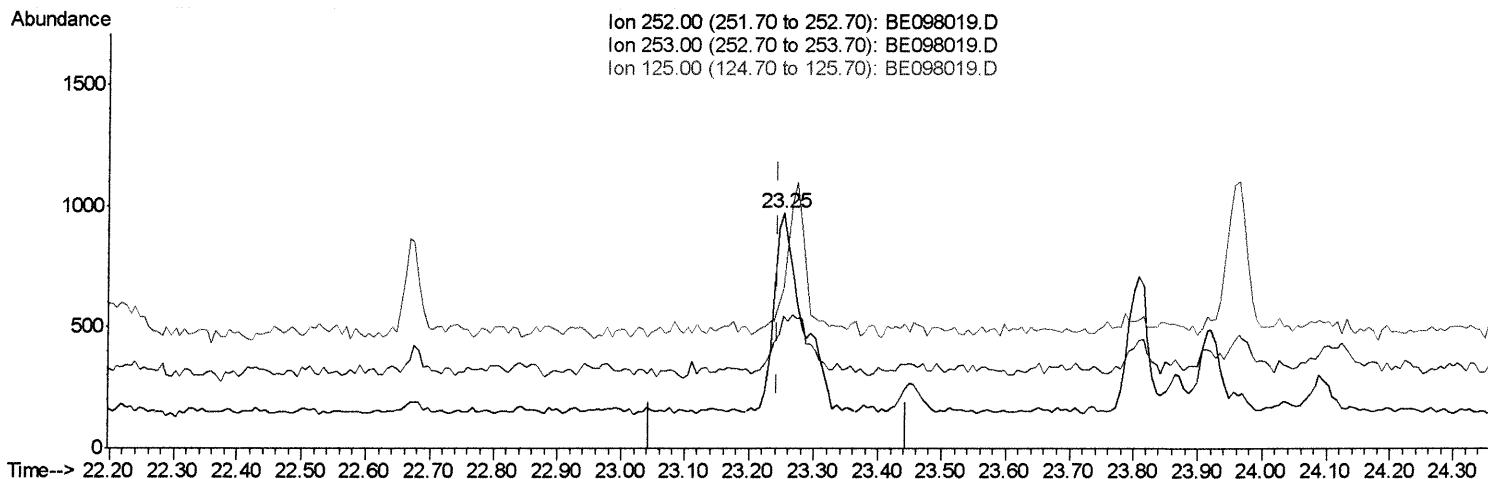

(21) Benzo(b)fluoranthene

23.251min (+0.007) 0.06ng/ul

response 2566

Ion	Exp%	Act%
252.00	100	100
253.00	23.50	56.07#
125.00	9.10	68.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102218\
Quantitation Report (Qedit)




Data File : BE098019.D
Acq On : 22 Oct 2018 21:10
Operator : SJ/JU
Sample : J5567-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AJ1

Manual Integrations
APPROVED

Sohil
10/23/2018 5:34:41 PM

Quant Time: Oct 23 02:38:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 23 02:34:53 2018
Response via : Initial Calibration

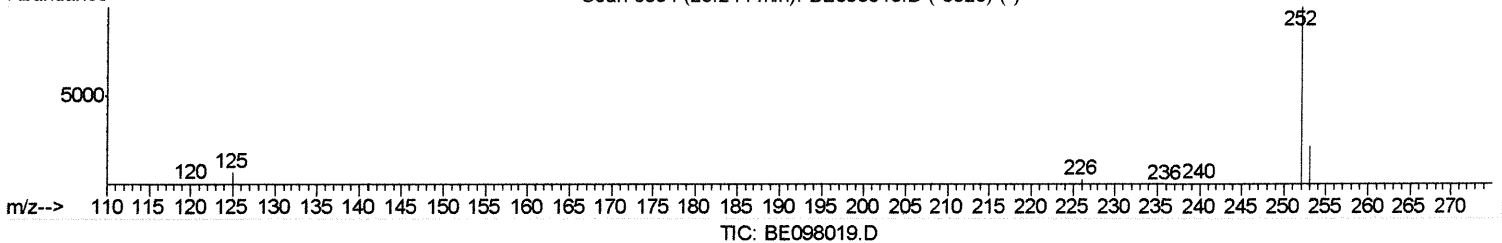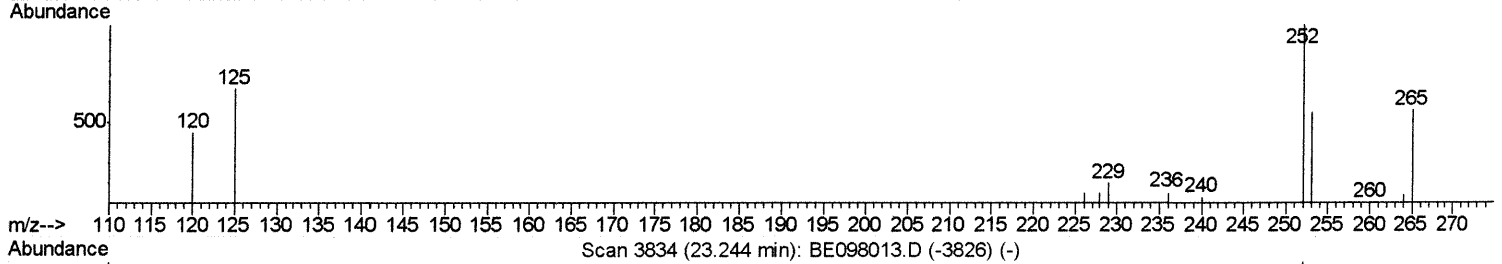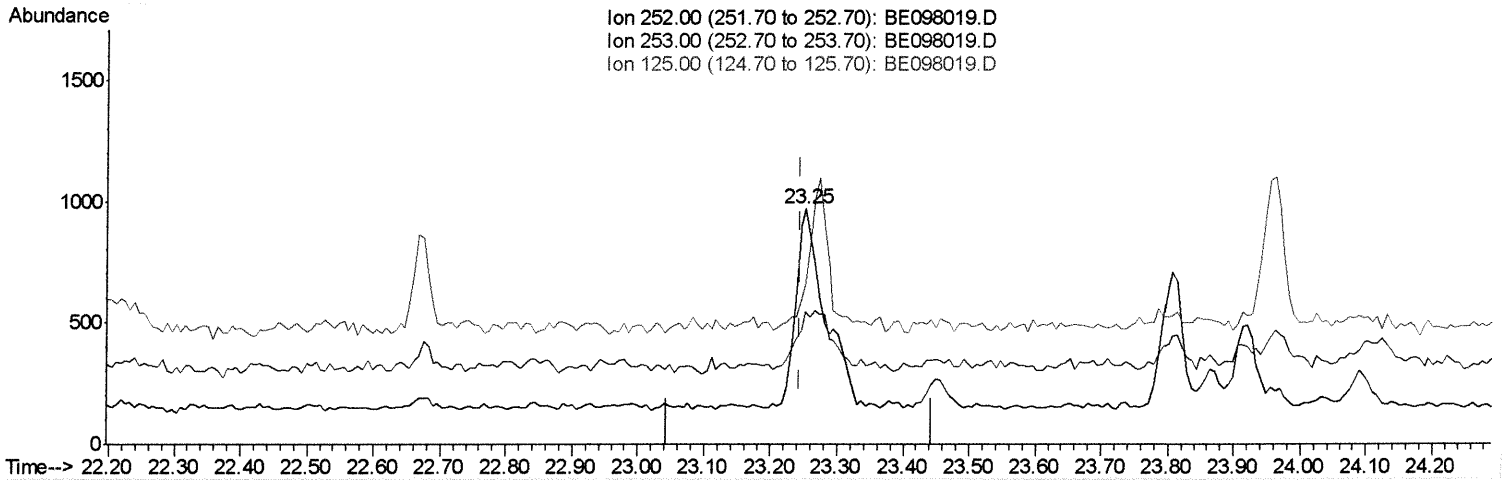

(21) Benzo(b)fluoranthene

23.251min (+0.007) 0.05ng/ul m

response 2081

Ion	Exp%	Act%
252.00	100	100
253.00	23.50	56.07#
125.00	9.10	68.00#
0.00	0.00	0.00

SJ 10/24/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102218\
Quantitation Report (QT Reviewed)

Data File : BE098019.D
Acq On : 22 Oct 2018 21:10
Operator : SJ/JU
Sample : J5567-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AJ1

Manual Integrations
APPROVED

Sohil
10/23/2018 5:34:41 PM

Quant Time: Oct 23 03:07:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 23 02:34:53 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	1747	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	8301	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.54	164	5658	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.30	188	13805	0.40	ng/ul	0.00
16) Chrysene-d12	21.48	240	15416	0.40	ng/ul	0.00
20) Perylene-d12	24.03	264	15861	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	478	0.04	ng/ul	0.00
14) Fluoranthene-d10	19.33	212	1324	0.03	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
15) Fluoranthene	19.36	202	921	0.021	ng/ul#	33
18) Benzo(a)anthracene	21.46	228	1106	0.026	ng/ul#	64
21) Benzo(b)fluoranthene	23.25	252	2081m	0.051	ng/ul	

SJ10/24/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed