

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102218\
 Data File : BE098006.D
 Acq On : 22 Oct 2018 12:35
 Operator : SJ/JU
 Sample : J5567-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AH5

Manual Integrations
 APPROVED

Sohil
 10/23/2018 5:34:06 PM

Quant Time: Oct 23 01:45:22 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 23 01:24:18 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	2442	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	12257	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.54	164	8956	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.30	188	20874m	0.40	ng/ul	0.00
16) Chrysene-d12	21.47	240	22473m	0.40	ng/ul	0.00
20) Perylene-d12	24.03	264	20358m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	6292	0.33	ng/ul	0.01
14) Fluoranthene-d10	19.32	212	18040m	0.27	ng/ul	0.00
Target Compounds						
21) Benzo(b)fluoranthene	23.25	252	2196m	0.042	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102218\
Data File : BE098006.D
Acq On : 22 Oct 2018 12:35
Operator : SJ/JU
Sample : J5567-07
Misc :
ALS Vial : 5 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
C0AH5

Quant Time: Oct 23 01:45:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 23 01:24:18 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
10/23/2018 5:34:06 PM

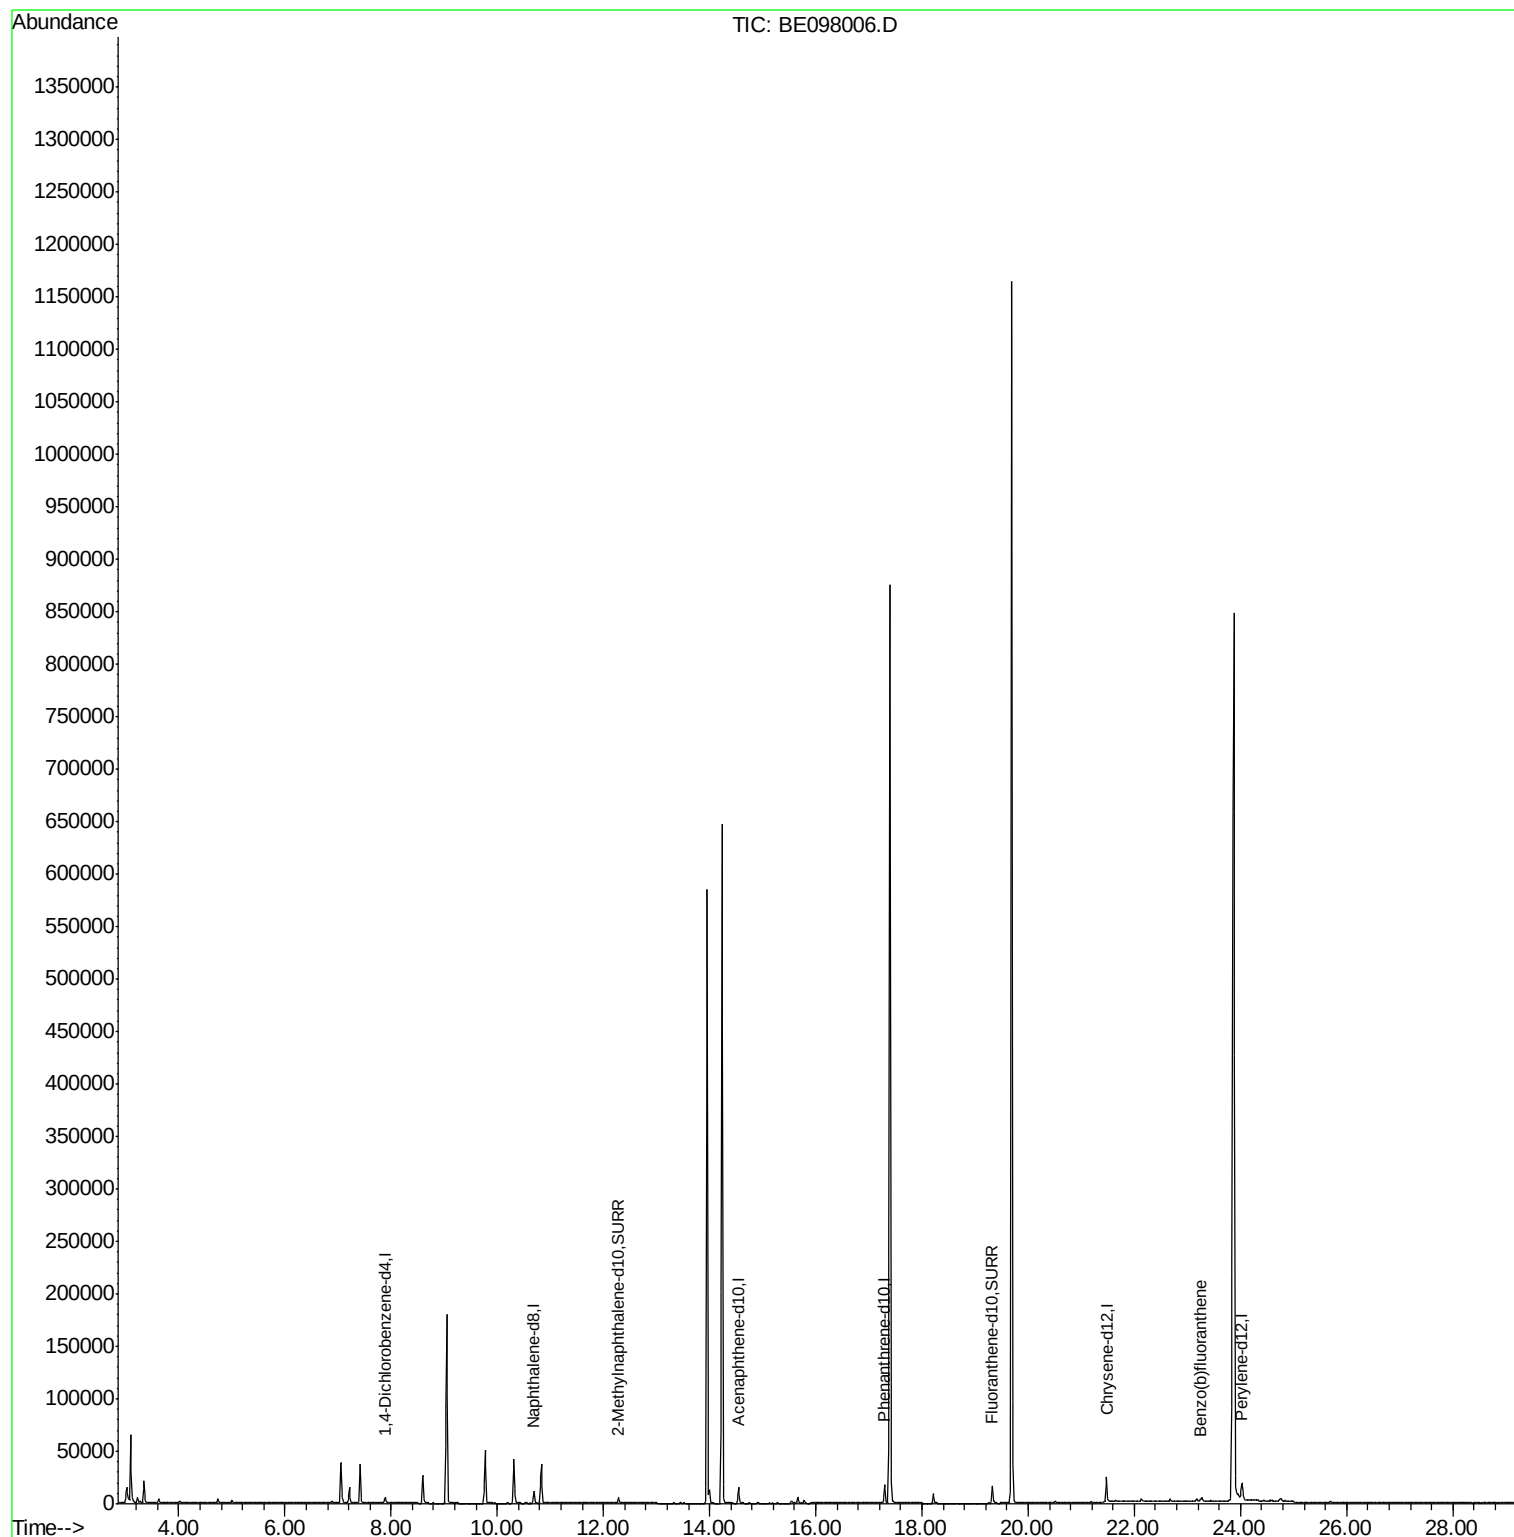

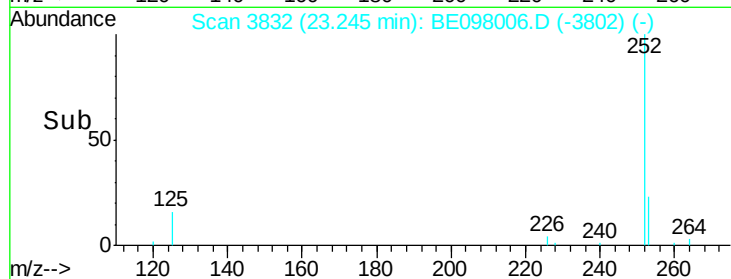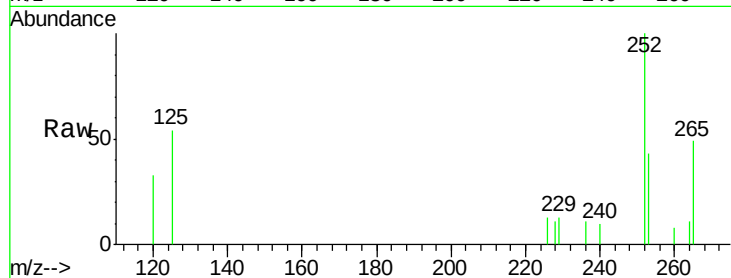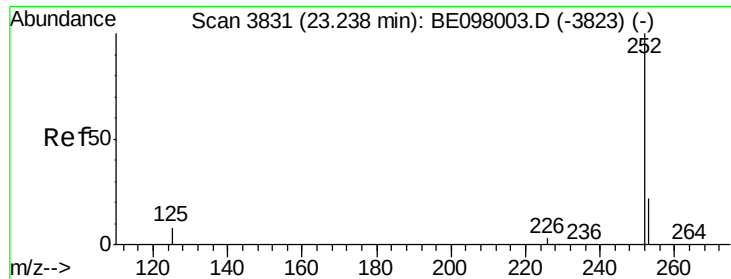

#21

Benzo(b)fluoranthene

Concen: 0.042 ng/ul m

RT: 23.25 min Scan# 3832

Delta R.T. 0.01 min

Lab File: BE098006.D

Acq: 22 Oct 2018 12:35

Instrument :

BNA_E

ClientSampleId :

C0AH5

Tgt Ion	Ratio	Lower	Upper
252	100		
253	43.2	0.0	47.0
125	53.8	0.0	18.2#

Manual Integrations
APPROVED

Sohil
10/23/2018 5:34:06 PM

