

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102218\
 Data File : BE098010.D
 Acq On : 22 Oct 2018 15:01
 Operator : SJ/JU
 Sample : J5567-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AE8

Manual Integrations
 APPROVED

Sohil
 10/23/2018 5:34:17 PM

Quant Time: Oct 23 02:14:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 23 01:24:18 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	2280	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	9662	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.54	164	7054	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.30	188	15573m	0.40	ng/ul	0.00
16) Chrysene-d12	21.47	240	16838m	0.40	ng/ul	0.00
20) Perylene-d12	24.03	264	15207m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	5911	0.39	ng/ul	0.00
14) Fluoranthene-d10	19.32	212	16090m	0.32	ng/ul	0.00
Target Compounds						
21) Benzo(b)fluoranthene	23.25	252	2047m	0.052	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102218\
Data File : BE098010.D
Acq On : 22 Oct 2018 15:01
Operator : SJ/JU
Sample : J5567-01
Misc :
ALS Vial : 9 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
C0AE8

Quant Time: Oct 23 02:14:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 23 01:24:18 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
10/23/2018 5:34:17 PM

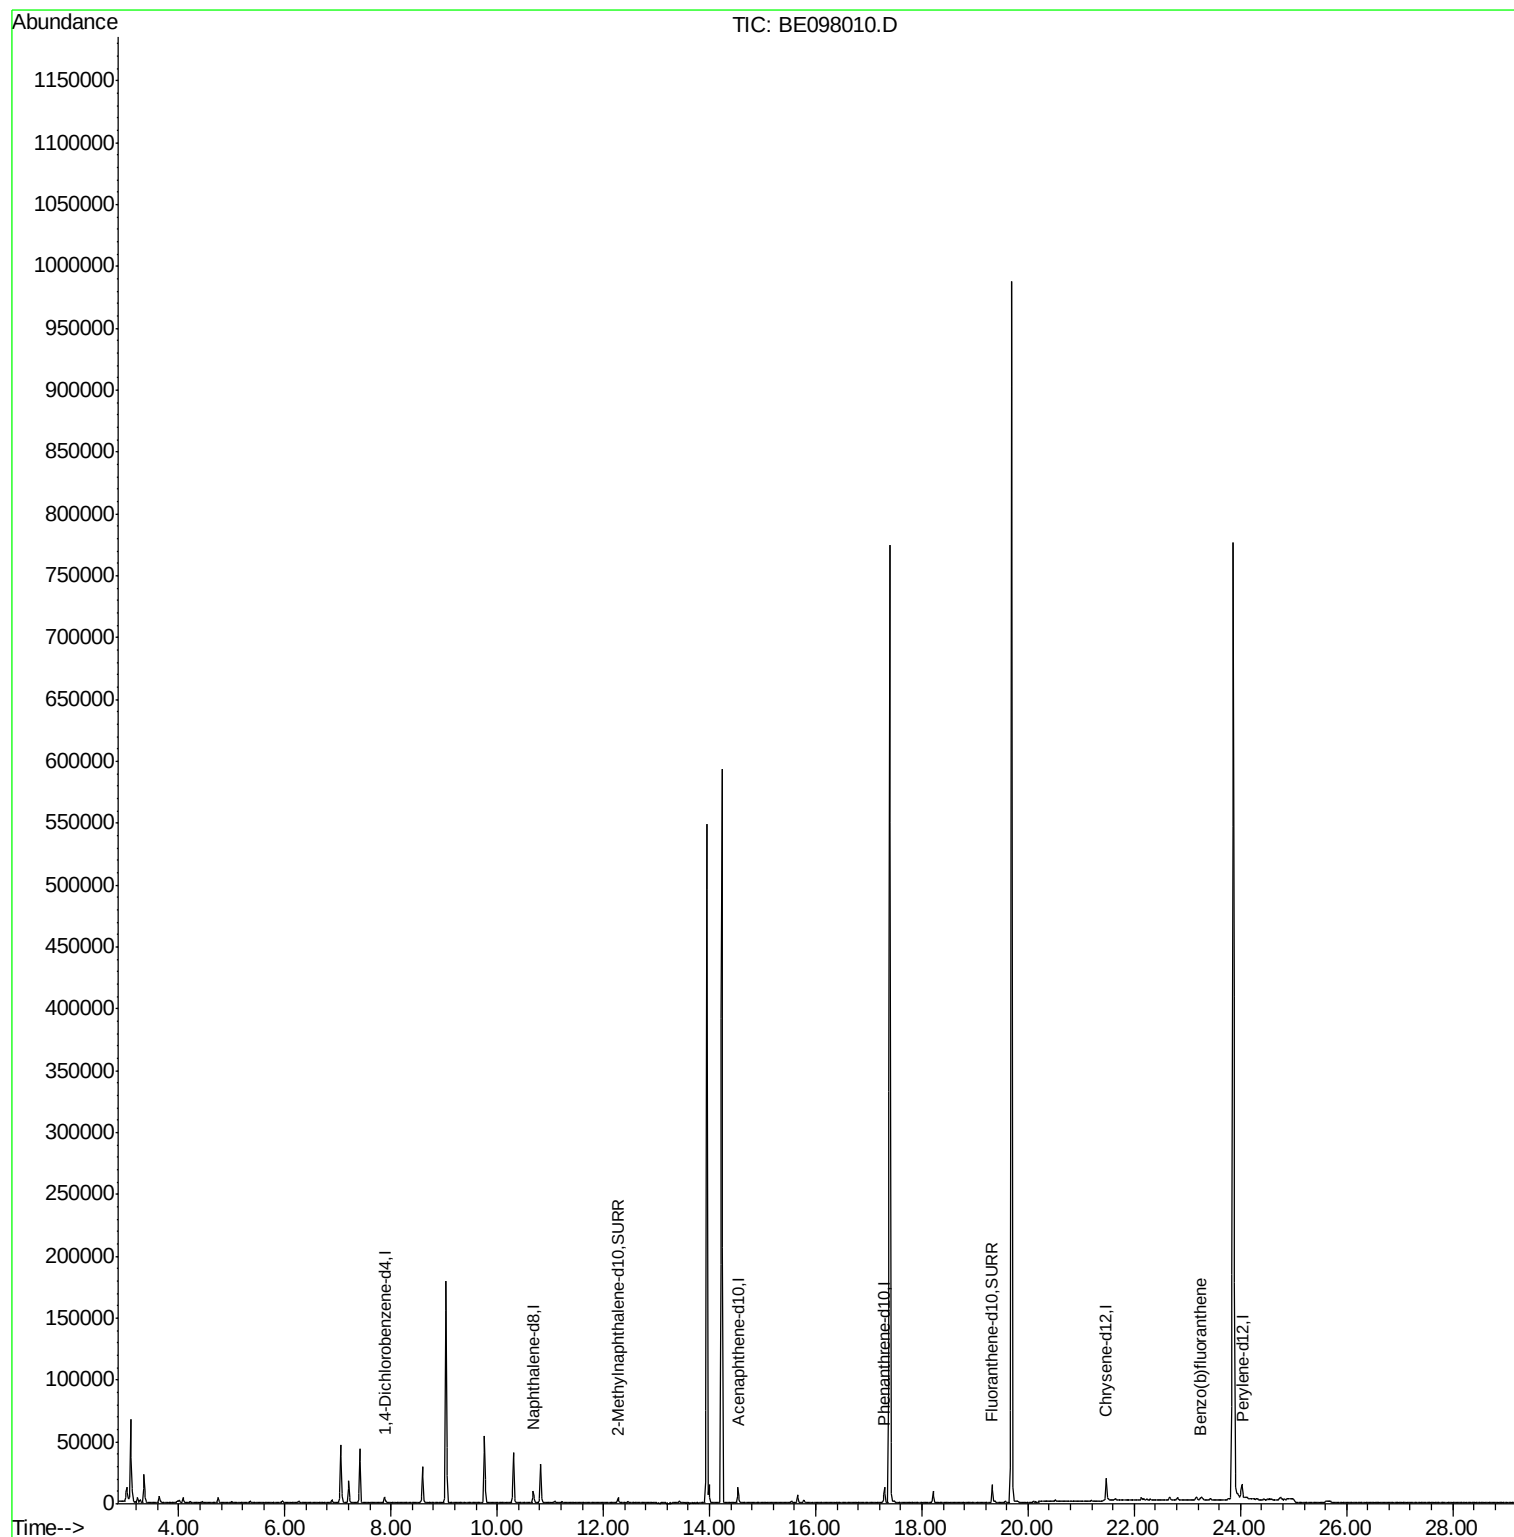

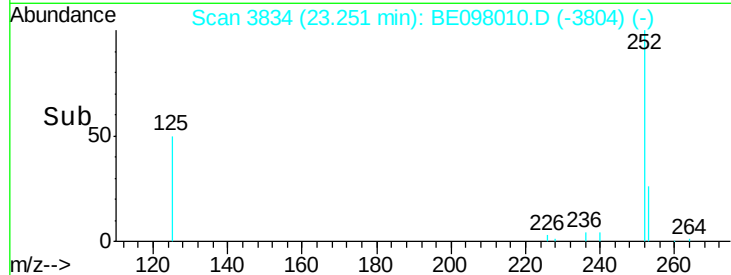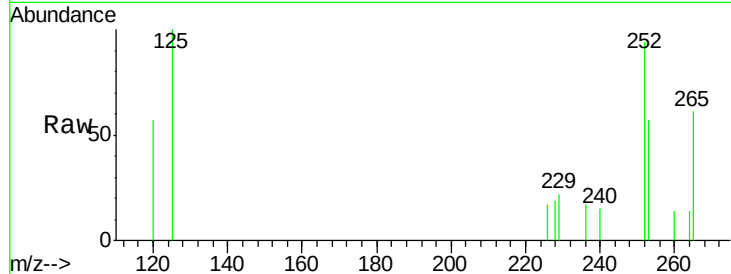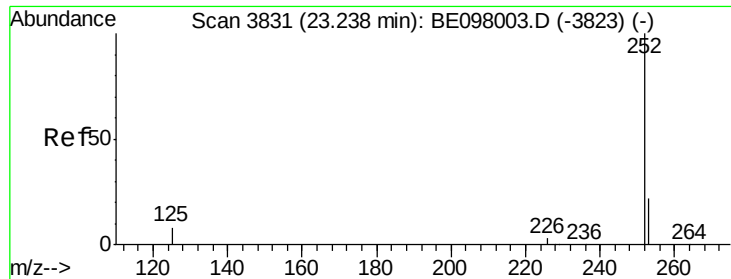

#21

Benzo(b)fluoranthene

Concen: 0.052 ng/ul m

RT: 23.25 min Scan# 3834

Delta R.T. 0.01 min

Lab File: BE098010.D

Acq: 22 Oct 2018 15:01

Instrument :

BNA_E

ClientSampleId :

C0AE8

Tgt Ion	Ratio	Lower	Upper
252	100		
253	60.9	0.0	47.0#
125	106.4	0.0	18.2#

Manual Integrations
APPROVED

Sohil
10/23/2018 5:34:17 PM

