

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102218\
 Data File : BE098027.D
 Acq On : 23 Oct 2018 2:05
 Operator : SJ/JU
 Sample : J5598-17
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AE9

Manual Integrations
 APPROVED

Sohil
 10/23/2018 5:35:06 PM

Quant Time: Oct 23 04:24:22 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 23 02:34:53 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	1476	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	7408	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.54	164	5682	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.30	188	12429m	0.40	ng/ul	0.00
16) Chrysene-d12	21.48	240	13848m	0.40	ng/ul	0.00
20) Perylene-d12	24.03	264	12811m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	5047	0.43	ng/ul	0.00
14) Fluoranthene-d10	19.33	212	14739m	0.36	ng/ul	0.00
Target Compounds						
8) Acenaphthene	14.62	153	2286	0.137	ng/ul#	25

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102218\
Data File : BE098027.D
Acq On : 23 Oct 2018 2:05
Operator : SJ/JU
Sample : J5598-17
Misc :
ALS Vial : 25 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
C0AE9

Quant Time: Oct 23 04:24:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 23 02:34:53 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
10/23/2018 5:35:06 PM

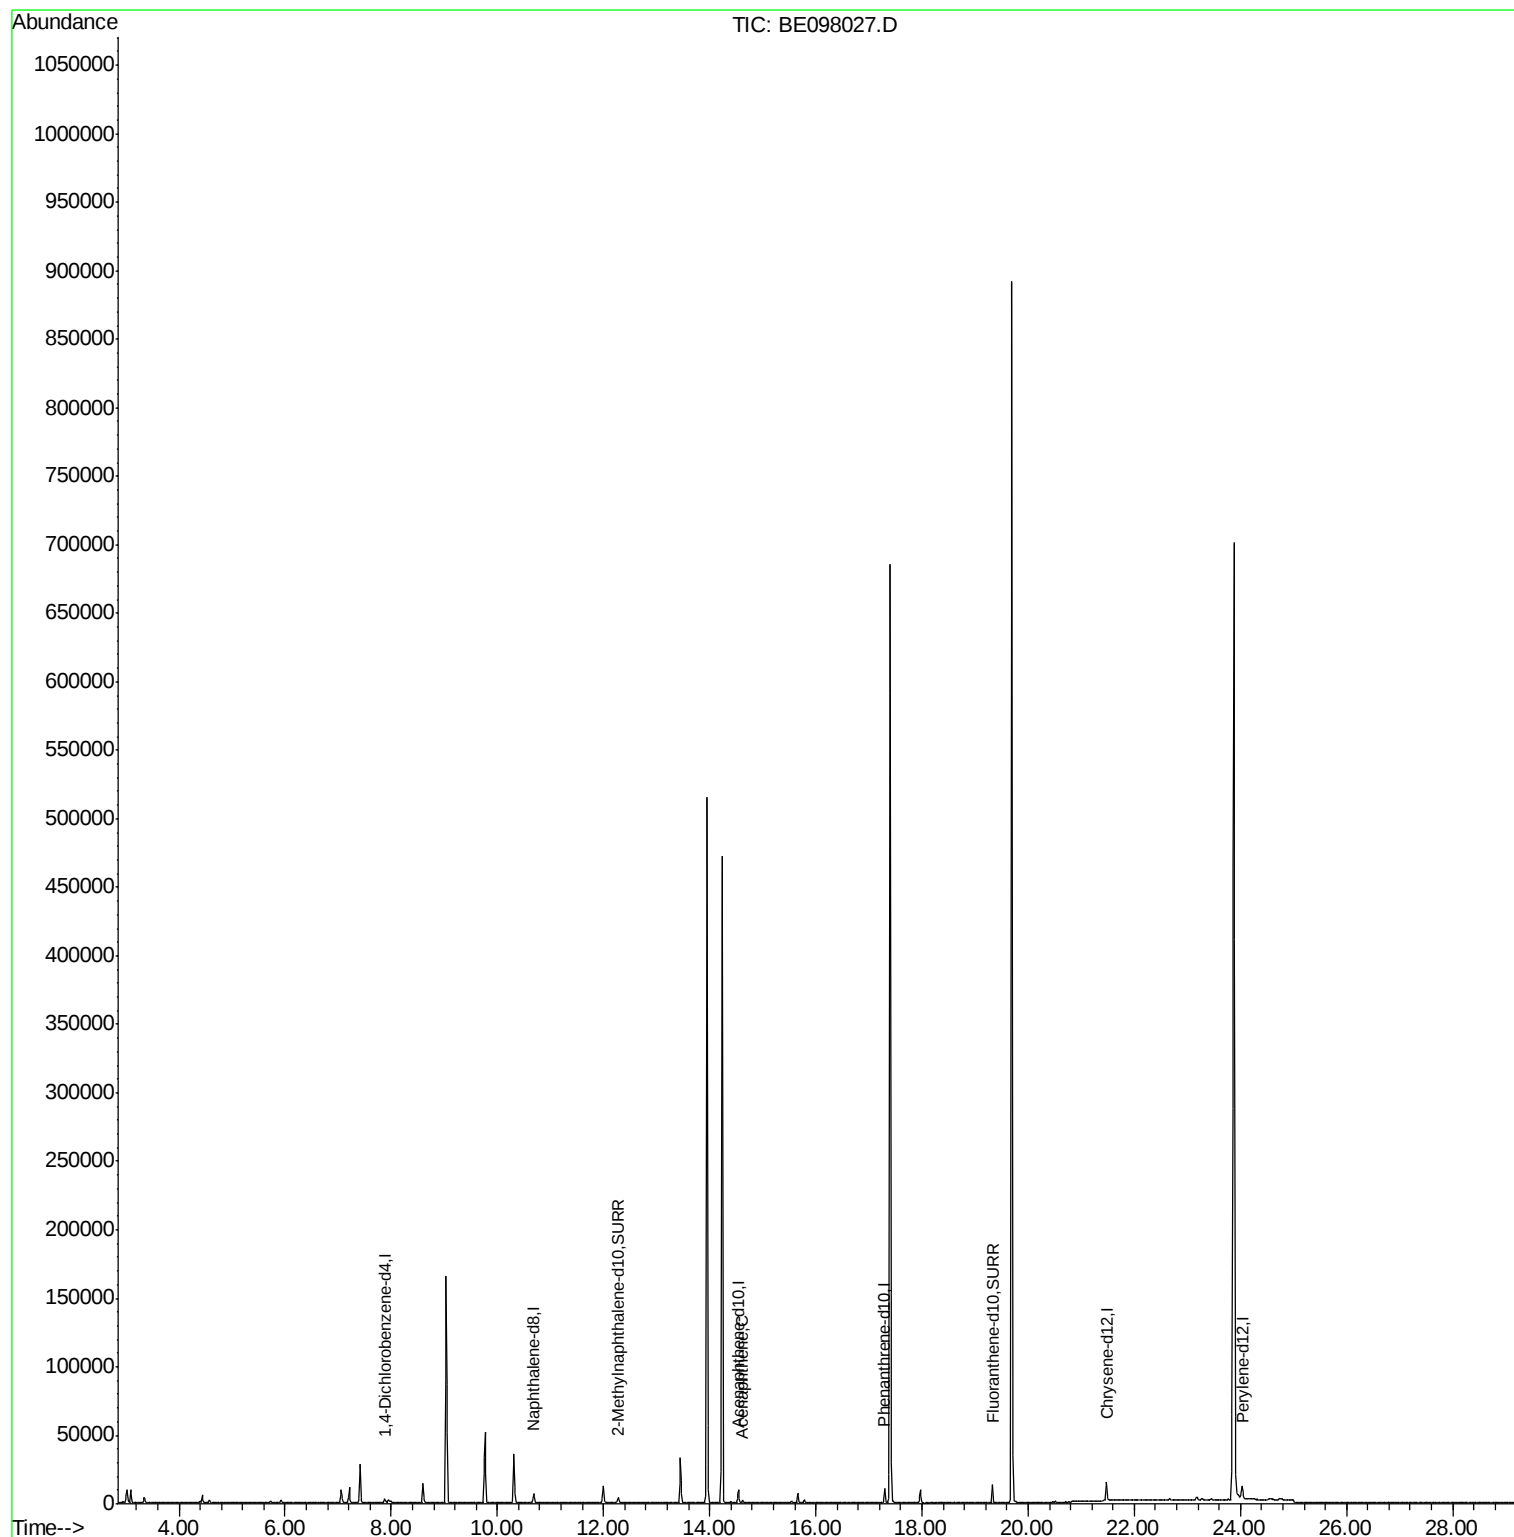

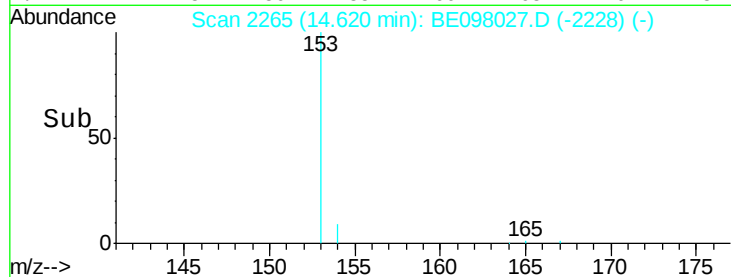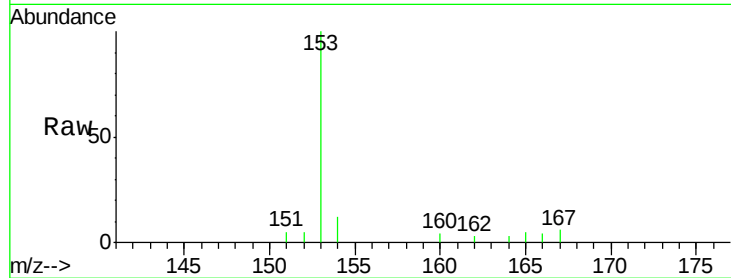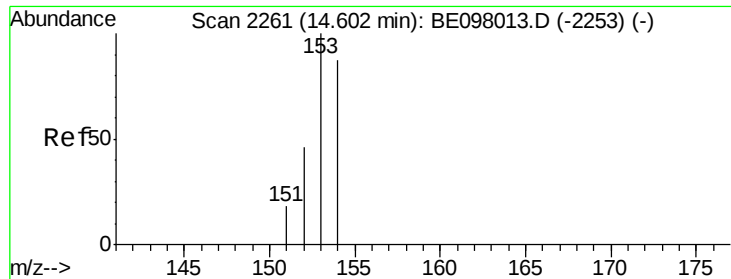

#8

Acenaphthene

Concen: 0.137 ng/ul

RT: 14.62 min Scan# 2265

Delta R.T. 0.02 min

Lab File: BE098027.D

Acq: 23 Oct 2018 2:05

Instrument :

BNA_E

ClientSampleId :

C0AE9

Tgt Ion:153 Resp: 2286

Ion Ratio Lower Upper

153 100

152 5.0 41.2 61.8#

154 12.3 68.6 103.0#

Manual Integrations
APPROVED

Sohil
10/23/2018 5:35:06 PM

