

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE102319\  
 Data File : BE100673.D  
 Acq On : 23 Oct 2019 22:09  
 Operator : JU  
 Sample : SSTDCCC0.4  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampled :

Quant Time: Oct 24 01:34:51 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE101019.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Oct 23 16:49:33 2019  
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	3764	0.40	ng	0.00
7) Naphthalene-d8	10.63	136	15626	0.40	ng	0.00
13) Acenaphthene-d10	14.47	164	10166	0.40	ng	0.00
19) Phenanthrene-d10	17.19	188	24687	0.40	ng	-0.01
27) Chrysene-d12	21.35	240	34862	0.40	ng	0.00
34) Perylene-d12	23.83	264	42093	0.40	ng	0.00

## System Monitoring Compounds

4) 2-Fluorophenol	5.44	112	4653	0.40	ng	0.00
5) Phenol-d6	7.01	99	6670	0.41	ng	0.00
8) Nitrobenzene-d5	8.99	82	5116	0.53	ng	0.00
11) 2-Methylnaphthalene-d10	12.22	152	9270	0.38	ng	0.00
14) 2,4,6-Tribromophenol	15.94	330	1419	0.53	ng	0.00
15) 2-Fluorobiphenyl	13.10	172	15293	0.41	ng	0.00
25) Fluoranthene-d10	19.22	212	119688	0.38	ng	0.00
29) Terphenyl-d14	19.82	244	31468	0.41	ng	0.00

## Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.38	88	2348	0.350	ng	91
3) n-Nitrosodimethylamine	3.69	42	2364	0.333	ng	89
6) bis(2-Chloroethyl)ether	7.27	93	4866	0.362	ng	97
9) Naphthalene	10.68	128	62079	0.378	ng	99
10) Hexachlorobutadiene	10.98	225	2770	0.388	ng	98
12) 2-Methylnaphthalene	12.30	142	10391	0.371	ng	99
16) Acenaphthylene	14.18	152	15727	0.360	ng	99
17) Acenaphthene	14.53	154	10341	0.366	ng	99
18) Fluorene	15.50	166	13750	0.366	ng	100
20) 4-Bromophenyl-phenylether	16.40	248	4587	0.365	ng	93
21) Hexachlorobenzene	16.51	284	4483	0.375	ng	100
22) Pentachlorophenol	16.85	266	1916	0.497	ng	97
23) Phenanthrene	17.23	178	26201	0.386	ng	100
24) Anthracene	17.32	178	21534	0.342	ng	99
26) Fluoranthene	19.25	202	35065	0.396	ng	99
28) Pyrene	19.61	202	37011	0.380	ng	100
30) Benzo(a)anthracene	21.34	228	41189	0.362	ng	100
31) Chrysene	21.39	228	43420	0.382	ng	99
32) Bis(2-ethylhexyl)phthalate	21.28	149	85957	0.361	ng	100
33) Indeno(1,2,3-cd)pyrene	26.43	276	50305	0.360	ng	99
35) Benzo(b)fluoranthene	23.07	252	43452	0.354	ng	99
36) Benzo(k)fluoranthene	23.12	252	45995	0.364	ng	100
37) Benzo(a)pyrene	23.71	252	40064	0.351	ng	99
38) Dibenzo(a,h)anthracene	26.46	278	41302	0.350	ng	100
39) Benzo(g,h,i)perylene	27.23	276	42510	0.358	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE102319\  
 Data File : BE100673.D  
 Acq On : 23 Oct 2019 22:09  
 Operator : JU  
 Sample : SSTDCCC0.4  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :

Quant Time: Oct 24 01:34:51 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE101019.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Oct 23 16:49:33 2019  
 Response via : Initial Calibration




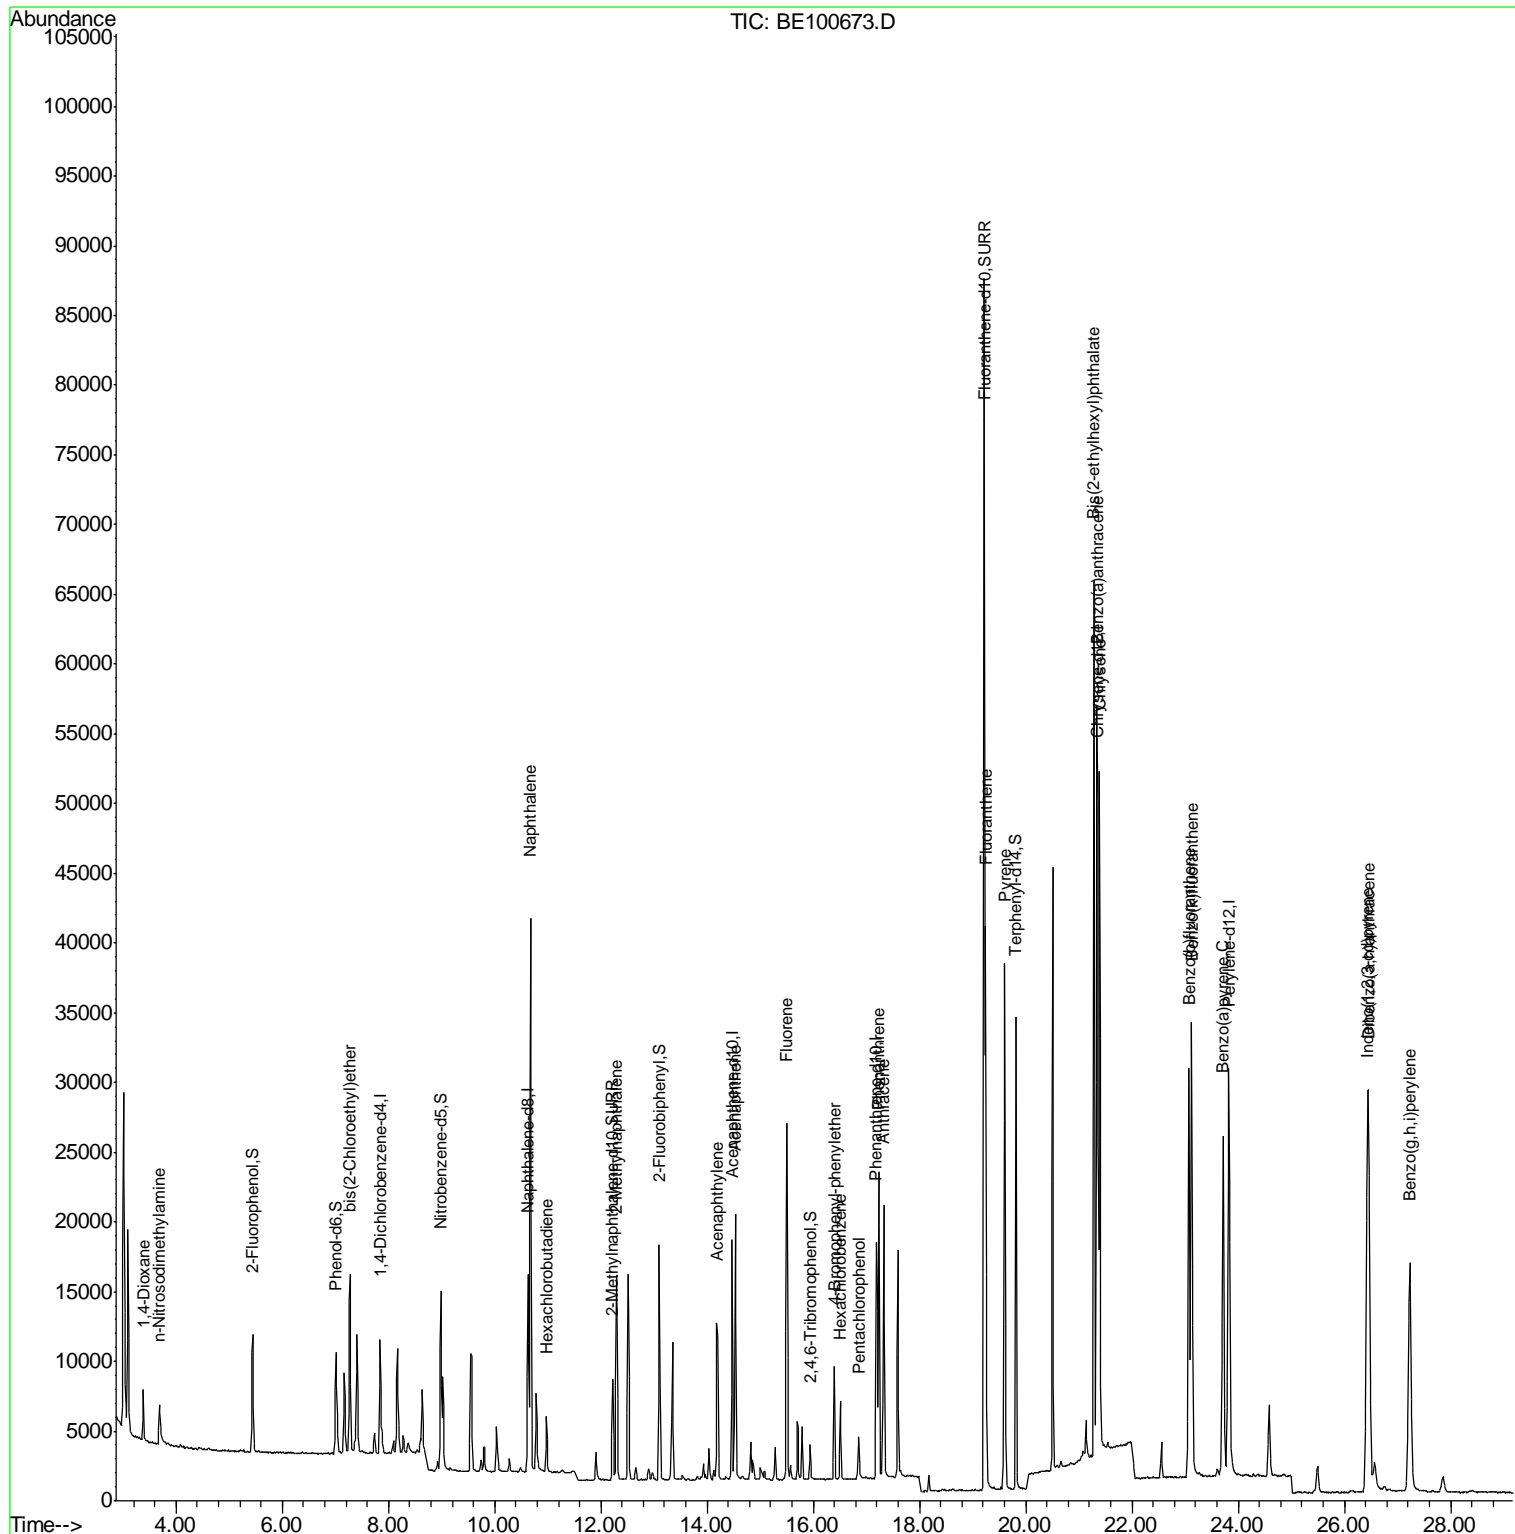




#1  
 1,4-Dichlorobenzene-d4  
 Concen: 0.400 ng  
 RT: 7.85 min Scan# 433  
 Delta R.T. -0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09




Instrument :  
 BNA\_E  
 ClientSampled :


Tgt Ion	Resp	Lower	Upper
152	3764		
152	100		
150	151.5	123.3	184.9
115	63.3	51.9	77.9

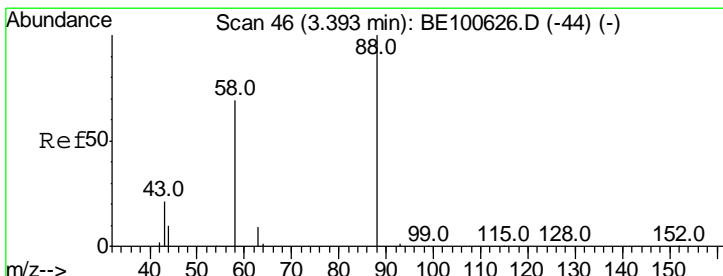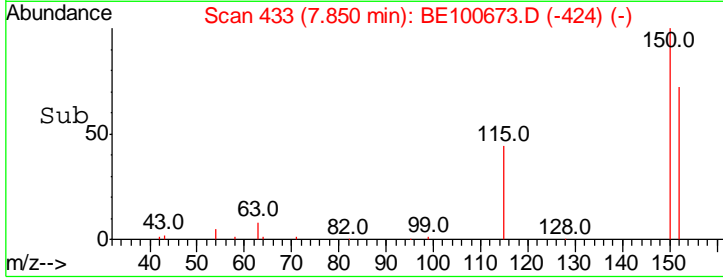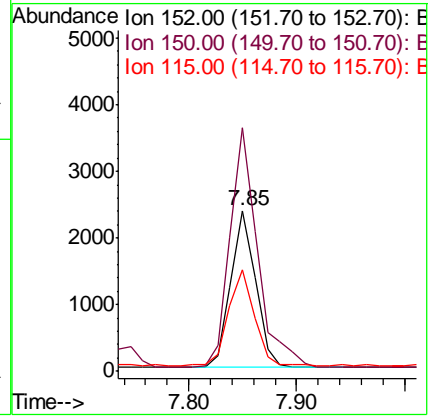

#2  
 1,4-Dioxane  
 Concen: 0.350 ng  
 RT: 3.38 min Scan# 45  
 Delta R.T. -0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Tgt Ion	Resp	Lower	Upper
88	2348		
88	100		
58	83.4	59.8	89.6
43	33.4	24.6	36.8


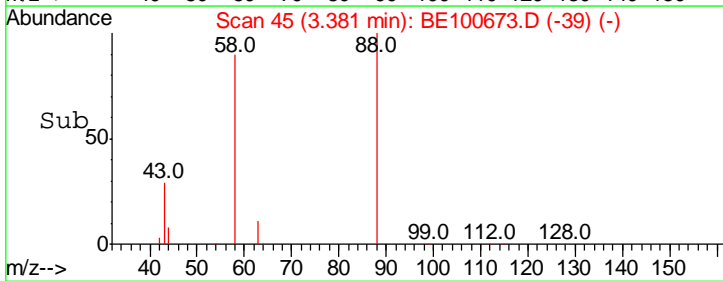
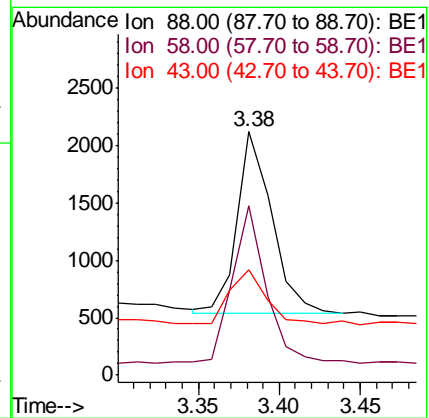
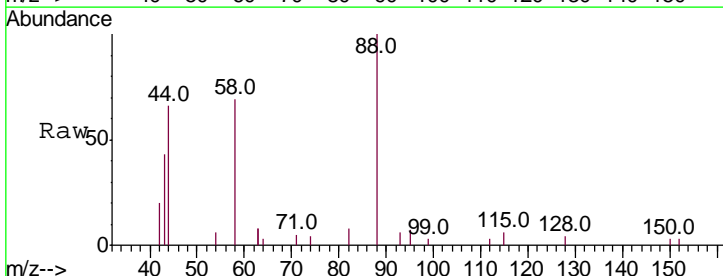




#3  
 n-Nitrosodimethylamine  
 Concen: 0.333 ng  
 RT: 3.69 min Scan# 72  
 Delta R.T. -0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09




Instrument :  
 BNA\_E  
 ClientSampled :


Tgt Ion	Resp	Lower	Upper
42	100		
74	134.1	97.2	145.8
44	17.3	16.6	24.8

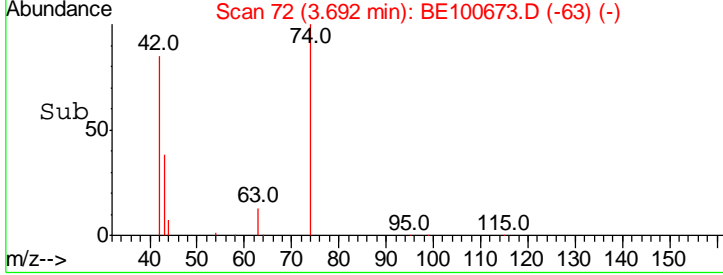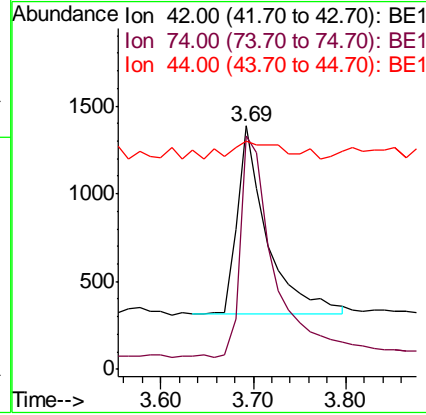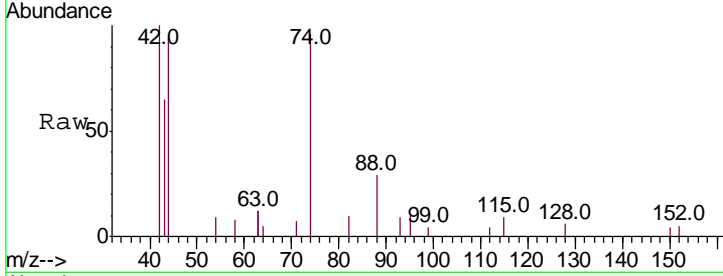

#4  
 2-Fluorophenol  
 Concen: 0.400 ng  
 RT: 5.44 min Scan# 224  
 Delta R.T. -0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Tgt Ion	Resp	Lower	Upper
112	100		
64	71.5	55.4	83.2
63	142.0	114.2	171.4


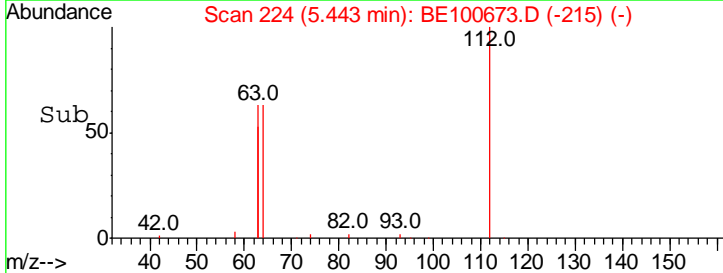
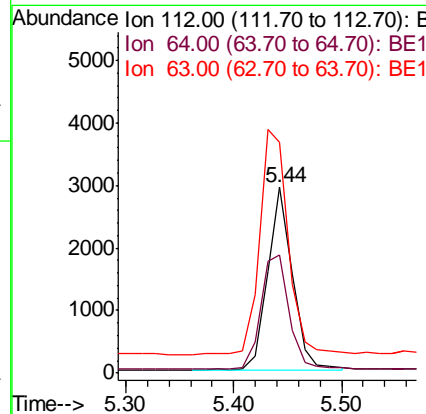
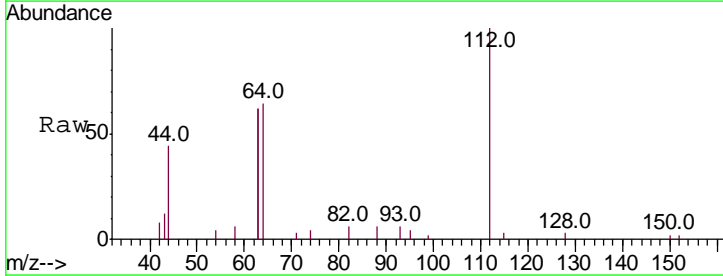




#5  
 Phenol-d6  
 Concen: 0.407 ng  
 RT: 7.01 min Scan# 360  
 Delta R.T. -0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09




Instrument :  
 BNA\_E  
 ClientSampled :


Tgt Ion	Resp	Lower	Upper
99	6670		
99	100		
42	22.3	17.7	26.5
71	34.0	27.4	41.0

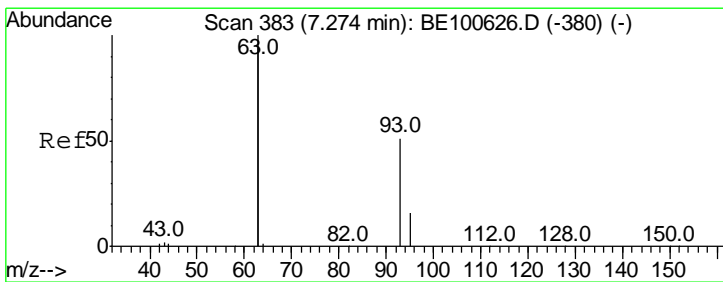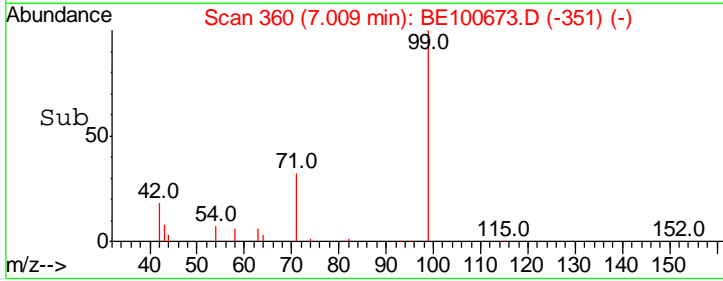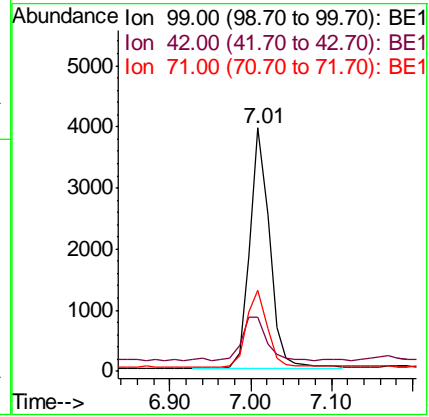

#6  
 bis(2-Chloroethyl)ether  
 Concen: 0.362 ng  
 RT: 7.27 min Scan# 383  
 Delta R.T. -0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Tgt Ion	Resp	Lower	Upper
93	4866		
93	100		
63	341.7	268.8	403.2
95	31.5	25.6	38.4

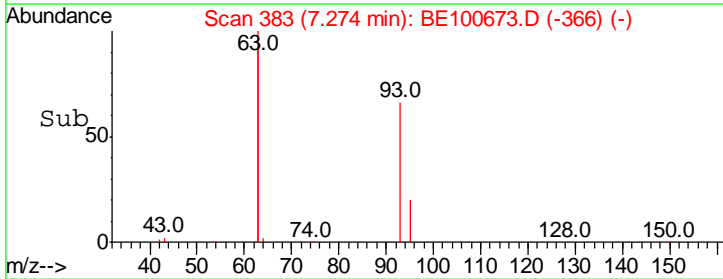
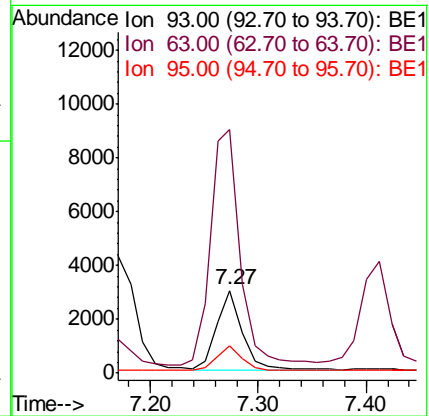



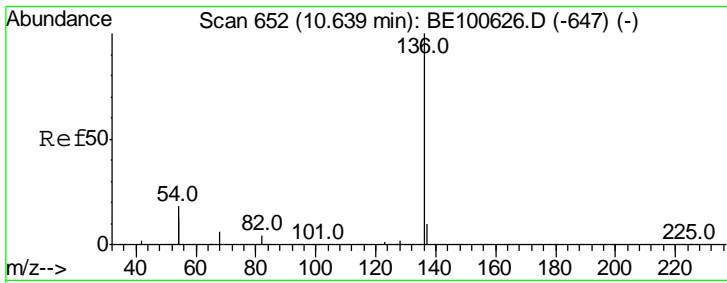

#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.63 min Scan# 651  
 Delta R.T. -0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09





Instrument :  
 BNA\_E  
 ClientSampled :


Tgt Ion	Resp	Lower	Upper
136	15626		
137	11.6	9.2	13.8
54	44.5	39.4	59.2
68	9.1	8.0	12.0

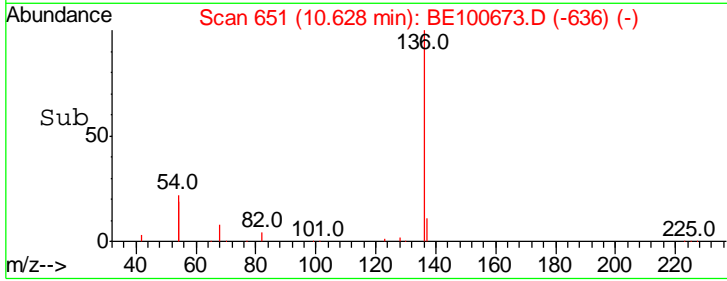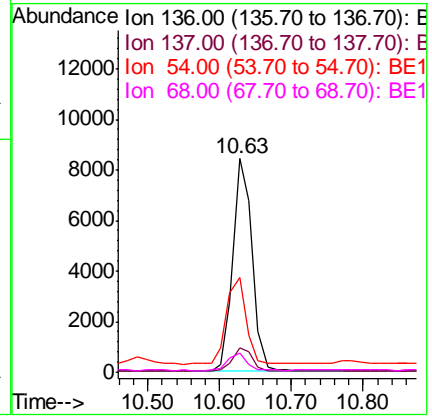

#8  
 Nitrobenzene-d5  
 Concen: 0.528 ng  
 RT: 8.99 min Scan# 525  
 Delta R.T. -0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Tgt Ion	Resp	Lower	Upper
82	5116		
128	143.1	107.8	161.8
54	205.3	166.1	249.1

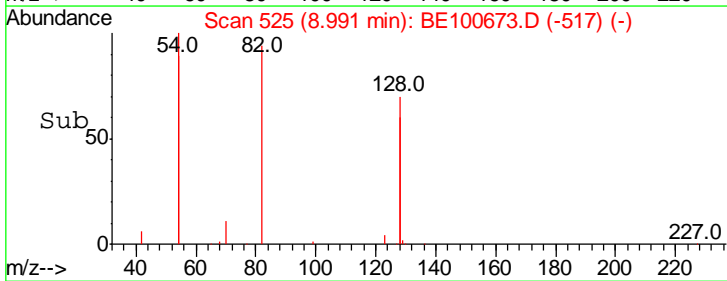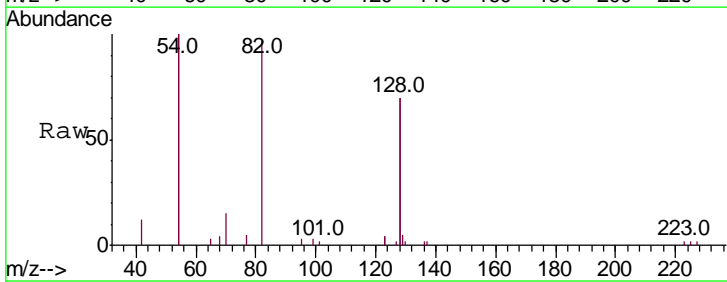
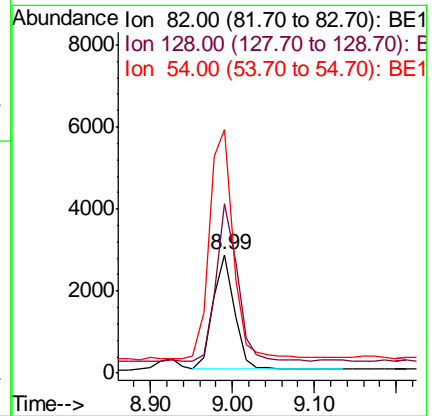
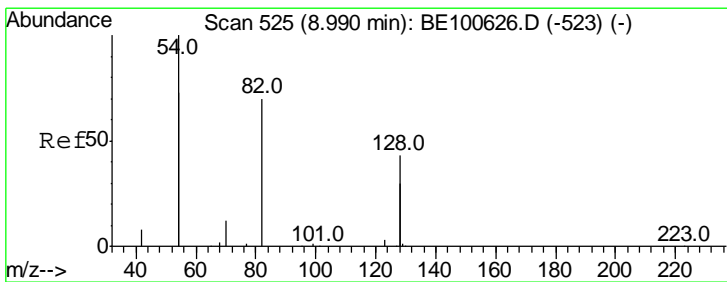


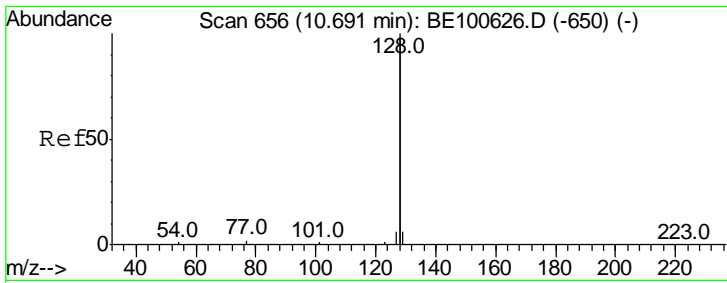

#9  
 Naphthalene  
 Concen: 0.378 ng  
 RT: 10.68 min Scan# 655  
 Delta R.T. -0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09





Instrument :  
 BNA\_E  
 ClientSampled :


Tgt Ion	Resp	Lower	Upper
128	100		
129	2.7	2.3	3.5
127	3.2	2.7	4.1

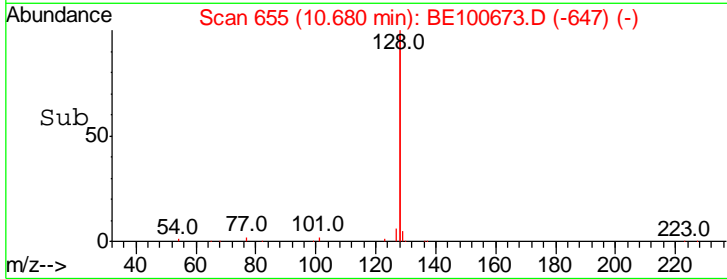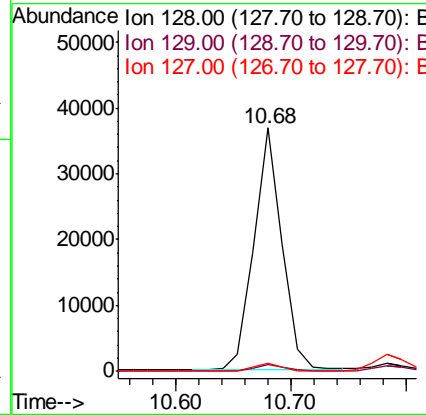

#10  
 Hexachlorobutadiene  
 Concen: 0.388 ng  
 RT: 10.98 min Scan# 678  
 Delta R.T. -0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Tgt Ion	Resp	Lower	Upper
225	100		
223	62.5	48.6	72.8
227	63.3	51.6	77.4

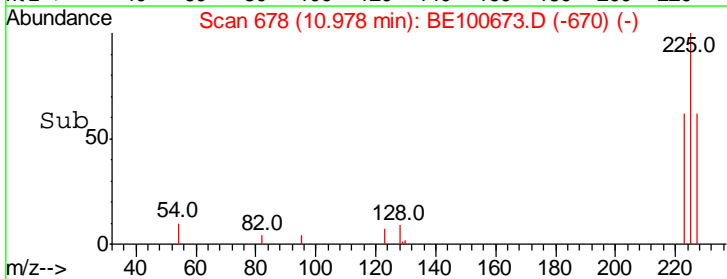

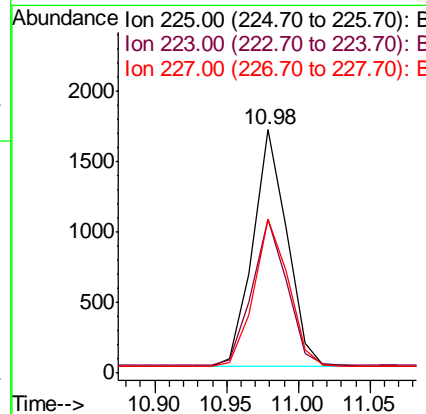



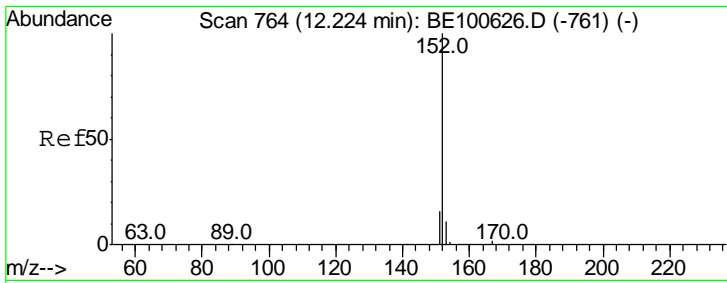

#11  
 2-Methylnaphthalene-d10  
 Concen: 0.376 ng  
 RT: 12.22 min Scan# 764  
 Delta R.T. 0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09




Instrument :  
 BNA\_E  
 ClientSampled :

Tgt Ion	Resp	Lower	Upper
152	100		
151	19.0	14.7	22.1

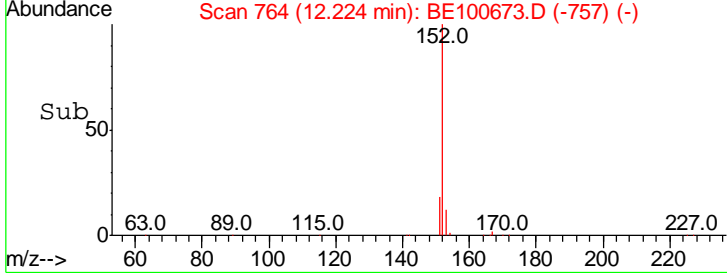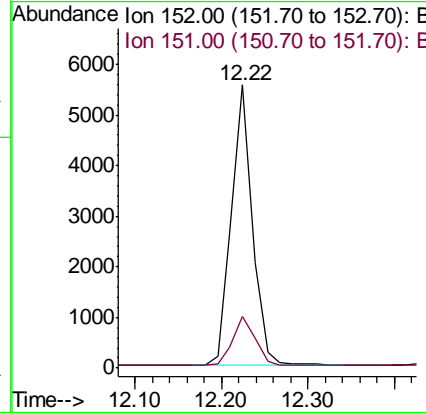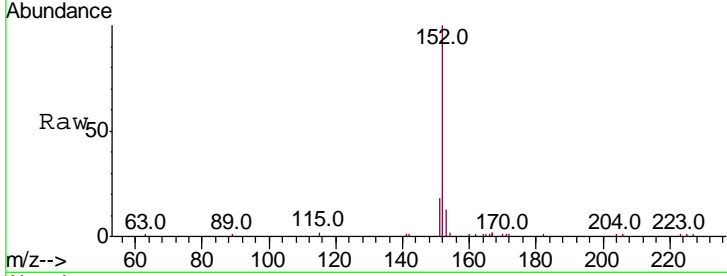


#12  
 2-Methylnaphthalene  
 Concen: 0.371 ng  
 RT: 12.30 min Scan# 769  
 Delta R.T. 0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Tgt Ion	Resp	Lower	Upper
142	100		
141	88.2	70.1	105.1
115	34.9	28.3	42.5

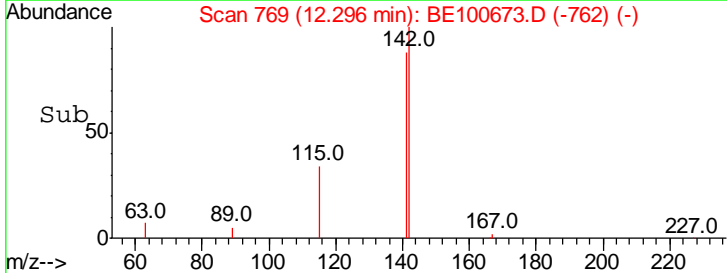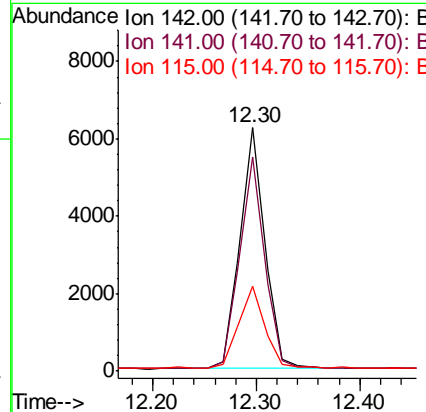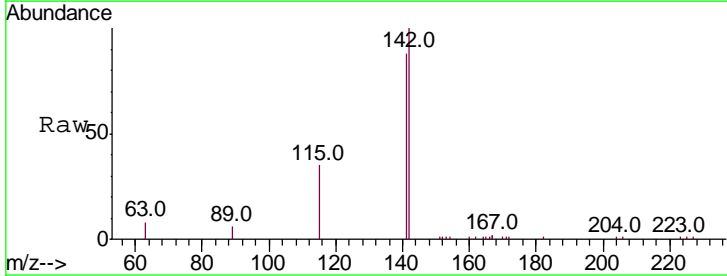









#13  
 Acenaphthene-d10  
 Concen: 0.400 ng  
 RT: 14.47 min Scan# 920  
 Delta R.T. 0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09




Instrument :  
 BNA\_E  
 ClientSampled :


Tgt Ion	Resp	Lower	Upper
164	10166		
162	97.5	82.0	123.0
160	45.7	37.5	56.3

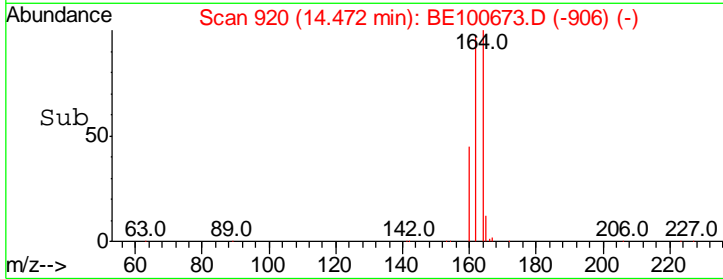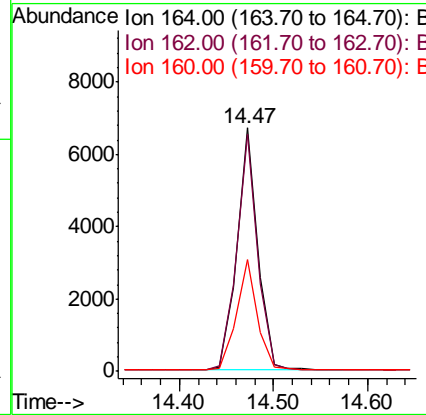

#14  
 2,4,6-Tribromophenol  
 Concen: 0.528 ng  
 RT: 15.94 min Scan# 1024  
 Delta R.T. 0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Tgt Ion	Resp	Lower	Upper
330	1419		
332	99.5	77.9	116.9
141	45.5	33.0	49.6

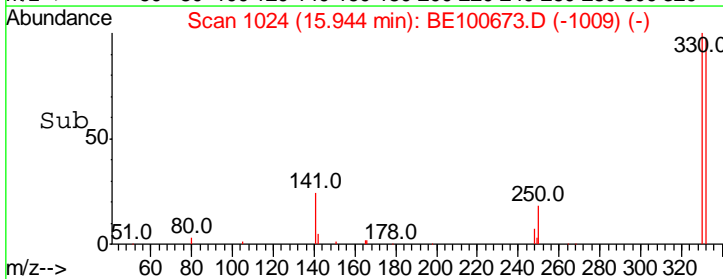
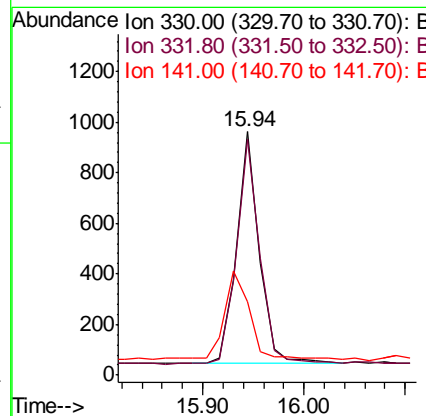



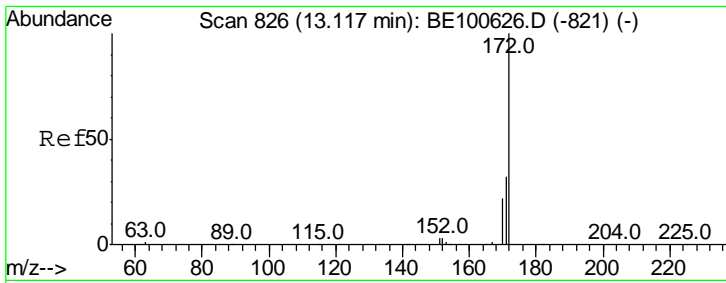

#15  
 2-Fluorobiphenyl  
 Concen: 0.413 ng  
 RT: 13.10 min Scan# 825  
 Delta R.T. 0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09





Instrument :  
 BNA\_E  
 ClientSampled :


Tgt Ion	Resp	Lower	Upper
172	100		
171	33.1	26.5	39.7
170	22.7	19.0	28.4

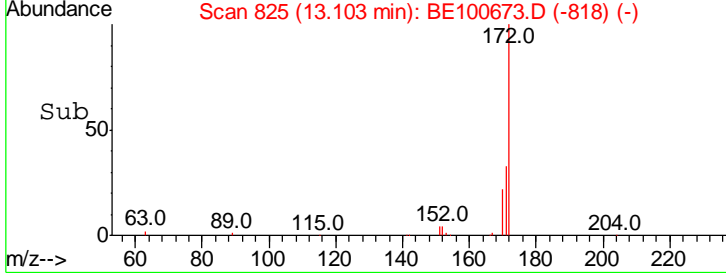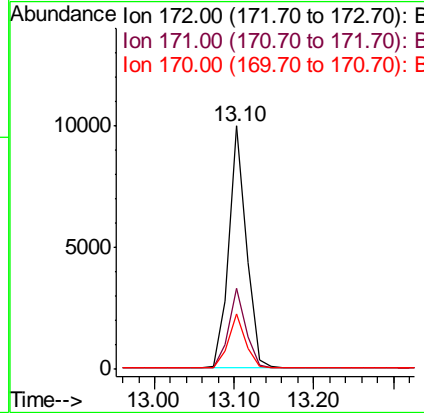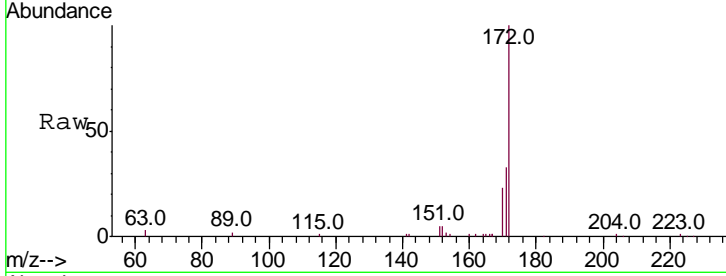

#16  
 Acenaphthylene  
 Concen: 0.360 ng  
 RT: 14.18 min Scan# 900  
 Delta R.T. -0.01 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Tgt Ion	Resp	Lower	Upper
152	100		
151	19.6	15.2	22.8
153	12.8	10.3	15.5

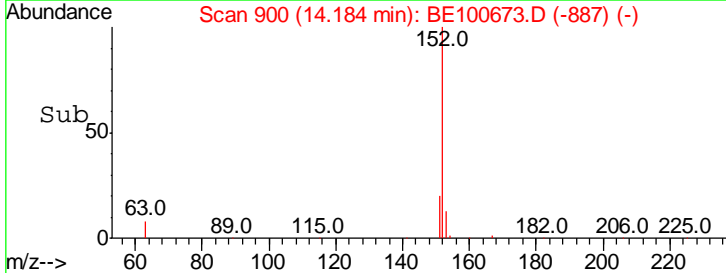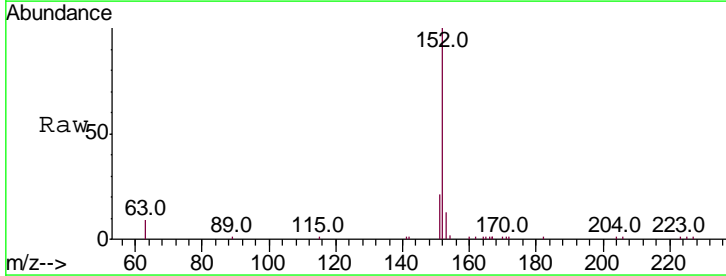
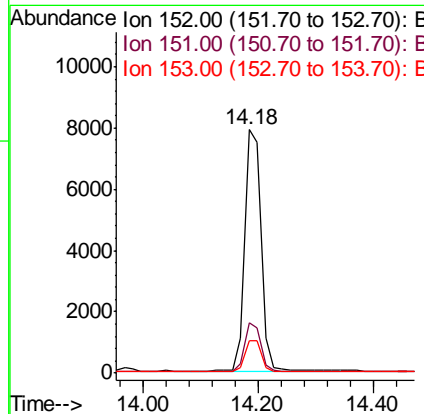
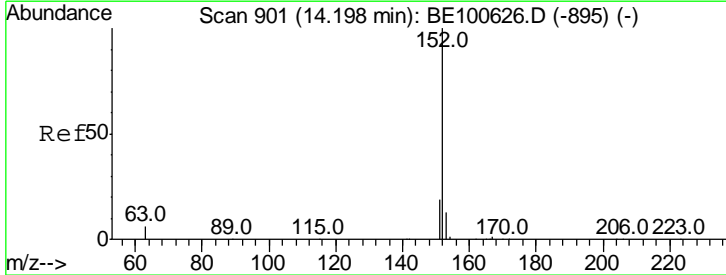


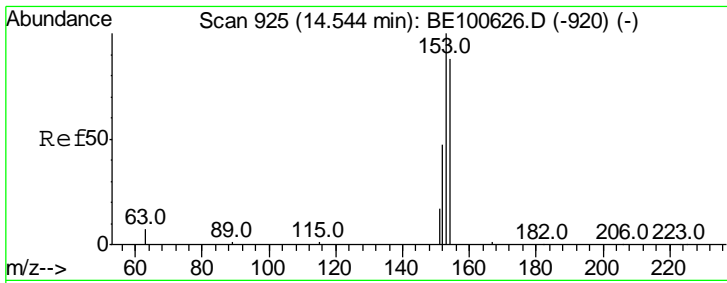

#17  
 Acenaphthene  
 Concen: 0.366 ng  
 RT: 14.53 min Scan# 924  
 Delta R.T. 0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09





Instrument :  
 BNA\_E  
 ClientSampled :


Tgt Ion	Resp	Lower	Upper
154	10341		
153	113.4	89.4	134.2
152	54.9	44.1	66.1

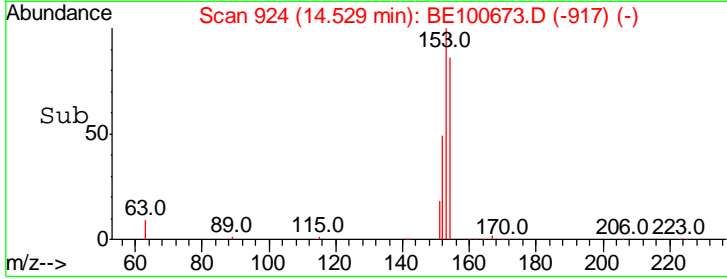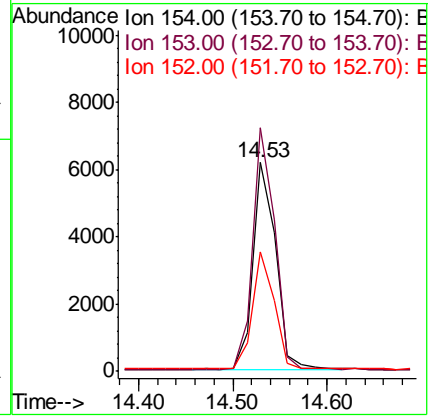

#18  
 Fluorene  
 Concen: 0.366 ng  
 RT: 15.50 min Scan# 991  
 Delta R.T. 0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Tgt Ion	Resp	Lower	Upper
166	13750		
165	98.7	78.6	117.8
167	13.3	10.9	16.3

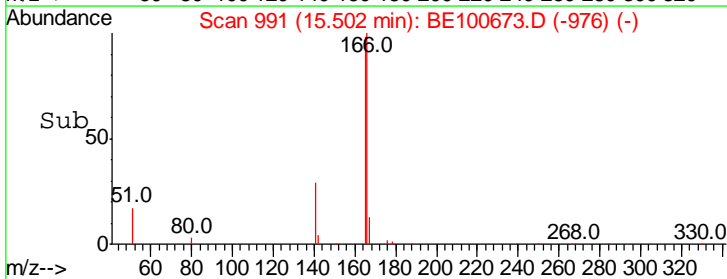
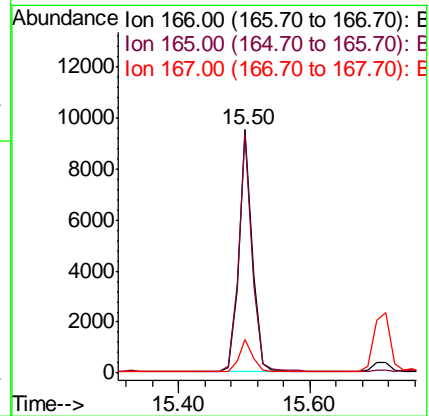



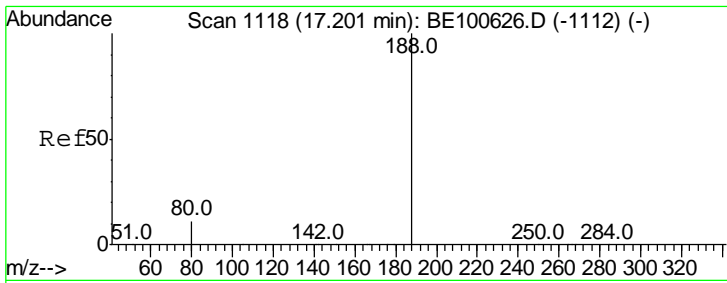

#19  
 Phenanthrene-d10  
 Concen: 0.400 ng  
 RT: 17.19 min Scan# 1117  
 Delta R.T. -0.01 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09





Instrument :  
 BNA\_E  
 ClientSampled :


Tgt Ion	Resp	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	12.4	5.4	8.0#

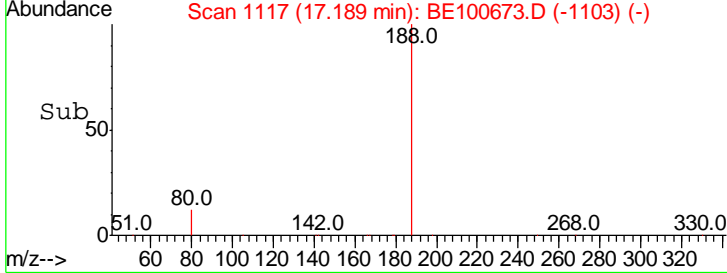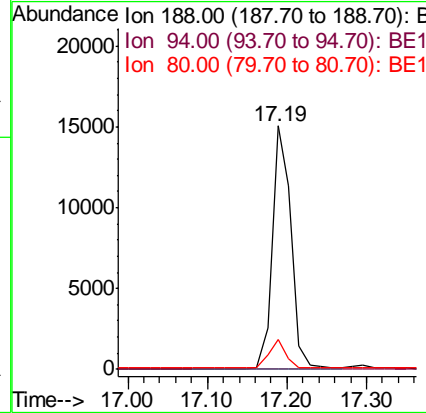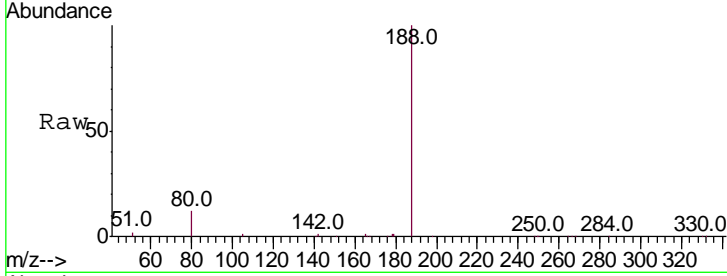

#20  
 4-Bromophenyl-phenylether  
 Concen: 0.365 ng  
 RT: 16.40 min Scan# 1058  
 Delta R.T. 0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Tgt Ion	Resp	Lower	Upper
248	100		
250	102.0	76.3	114.5
141	42.0	37.3	55.9

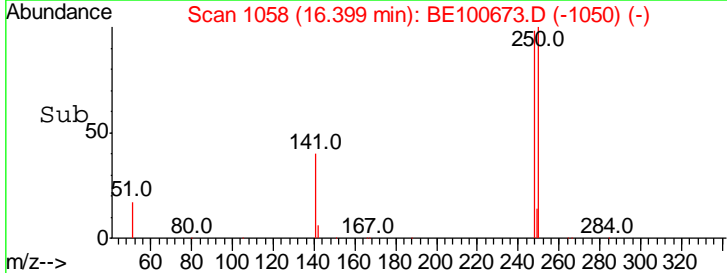
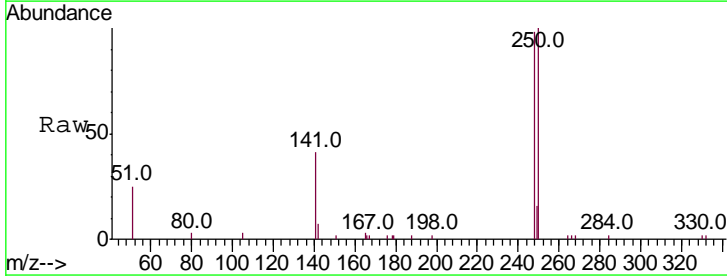
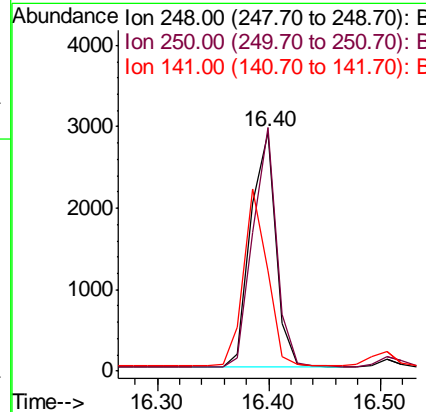
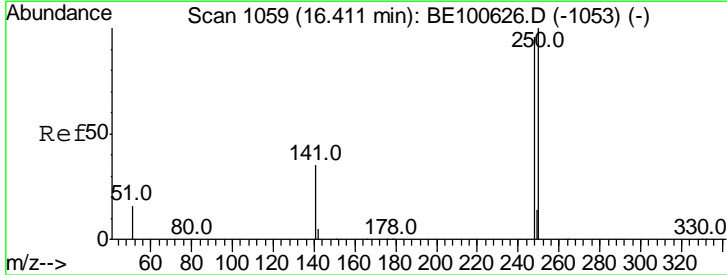


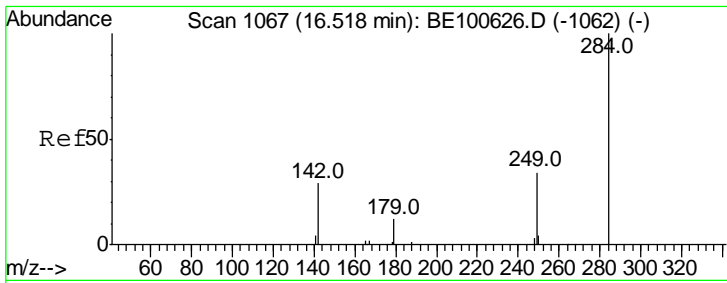

#21  
 Hexachlorobenzene  
 Concen: 0.375 ng  
 RT: 16.51 min Scan# 1066  
 Delta R.T. -0.01 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09




Instrument :  
 BNA\_E  
 ClientSampled :


Tgt Ion	Resp	Lower	Upper
284	4483		
142	35.7	28.6	42.8
249	33.0	26.3	39.5

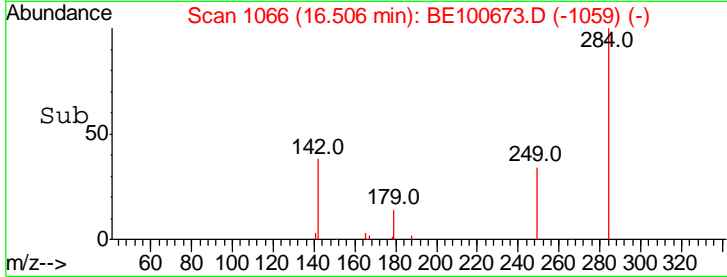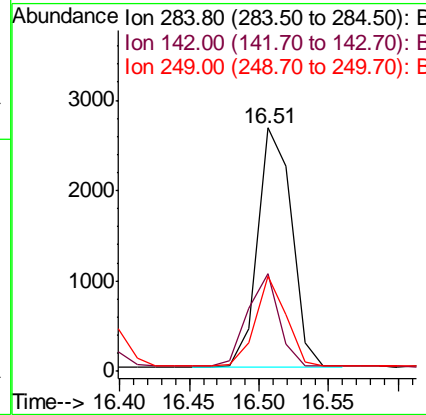

#22  
 Pentachlorophenol  
 Concen: 0.497 ng  
 RT: 16.85 min Scan# 1092  
 Delta R.T. 0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Tgt Ion	Resp	Lower	Upper
266	1916		
264	61.5	52.2	78.4
268	65.2	53.1	79.7

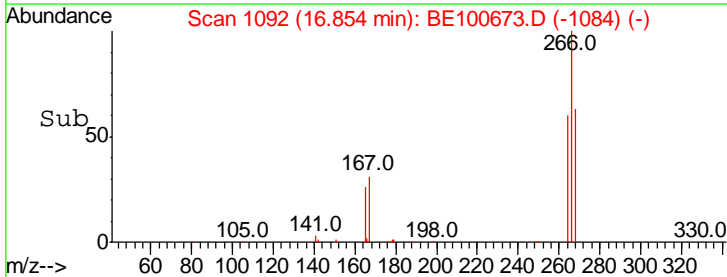
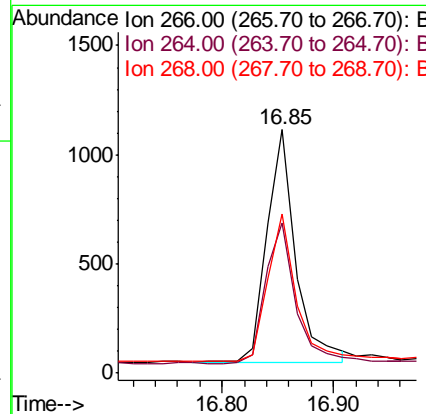



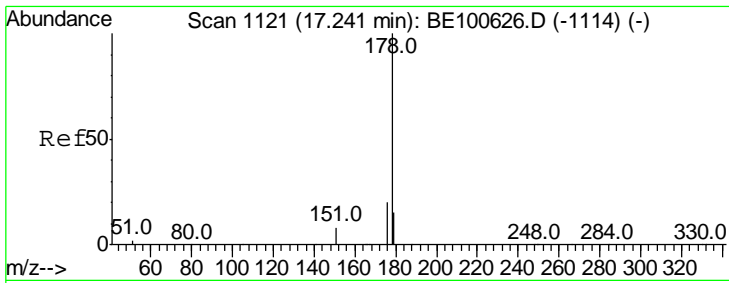

#23  
 Phenanthrene  
 Concen: 0.386 ng  
 RT: 17.23 min Scan# 1120  
 Delta R.T. -0.01 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09





Instrument :  
 BNA\_E  
 ClientSampled :


Tgt Ion	Resp	Lower	Upper
178	26201		
176	19.1	15.2	22.8
179	15.5	12.1	18.1

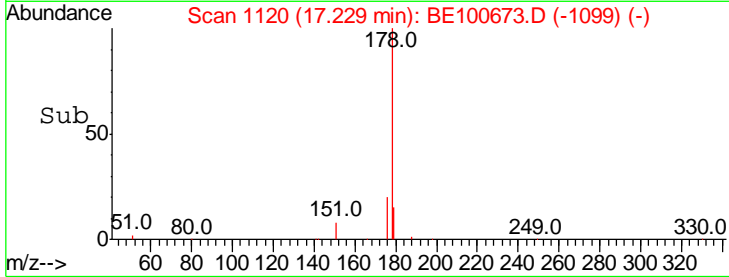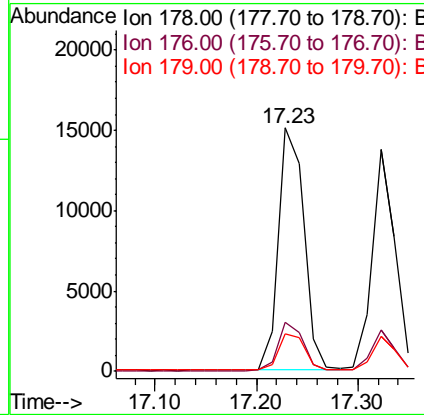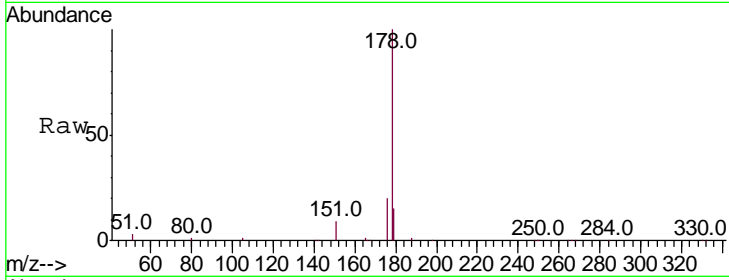

#24  
 Anthracene  
 Concen: 0.342 ng  
 RT: 17.32 min Scan# 1127  
 Delta R.T. 0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Tgt Ion	Resp	Lower	Upper
178	21534		
176	18.3	15.0	22.4
179	15.4	12.5	18.7

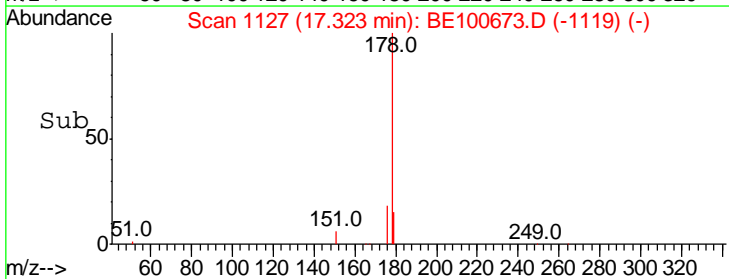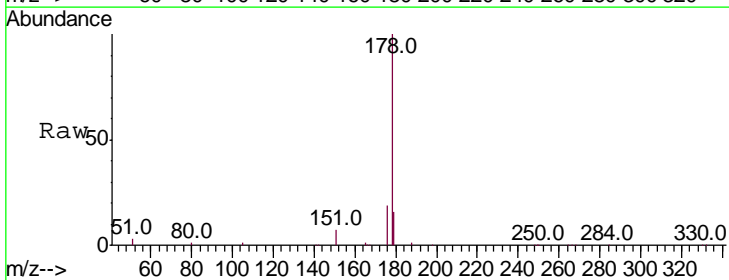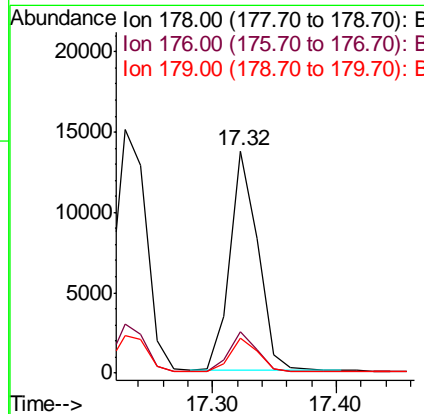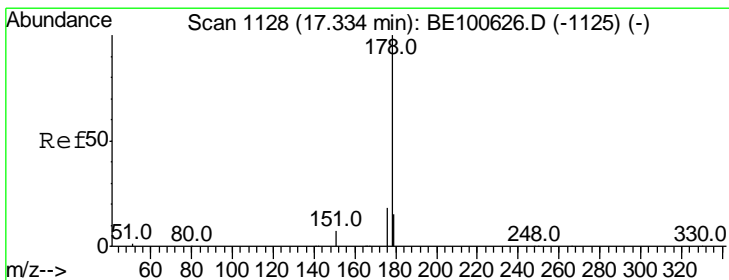






#25  
 Fluoranthene-d10  
 Concen: 0.376 ng  
 RT: 19.22 min Scan# 1384  
 Delta R.T. -0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Instrument :  
 BNA\_E  
 ClientSampled :

Tgt Ion: 212 Resp: 119688





Ion	Ratio	Lower	Upper
212	100		
106	2.8	2.3	3.5
104	1.6	1.3	1.9

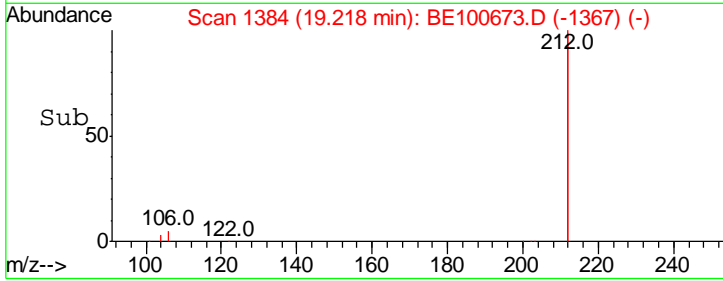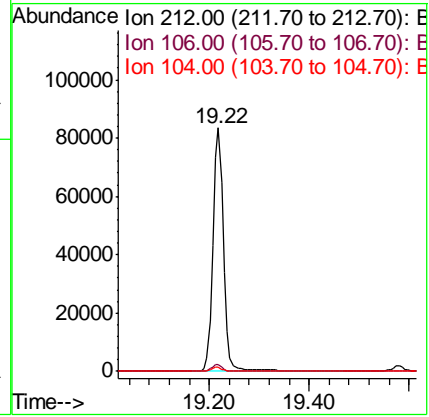


#26  
 Fluoranthene  
 Concen: 0.396 ng  
 RT: 19.25 min Scan# 1389  
 Delta R.T. -0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Tgt Ion: 202 Resp: 35065

Ion	Ratio	Lower	Upper
202	100		
101	10.4	8.5	12.7
203	17.0	13.8	20.8

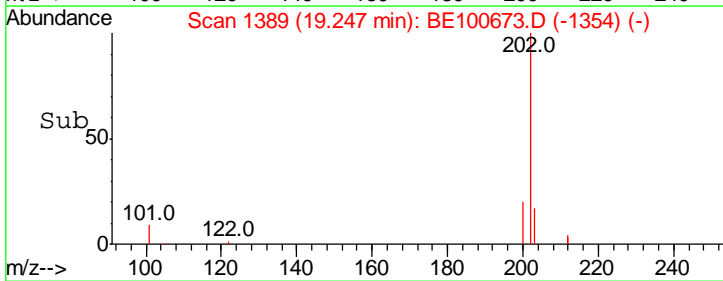

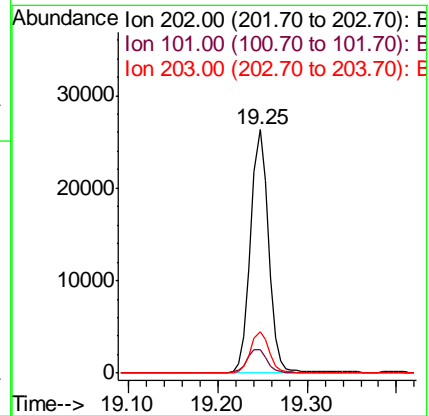



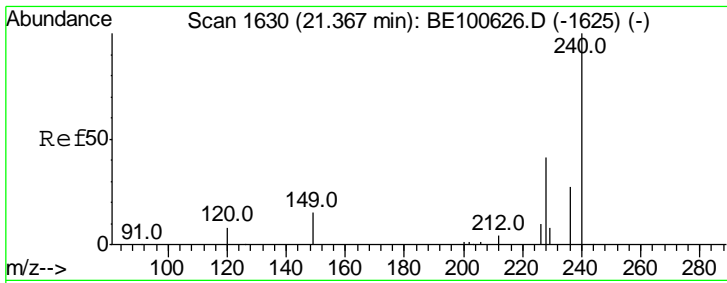

#27  
 Chrysene-d12  
 Concen: 0.400 ng  
 RT: 21.35 min Scan# 1629  
 Delta R.T. -0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09




Instrument :  
 BNA\_E  
 ClientSampled :

Tgt Ion	Resp	Lower	Upper
240	100		
120	9.0	7.6	11.4
236	27.1	22.1	33.1

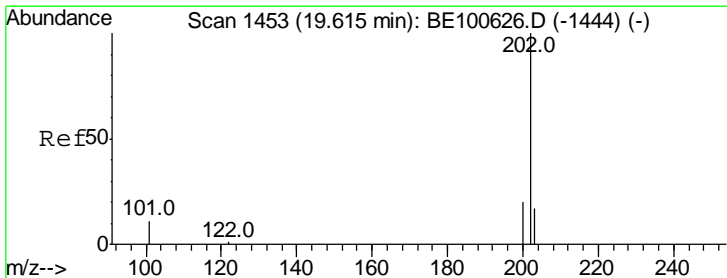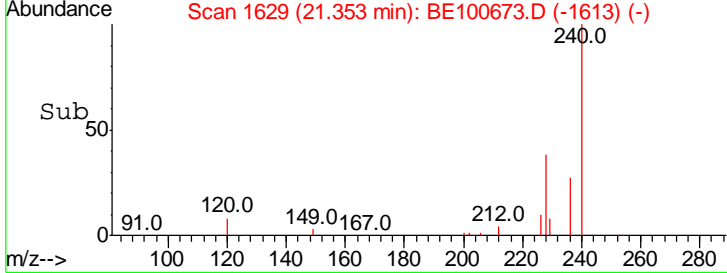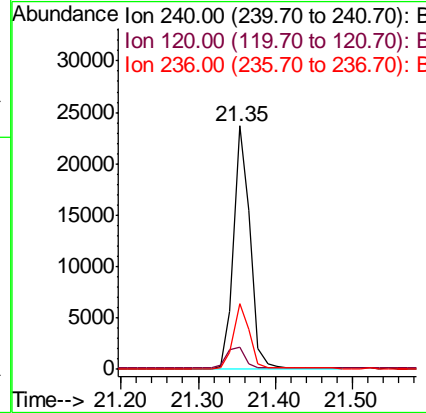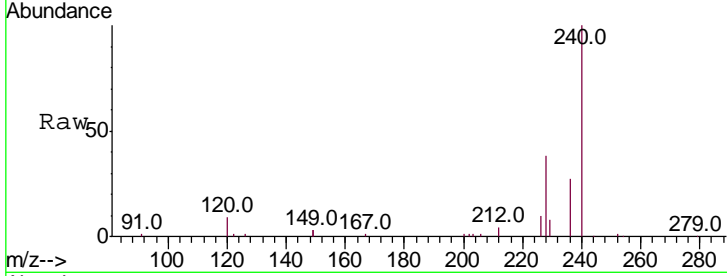


#28  
 Pyrene  
 Concen: 0.380 ng  
 RT: 19.61 min Scan# 1452  
 Delta R.T. -0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Tgt Ion	Resp	Lower	Upper
202	100		
200	20.8	16.7	25.1
203	17.8	14.0	21.0

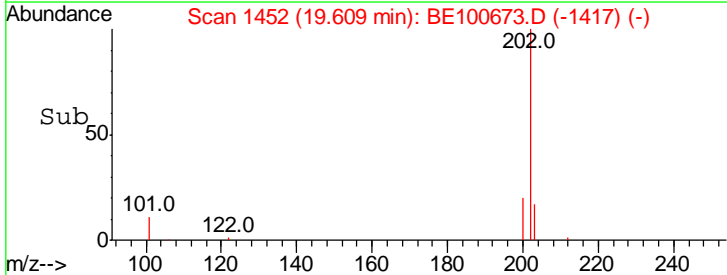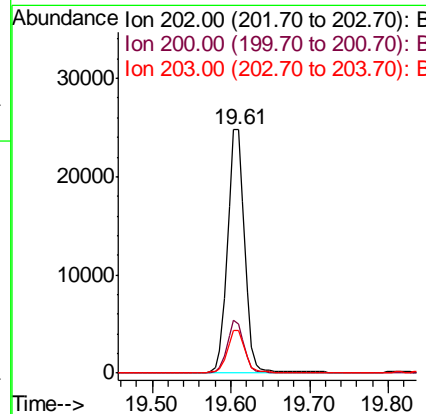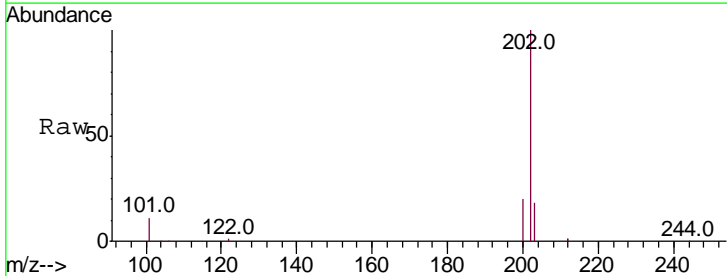








#29  
 Terphenyl-d14  
 Concen: 0.413 ng  
 RT: 19.82 min Scan# 1488  
 Delta R.T. -0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09





Instrument :  
 BNA\_E  
 ClientSampled :


Tgt Ion	Resp	Lower	Upper
244	100		
212	28.4	23.7	35.5
122	8.4	7.9	11.9

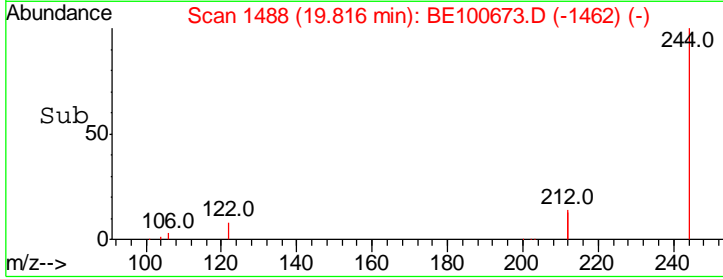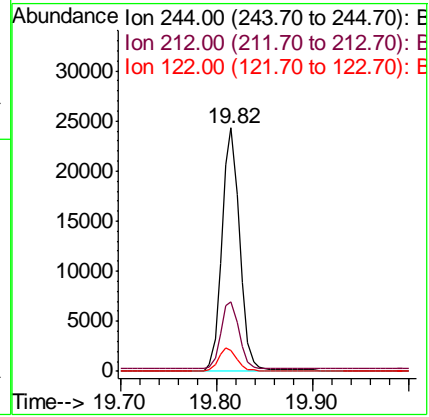

#30  
 Benzo(a)anthracene  
 Concen: 0.362 ng  
 RT: 21.34 min Scan# 1628  
 Delta R.T. -0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Tgt Ion	Resp	Lower	Upper
228	100		
226	26.9	21.4	32.0
229	20.0	16.0	24.0

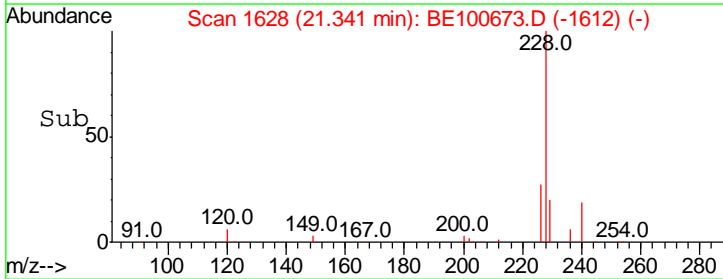

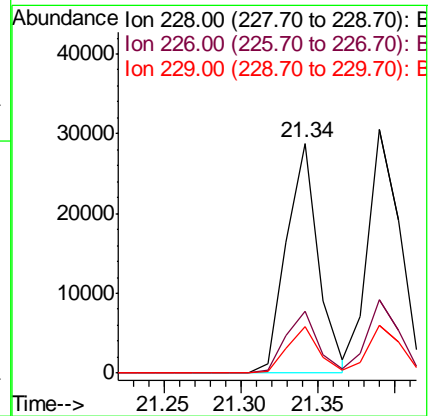





#31  
 Chrysene  
 Concen: 0.382 ng  
 RT: 21.39 min Scan# 1632  
 Delta R.T. -0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09




Instrument :  
 BNA\_E  
 ClientSampled :


Tgt Ion	Resp	Lower	Upper
228	100		
226	30.1	24.6	37.0
229	19.5	15.8	23.8

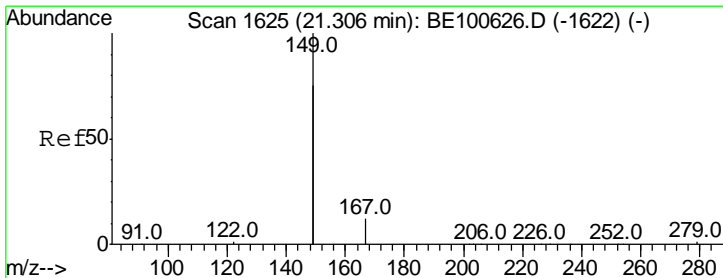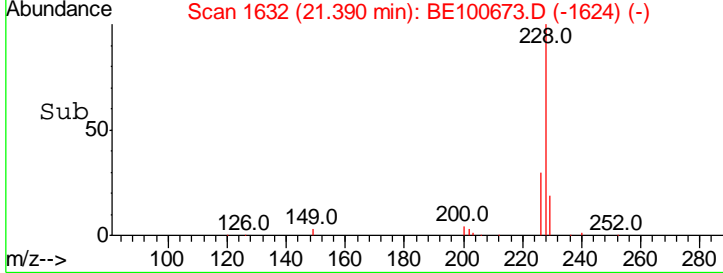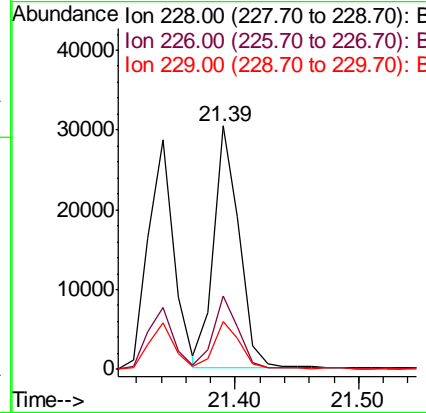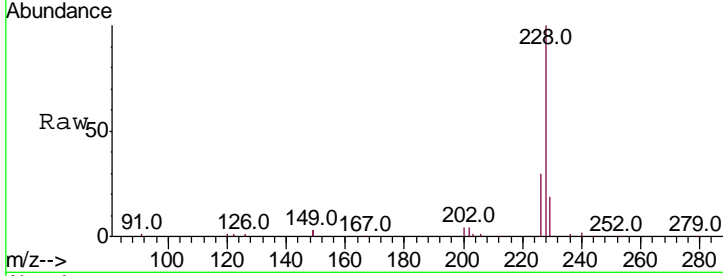

#32  
 Bis(2-ethylhexyl)phthalate  
 Concen: 0.361 ng  
 RT: 21.28 min Scan# 1623  
 Delta R.T. -0.01 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Tgt Ion	Resp	Lower	Upper
149	100		
167	6.8	5.5	8.3
279	1.1	0.9	1.3


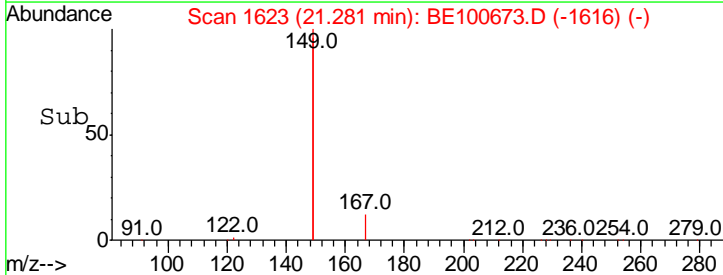
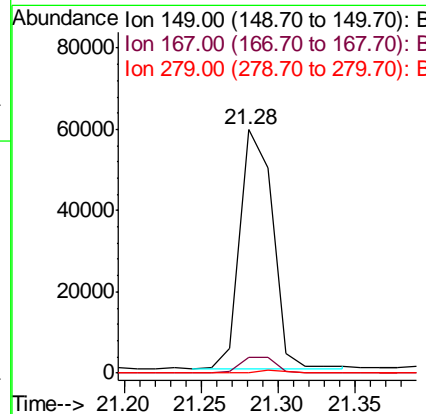
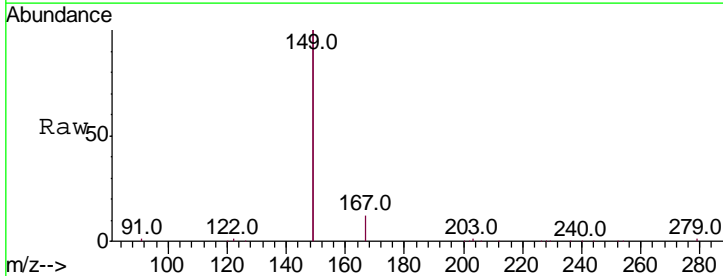


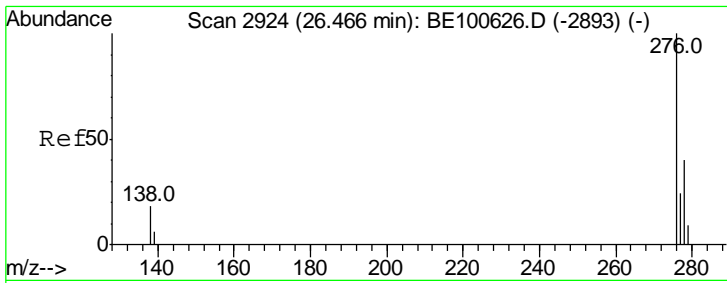

#33  
 Indeno(1,2,3-cd)pyrene  
 Concen: 0.360 ng  
 RT: 26.43 min Scan# 2913  
 Delta R.T. -0.01 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09




Instrument :  
 BNA\_E  
 ClientSampled :


Tgt Ion	Resp	Lower	Upper
276	100		
138	19.2	15.3	22.9
277	24.7	19.4	29.2

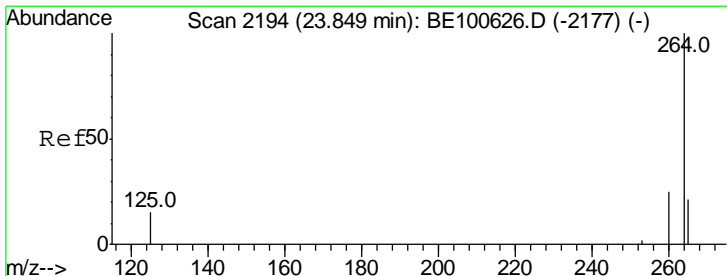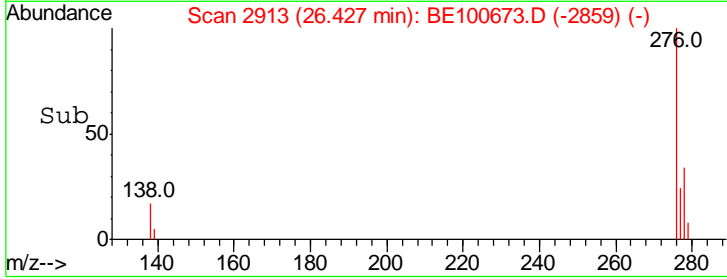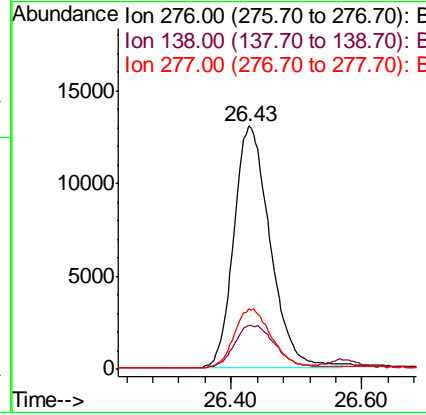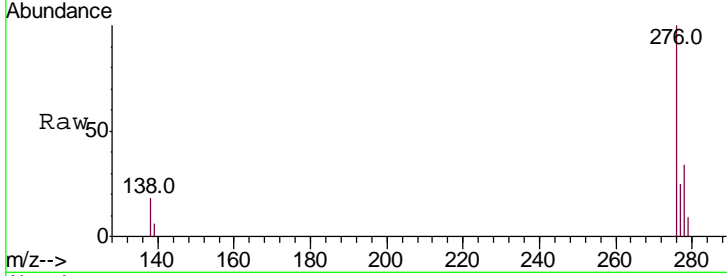

#34  
 Perylene-d12  
 Concen: 0.400 ng  
 RT: 23.83 min Scan# 2188  
 Delta R.T. -0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Tgt Ion	Resp	Lower	Upper
264	100		
260	24.7	19.4	29.2
265	27.3	21.7	32.5


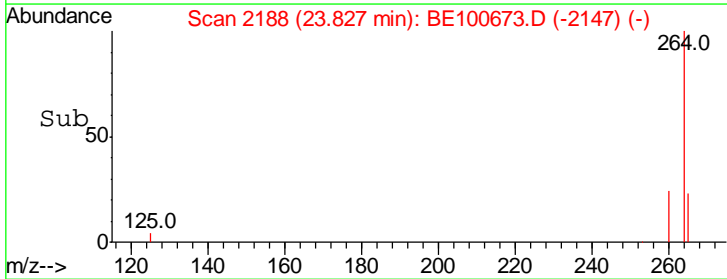
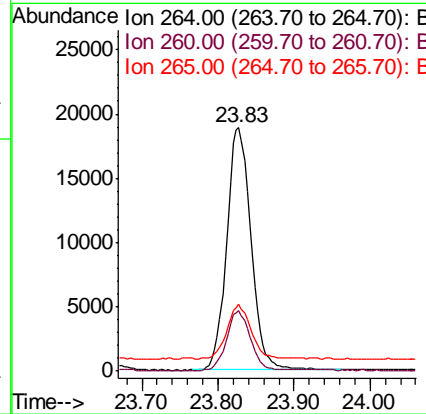
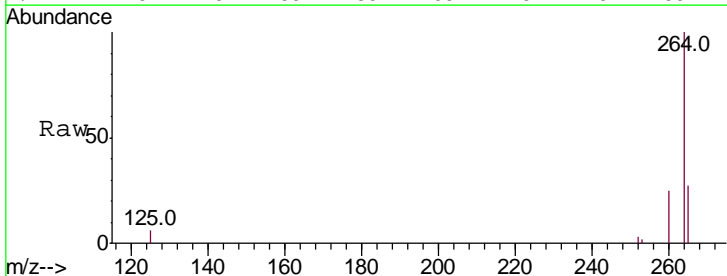




#35  
 Benzo(b)fluoranthene  
 Concen: 0.354 ng  
 RT: 23.07 min Scan# 1976  
 Delta R.T. -0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09




Instrument :  
 BNA\_E  
 ClientSampled :


Tgt Ion	Resp	Lower	Upper
252	100		
253	22.9	18.4	27.6
125	8.8	7.6	11.4

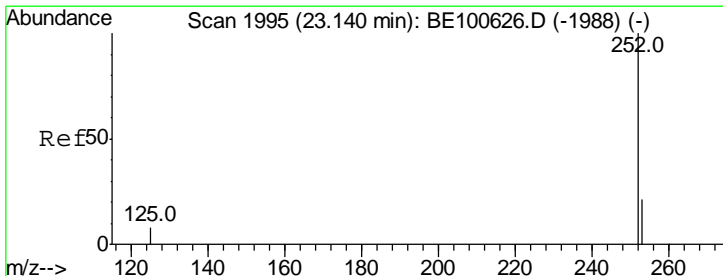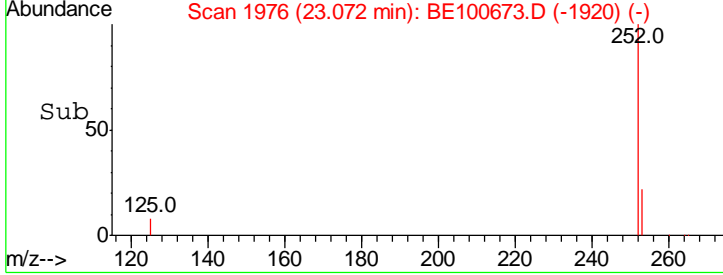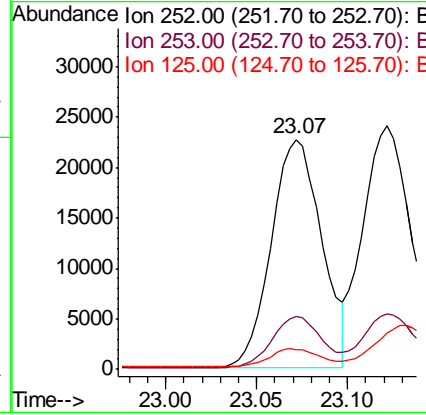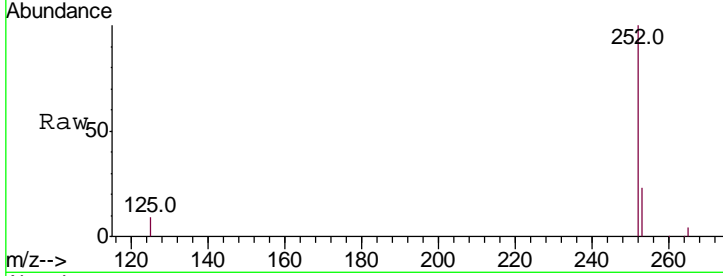

#36  
 Benzo(k)fluoranthene  
 Concen: 0.364 ng  
 RT: 23.12 min Scan# 1990  
 Delta R.T. -0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Tgt Ion	Resp	Lower	Upper
252	100		
253	23.0	18.4	27.6
125	14.8	11.6	17.4

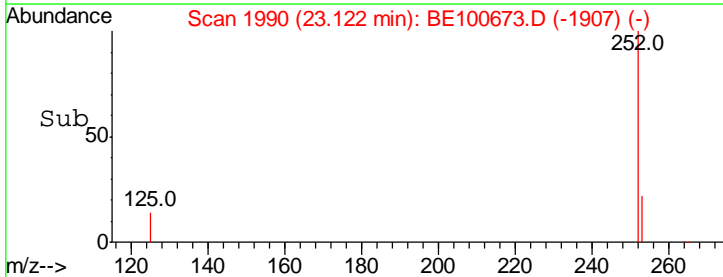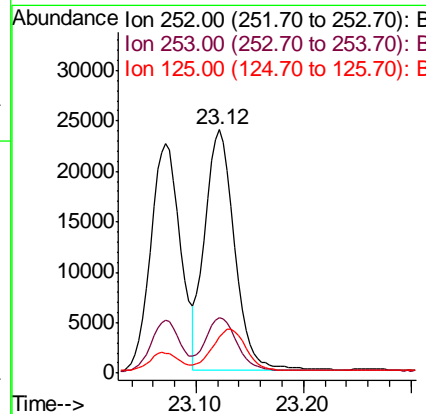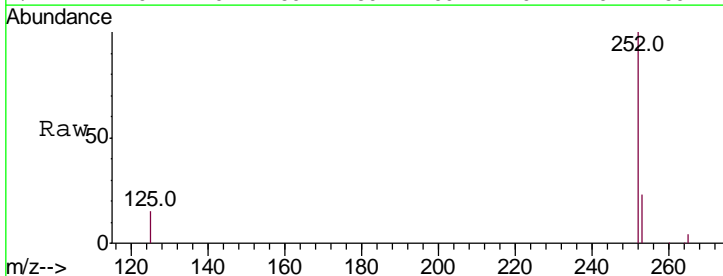







#37  
 Benzo(a)pyrene  
 Concen: 0.351 ng  
 RT: 23.71 min Scan# 2156  
 Delta R.T. -0.01 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Instrument :  
 BNA\_E  
 ClientSampled :

Tgt Ion: 252 Resp: 40064




Ion	Ratio	Lower	Upper
252	100		
253	22.6	18.4	27.6
125	10.2	8.2	12.4

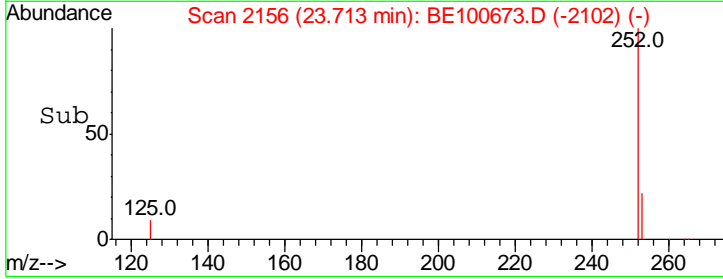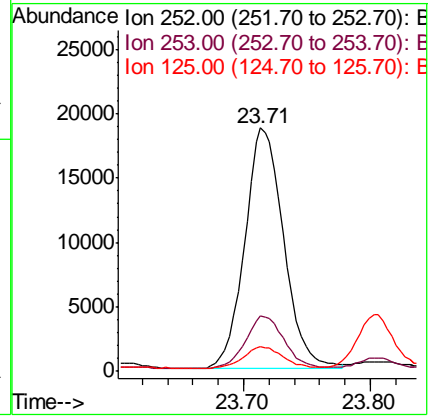


#38  
 Dibenzo(a,h)anthracene  
 Concen: 0.350 ng  
 RT: 26.46 min Scan# 2922  
 Delta R.T. -0.00 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Tgt Ion: 278 Resp: 41302

Ion	Ratio	Lower	Upper
278	100		
139	13.2	10.9	16.3
279	24.3	19.4	29.2

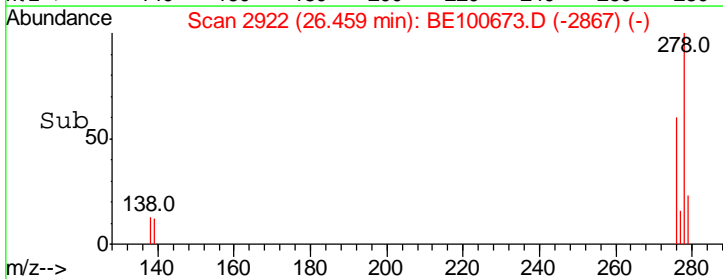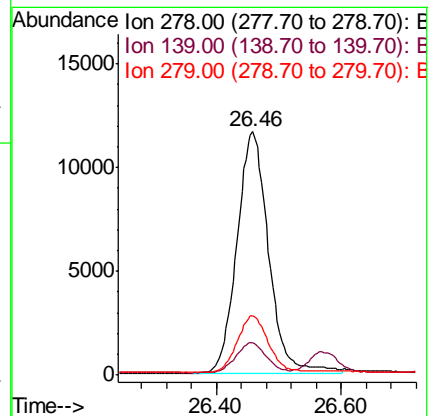



#39  
 Benzo(a,h,i)perylene  
 Concen: 0.358 ng  
 RT: 27.23 min Scan# 3137  
 Delta R.T. -0.01 min  
 Lab File: BE100673.D  
 Acq: 23 Oct 2019 22:09

Instrument :  
 BNA\_E  
 ClientSampled :

Tot Ion: 276 Resp: 42510

Ion	Ratio	Lower	Upper
276	100		
277	24.4	19.4	29.0
138	18.4	13.6	20.4

