
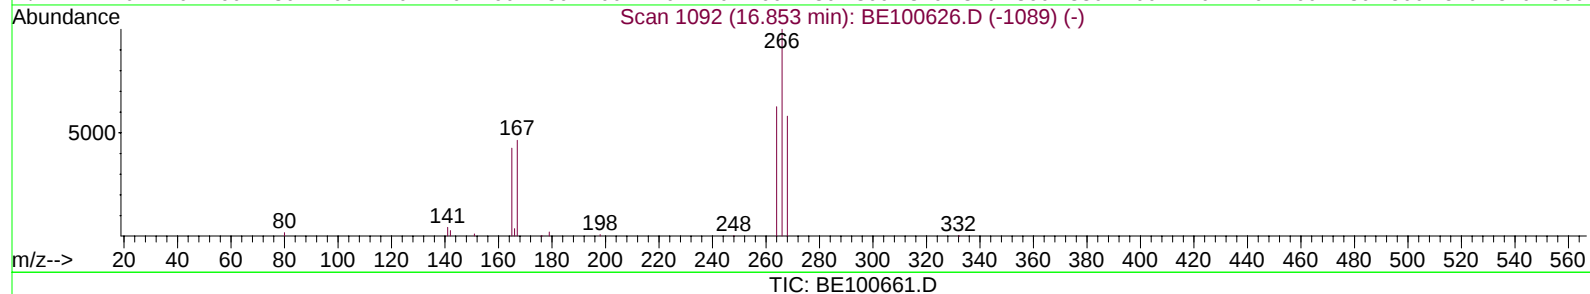
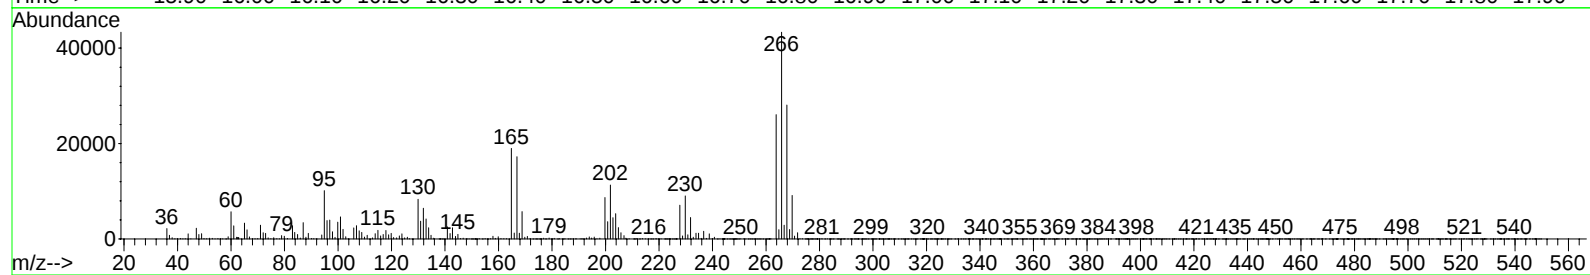


```

Data Path   : Z:\svoasrv\HPCHEM1\BNA E\Data\BE102319\
Data File   : BE100661.D
Acq On      : 23 Oct 2019   14:48
Operator    : JU
Sample      : DFTPP
Misc        :
ALS Vial    : 1      Sample Multiplier: 1

```

Quant Time: Oct 23 18:35:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 23 16:49:33 2019
Response via : Initial Calibration

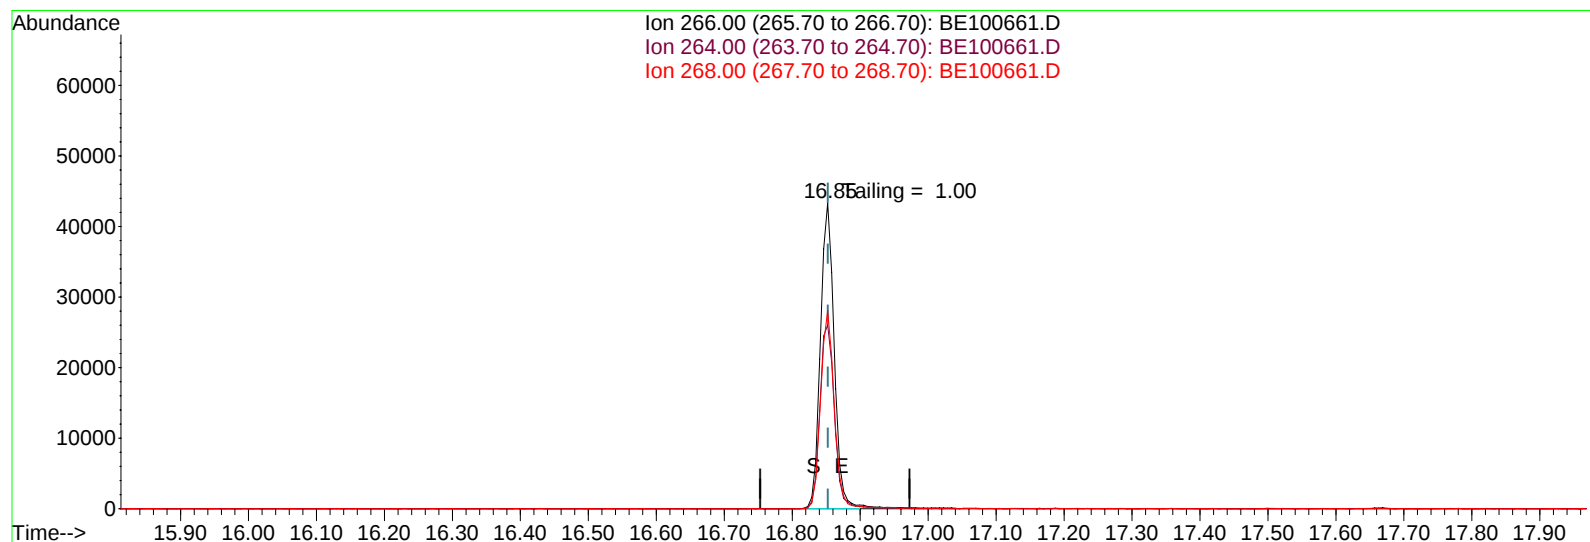

(22) Pentachlorophenol

16.852min (-0.001) 79061.44ng

response 61738

Ion	Exp%	Act%
266.00	100	100
264.00	65.30	60.13
268.00	66.40	64.81
0.00	0.00	0.00