


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE102319\
 Data File : BE100661.D
 Acq On : 23 Oct 2019 14:48
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE101019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 23 16:49:33 2019

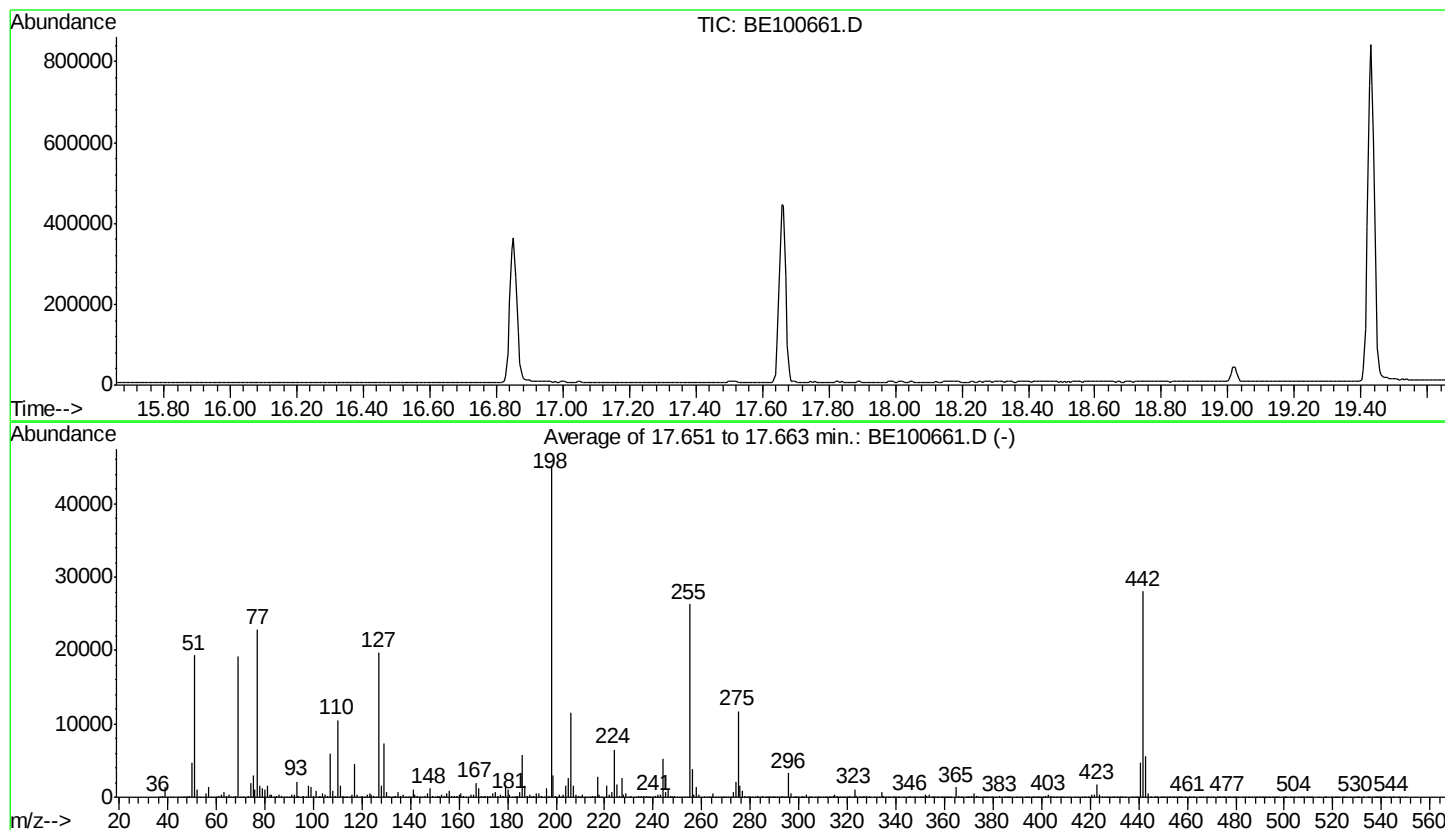

AutoFind: Scans 2564, 2565, 2566; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	19293	PASS
68	69	0.00	2	1.1	206	PASS
69	198	0.00	100	42.5	19207	PASS
70	69	0.00	2	0.5	92	PASS
127	198	10	80	43.6	19696	PASS
197	198	0.00	2	0.2	96	PASS
198	198	100	100	100.0	45195	PASS
199	198	5	9	6.6	2999	PASS
275	198	10	60	25.9	11717	PASS
365	198	1	100	3.0	1354	PASS
441	198	0.01	100	10.4	4702	PASS
442	198	50	100	62.0	28043	PASS
443	442	15	24	19.9	5591	PASS