


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE102418\
 Data File : BE098031.D
 Acq On : 24 Oct 2018 9:34
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE102418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 24 13:49:35 2018

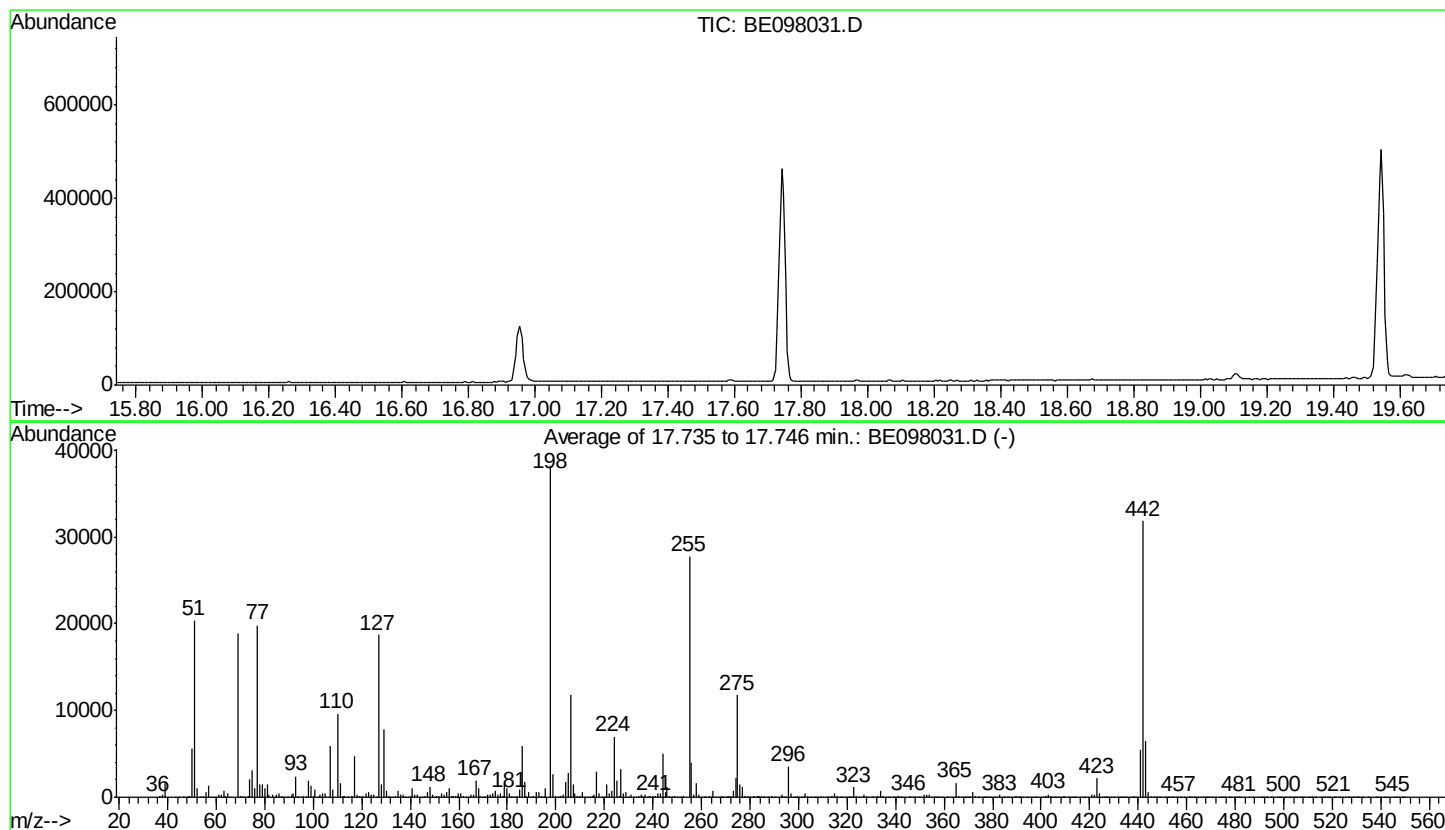

AutoFind: Scans 2578, 2579, 2580; Background Corrected with Scan 2571

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.3	20339	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	49.2	18811	PASS
70	69	0.00	2	0.6	119	PASS
127	198	10	80	48.9	18696	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38195	PASS
199	198	5	9	7.0	2662	PASS
275	198	10	60	30.7	11738	PASS
365	198	1	100	4.3	1656	PASS
441	198	0.01	100	14.2	5439	PASS
442	198	50	100	83.4	31842	PASS
443	442	15	24	20.5	6536	PASS