


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102518\
Quantitation Report (QT Reviewed)
Data File : BE098060.D
Acq On : 25 Oct 2018 17:57
Operator : SJ/JU
Sample : J5568-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AJ9

Manual Integrations
APPROVED

Sohil
10/26/2018 3:47:37 PM

Quant Time: Oct 26 05:54:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 26 05:34:25 2018
Response via : Initial Calibration

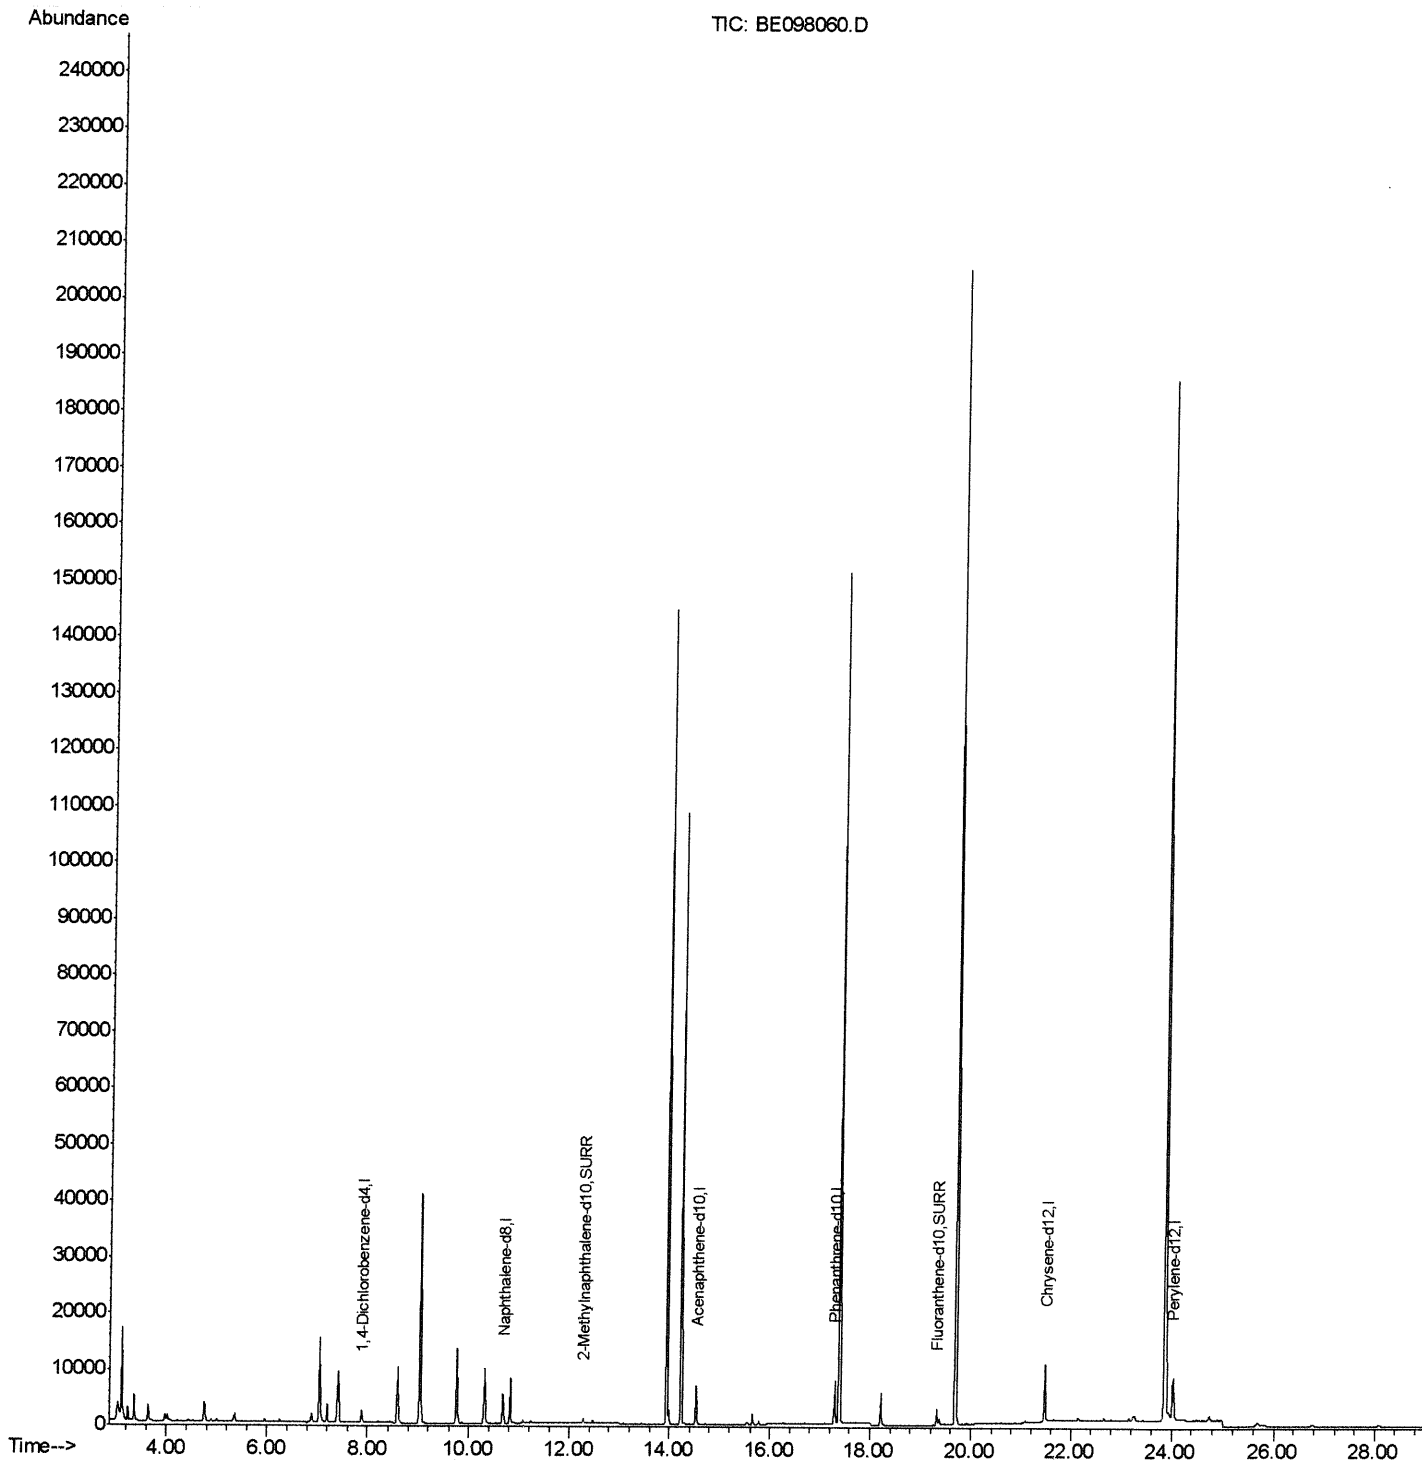

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102518\
Quantitation Report (Qedit)




Data File : BE098060.D
Acq On : 25 Oct 2018 17:57
Operator : SJ/JU
Sample : J5568-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AJ9

Manual Integrations
APPROVED

Sohil
10/26/2018 3:47:37 PM

Quant Time: Oct 26 05:37:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 26 05:34:25 2018
Response via : Initial Calibration

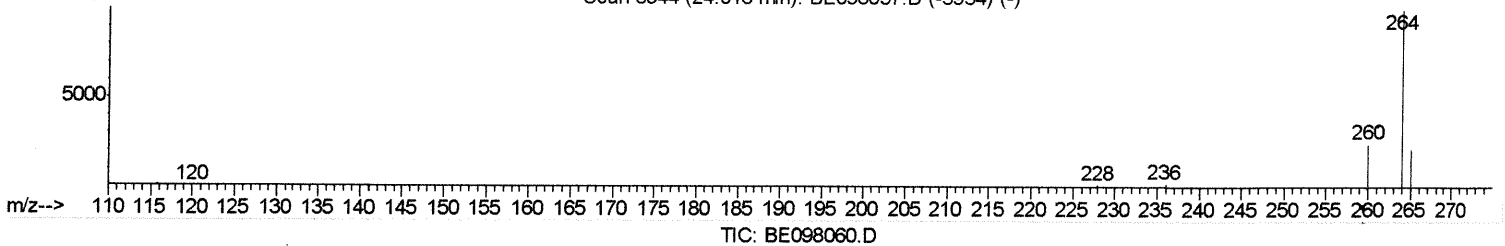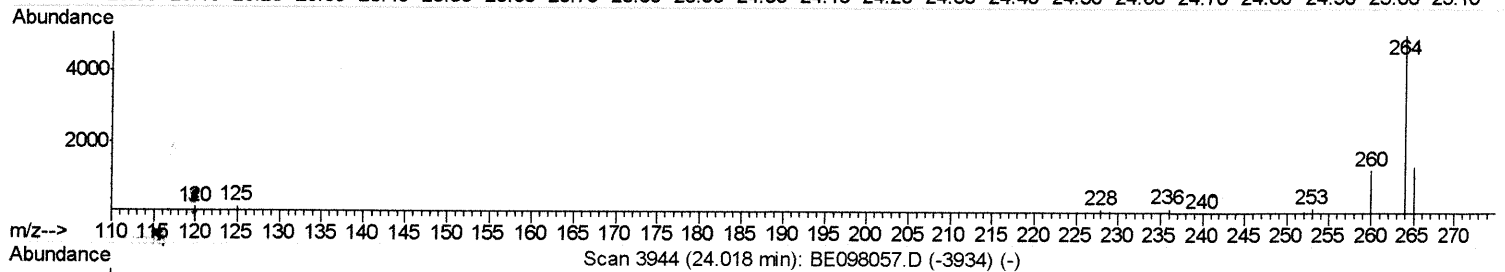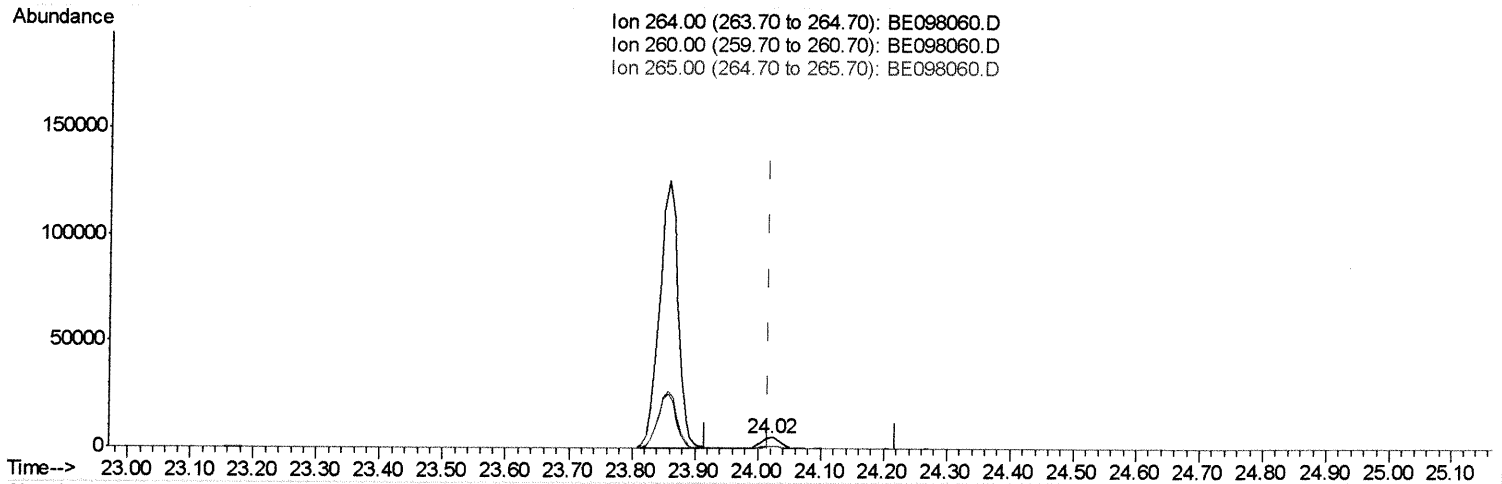

(20) Perylene-d12 (I)

24.018min (+0.000) 0.40ng/ul

response 11538

Ion	Exp%	Act%
264.00	100	100
260.00	25.20	25.08
265.00	28.00	27.42
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102518\
Quantitation Report (Qedit)




Data File : BE098060.D
Acq On : 25 Oct 2018 17:57
Operator : SJ/JU
Sample : J5568-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AJ9

Manual Integrations
APPROVED

Sohil
10/26/2018 3:47:37 PM

Quant Time: Oct 26 05:37:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 26 05:34:25 2018
Response via : Initial Calibration

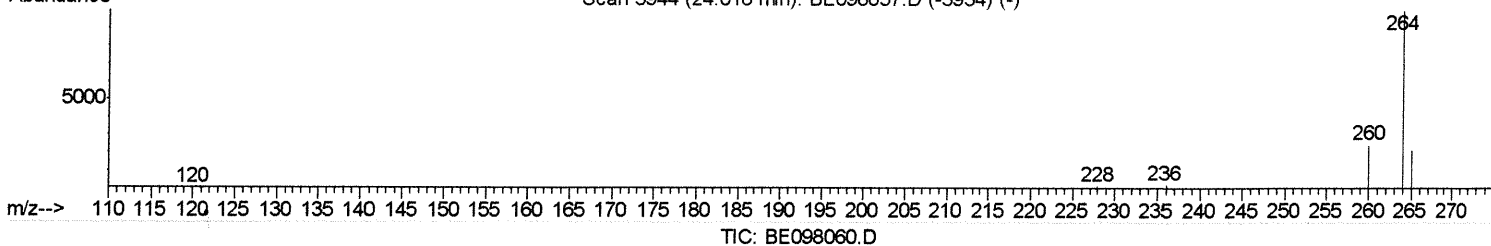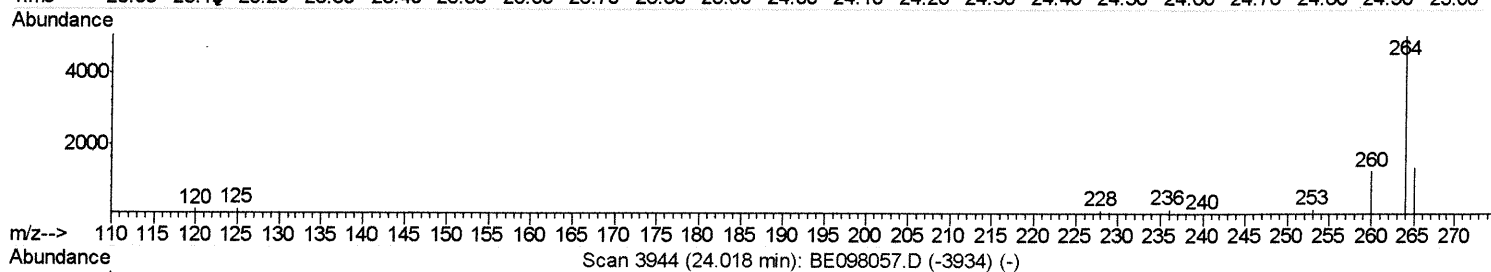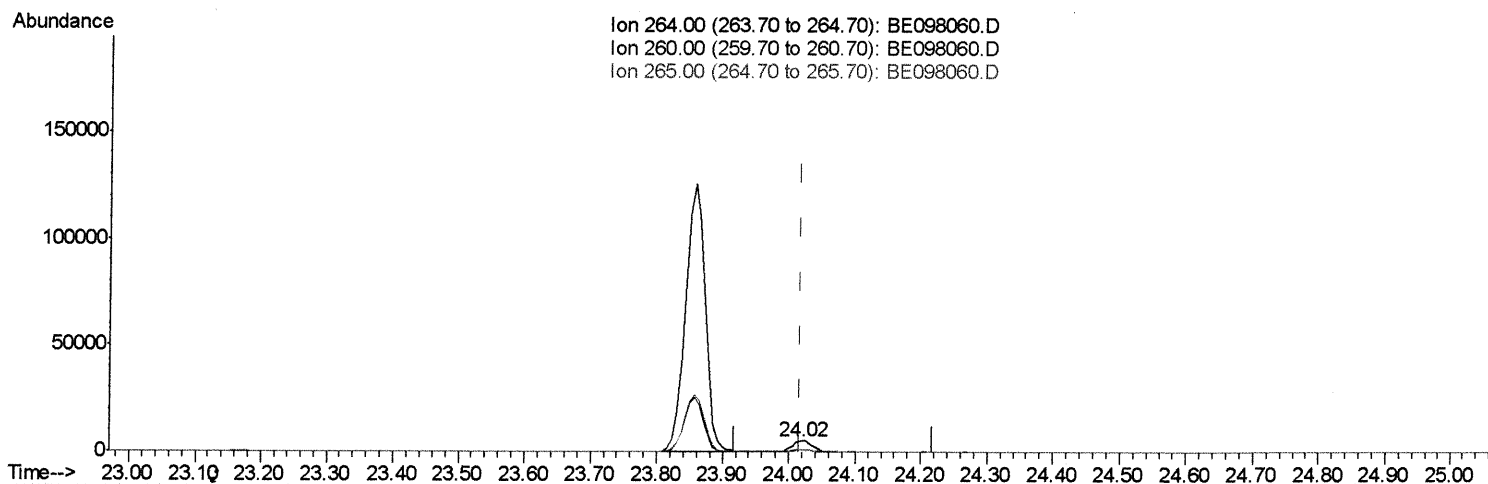

(20) Perylene-d12 (I)

24.018min (+0.000) 0.40ng/ul m

> SJ 10/29/18

response 10181

Ion	Exp%	Act%
264.00	100	100
260.00	25.20	25.08
265.00	28.00	27.42
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102518\
 Quantitation Report (QT Reviewed)
 Data File : BE098060.D
 Acq On : 25 Oct 2018 17:57
 Operator : SJ/JU
 Sample : J5568-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AJ9

Manual Integrations
 APPROVED

Sohil
 10/26/2018 3:47:37 PM

Quant Time: Oct 26 05:54:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 26 05:34:25 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	1073	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	5525	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	3868	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.29	188	9262	0.40	ng/ul	0.00
16) Chrysene-d12	21.47	240	12167	0.40	ng/ul	0.00
20) Perylene-d12	24.02	264	10181m>	0.40	ng/ul	0.00

SJ 10/29/18

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.27	152	1117	0.11	ng/ul	0.00
14) Fluoranthene-d10	19.32	212	3220	0.11	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed