

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_E\DATA\BE102518\  
Quantitation Report (QT Reviewed)


Data File : BE098066.D  
Acq On : 25 Oct 2018 21:41  
Operator : SJ/JU  
Sample : J5568-13  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
C0AK8

Manual Integrations  
APPROVED

Sohil  
10/26/2018 3:47:43 PM

Quant Time: Oct 26 07:01:30 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\SOM-EPA-SIM-BE102518.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 26 05:34:25 2018  
Response via : Initial Calibration

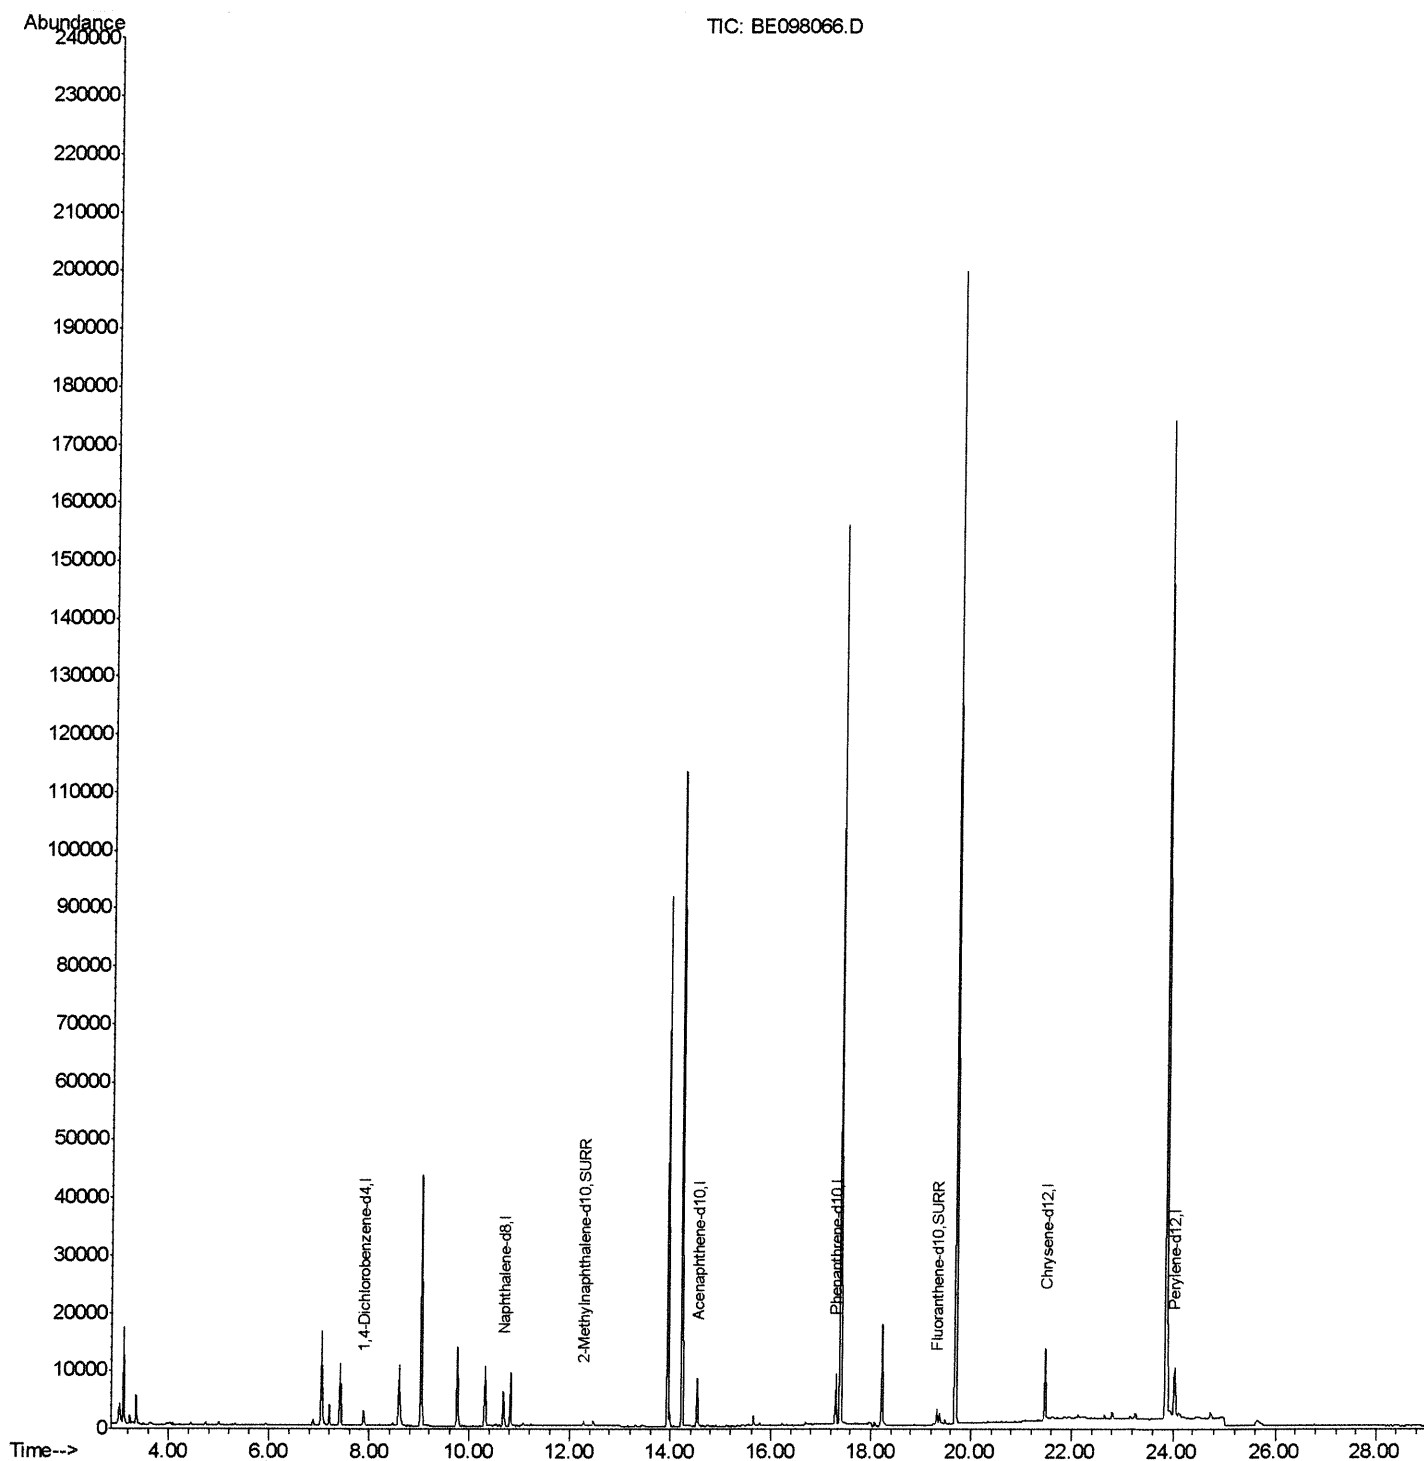

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_E\DATA\BE102518\  
Quantitation Report (Qedit)




Data File : BE098066.D  
Acq On : 25 Oct 2018 21:41  
Operator : SJ/JU  
Sample : J5568-13  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
C0AK8

Manual Integrations  
APPROVED

Sohil  
10/26/2018 3:47:43 PM

Quant Time: Oct 26 05:37:47 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\SOM-EPA-SIM-BE102518.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 26 05:34:25 2018  
Response via : Initial Calibration

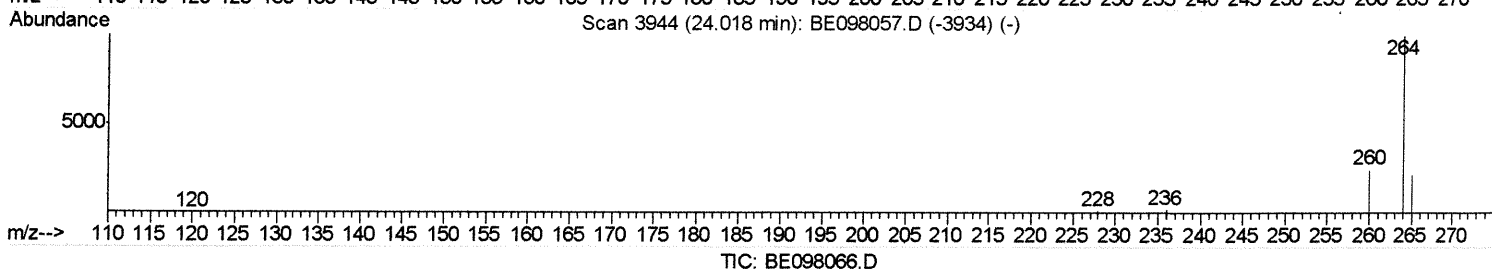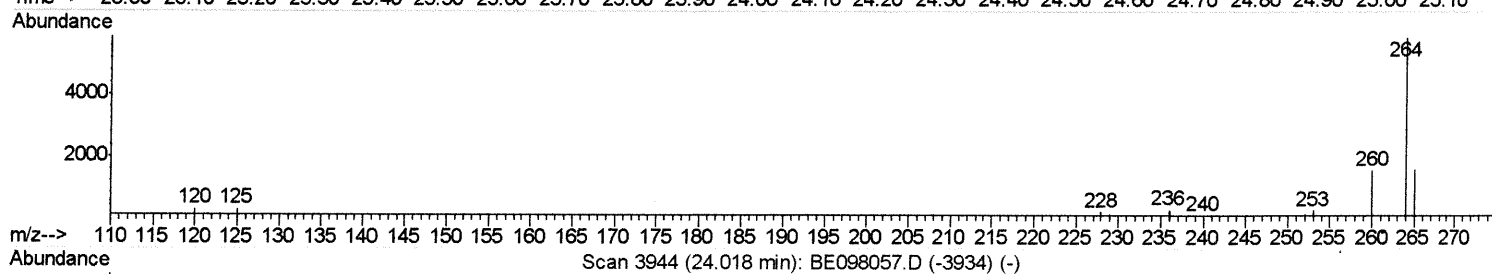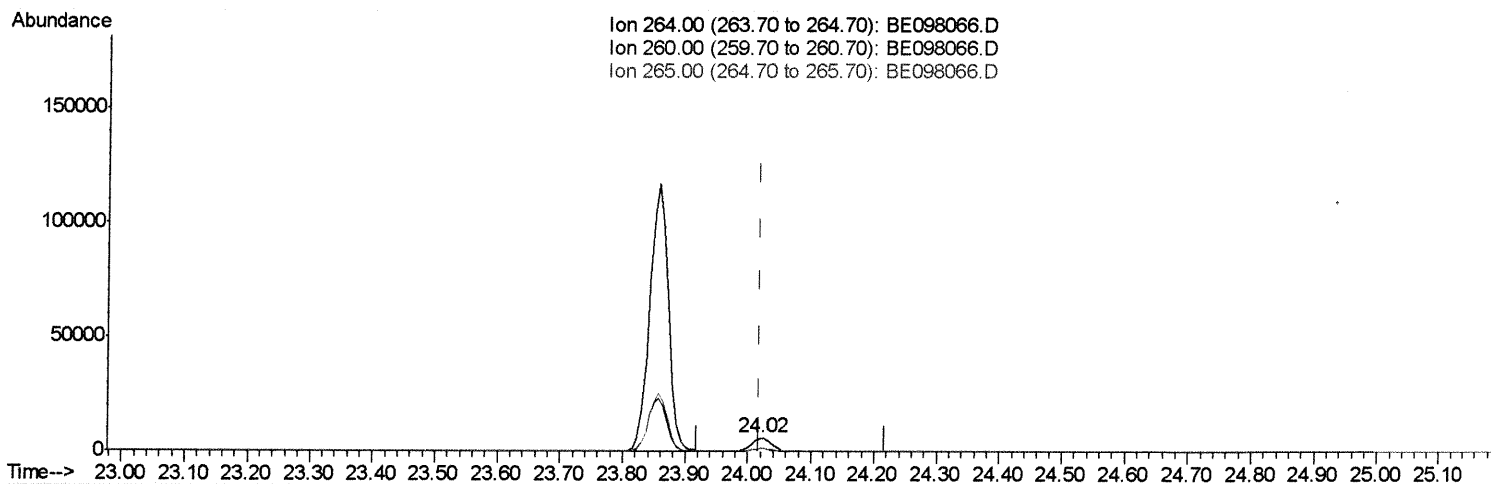

(20) Perylene-d12 (I)

24.019min (+0.001) 0.40ng/ul

response 13215

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 264.00 | 100   | 100   |
| 260.00 | 25.20 | 26.30 |
| 265.00 | 28.00 | 26.81 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_E\DATA\BE102518\  
Quantitation Report (Qedit)




Data File : BE098066.D  
Acq On : 25 Oct 2018 21:41  
Operator : SJ/JU  
Sample : J5568-13  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
C0AK8

Manual Integrations  
APPROVED

Sohil  
10/26/2018 3:47:43 PM

Quant Time: Oct 26 05:37:47 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\SOM-EPA-SIM-BE102518.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 26 05:34:25 2018  
Response via : Initial Calibration

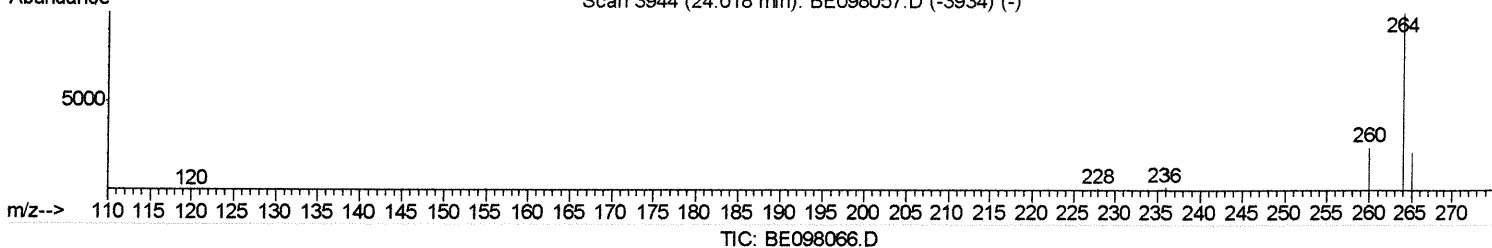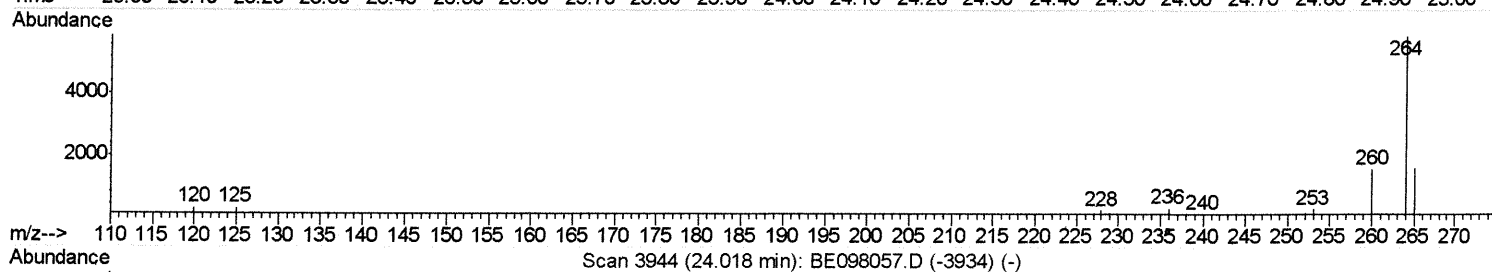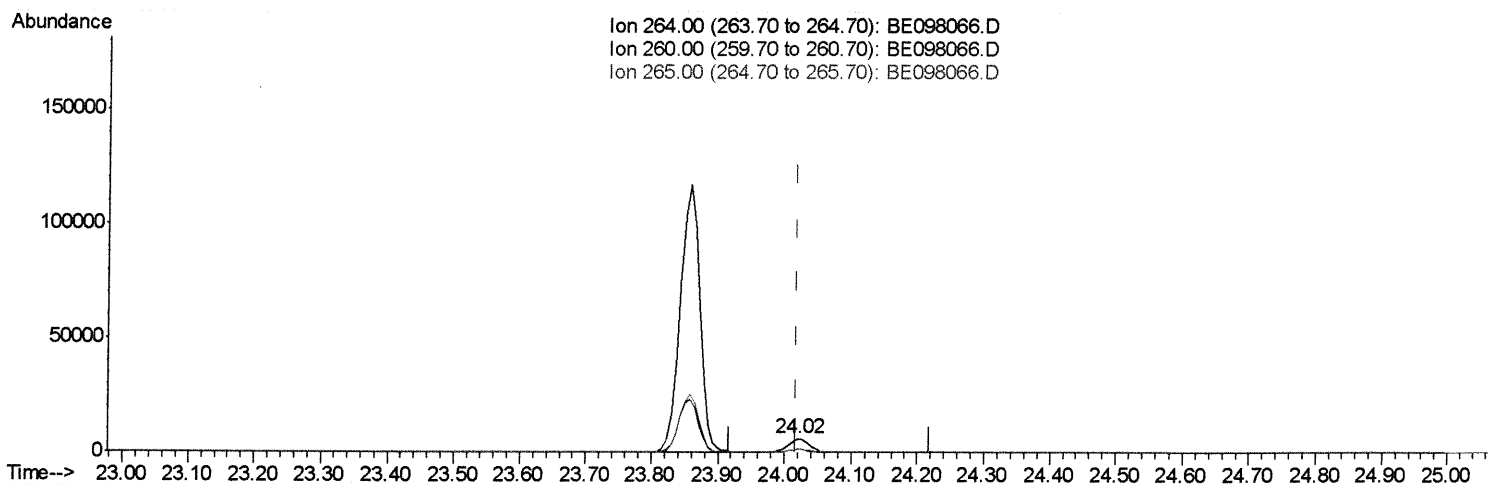

(20) Perylene-d12 (I)

24.019min (+0.001) 0.40ng/ul m) SJ 10/29/18

response 12182

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 264.00 | 100   | 100   |
| 260.00 | 25.20 | 26.30 |
| 265.00 | 28.00 | 26.81 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_E\DATA\BE102518\  
Quantitation Report (QT Reviewed)

Data File : BE098066.D  
Acq On : 25 Oct 2018 21:41  
Operator : SJ/JU  
Sample : J5568-13  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
C0AK8

Manual Integrations  
APPROVED

Sohil  
10/26/2018 3:47:43 PM

Quant Time: Oct 26 07:01:30 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\SOM-EPA-SIM-BE102518.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 26 05:34:25 2018  
Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc | Units | Dev(Min) |
|---------------------------|-------|------|----------|------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.88  | 152  | 1255     | 0.40 | ng/ul | 0.00     |
| 2) Naphthalene-d8         | 10.67 | 136  | 6303     | 0.40 | ng/ul | 0.00     |
| 6) Acenaphthene-d10       | 14.53 | 164  | 4523     | 0.40 | ng/ul | 0.00     |
| 10) Phenanthrene-d10      | 17.29 | 188  | 10753    | 0.40 | ng/ul | 0.00     |
| 16) Chrysene-d12          | 21.47 | 240  | 15175    | 0.40 | ng/ul | 0.00     |
| 20) Perylene-d12          | 24.02 | 264  | 12182m   | 0.40 | ng/ul | 0.00     |

SD 10/29/18

System Monitoring Compounds

|                            |       |     |      |      |       |      |
|----------------------------|-------|-----|------|------|-------|------|
| 4) 2-Methylnaphthalene-d10 | 12.27 | 152 | 1185 | 0.11 | ng/ul | 0.00 |
| 14) Fluoranthene-d10       | 19.32 | 212 | 3161 | 0.09 | ng/ul | 0.00 |

| Target Compounds | Qvalue |
|------------------|--------|
|------------------|--------|

(#) = qualifier out of range (m) = manual integration (+) = signals summed