

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102518\
Quantitation Report (QT Reviewed)


Data File : BE098069.D
Acq On : 25 Oct 2018 23:31
Operator : SJ/JU
Sample : J5568-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AK5

Manual Integrations
APPROVED

Sohil
10/26/2018 3:47:46 PM

Quant Time: Oct 26 07:20:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 26 05:34:25 2018
Response via : Initial Calibration

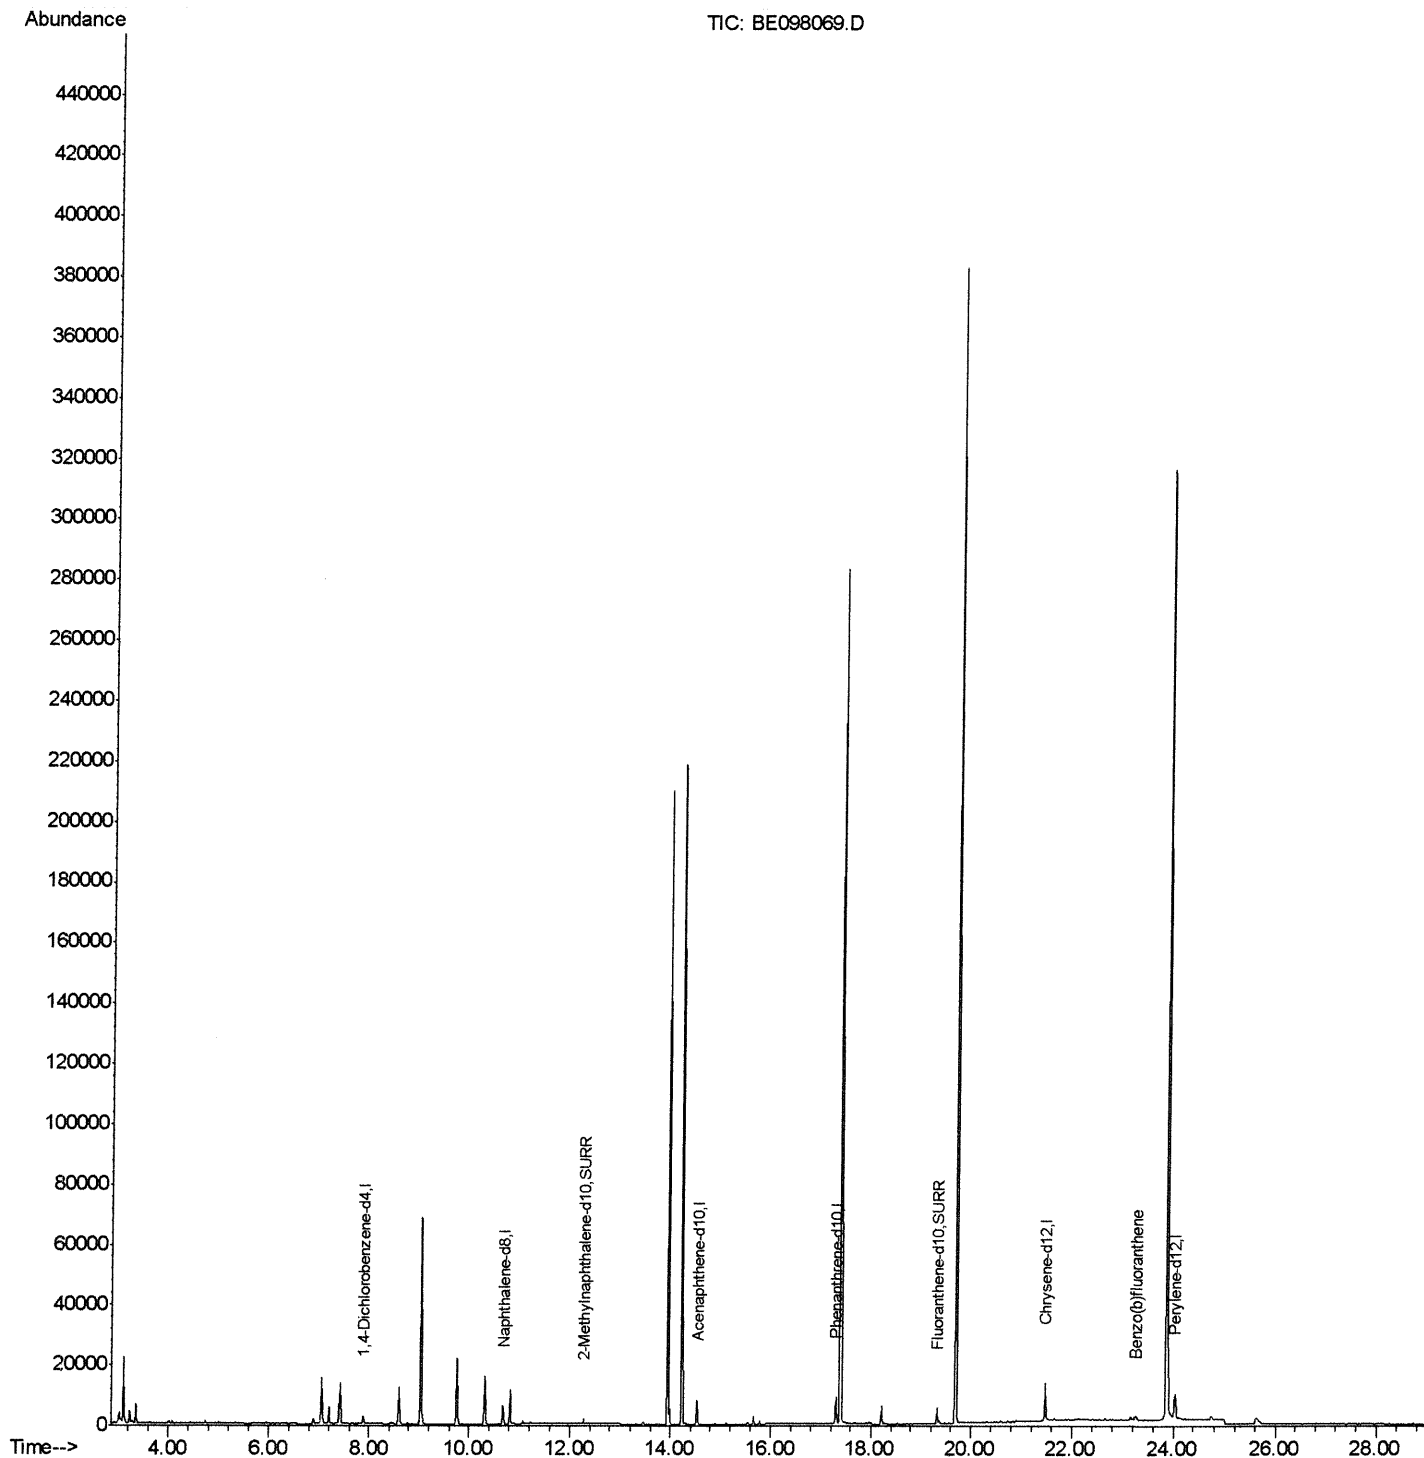

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102518\
Quantitation Report (Qedit)



Data File : BE098069.D
Acq On : 25 Oct 2018 23:31
Operator : SJ/JU
Sample : J5568-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AK5

Manual Integrations
APPROVED

Sohil
10/26/2018 3:47:46 PM

Quant Time: Oct 26 05:38:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 26 05:34:25 2018
Response via : Initial Calibration

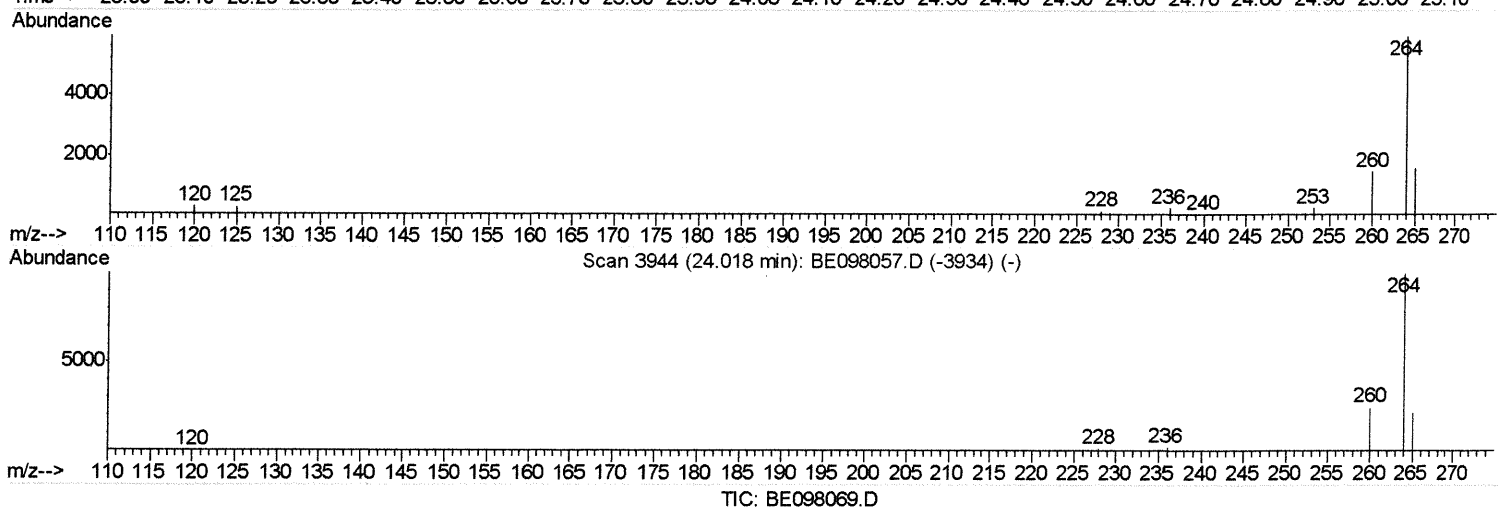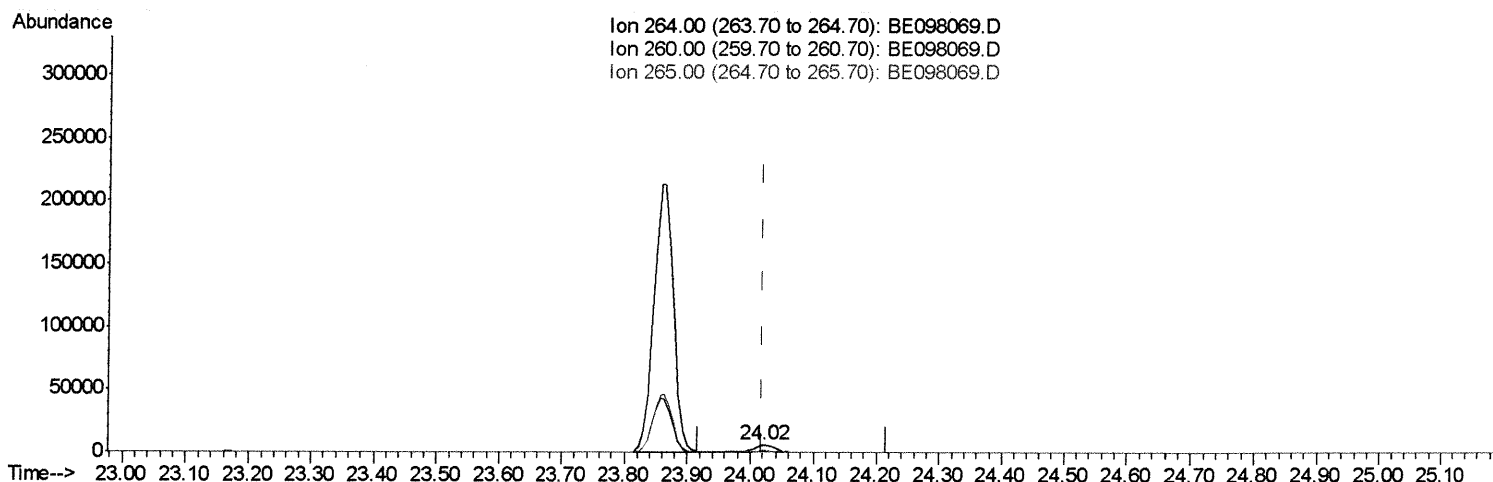

(20) Perylene-d12 (I)

24.018min (-0.000) 0.40ng/ul

response 13721

Ion	Exp%	Act%
264.00	100	100
260.00	25.20	25.24
265.00	28.00	27.64
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102518\
Quantitation Report (Qedit)




Data File : BE098069.D
Acq On : 25 Oct 2018 23:31
Operator : SJ/JU
Sample : J5568-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AK5

Manual Integrations
APPROVED

Sohil
10/26/2018 3:47:46 PM

Quant Time: Oct 26 05:38:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 26 05:34:25 2018
Response via : Initial Calibration

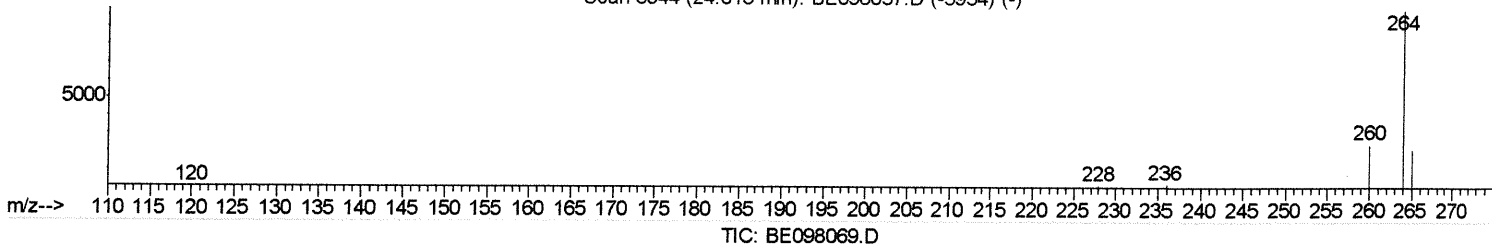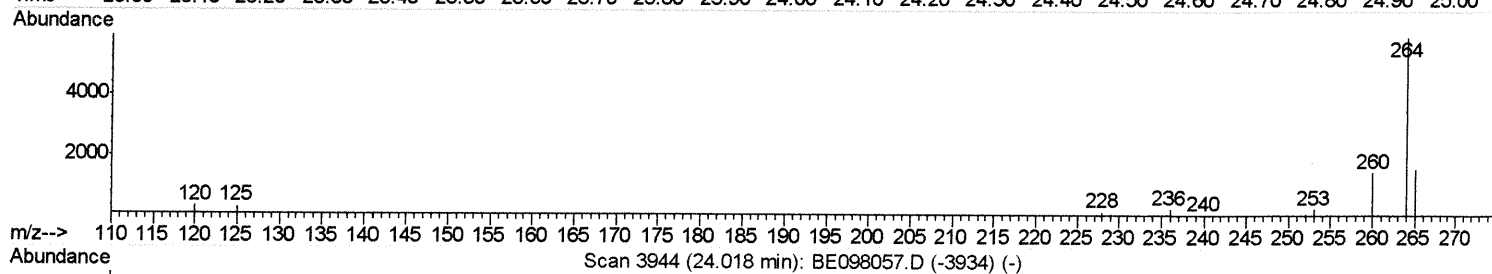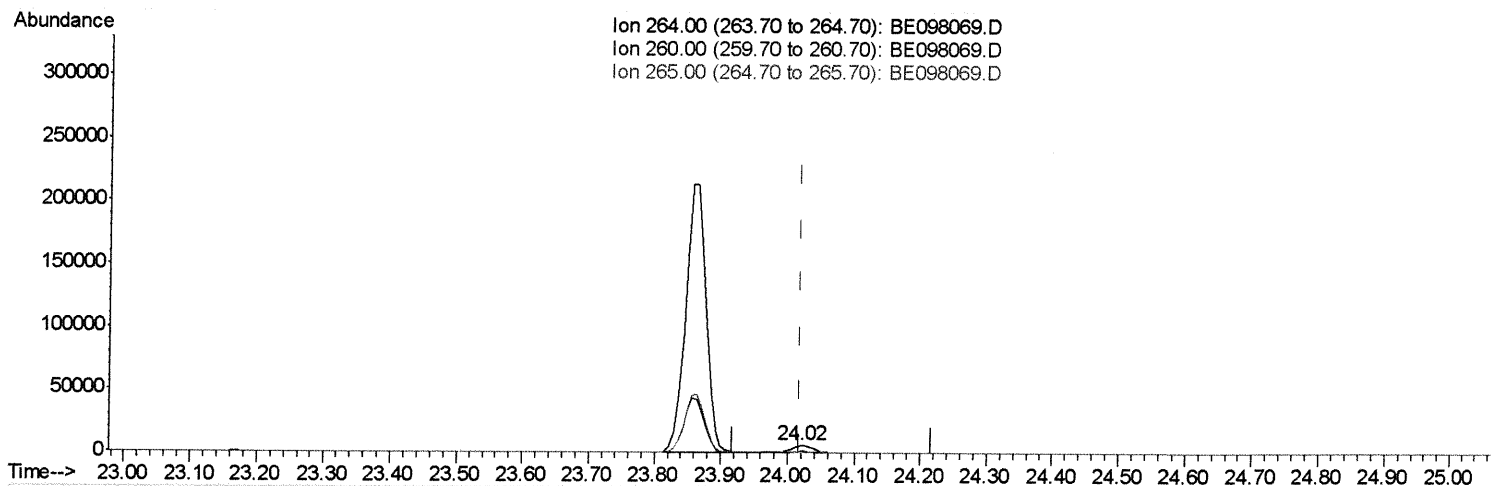

(20) Perylene-d12 (I)

24.018min (-0.000) 0.40ng/ul m> SJ 10/24/18

response 11841

Ion	Exp%	Act%
264.00	100	100
260.00	25.20	25.24
265.00	28.00	27.64
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102518\
Quantitation Report (Qedit)




Data File : BE098069.D
Acq On : 25 Oct 2018 23:31
Operator : SJ/JU
Sample : J5568-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AK5

Manual Integrations
APPROVED

Sohil
10/26/2018 3:47:46 PM

Quant Time: Oct 26 07:17:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 26 05:34:25 2018
Response via : Initial Calibration

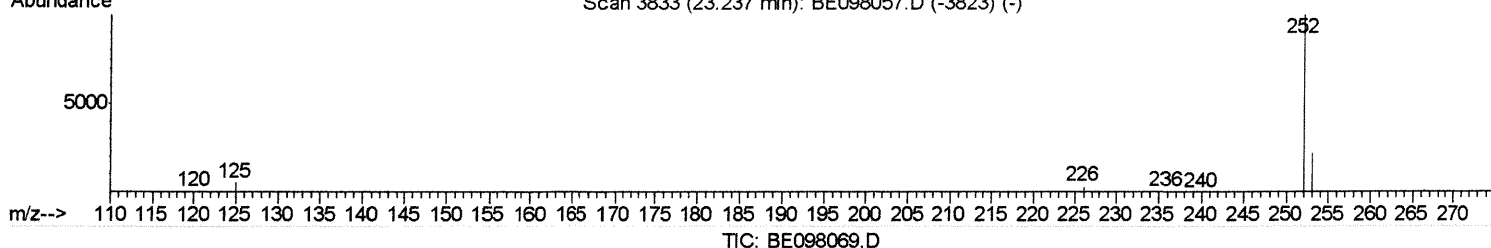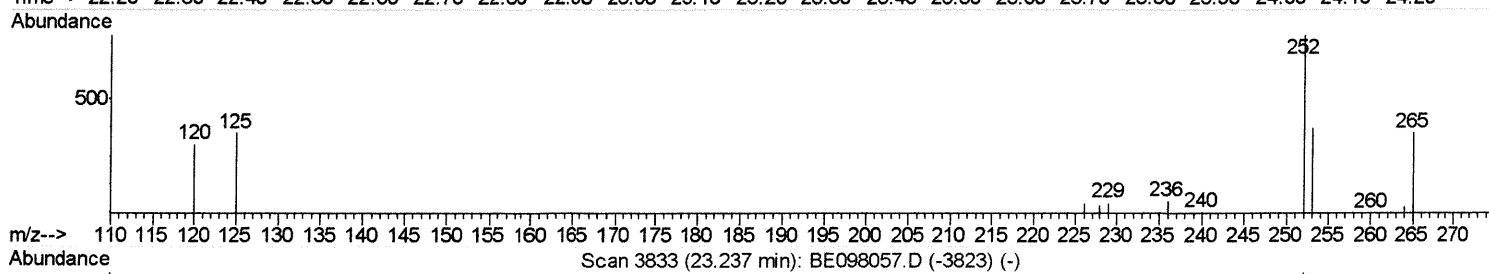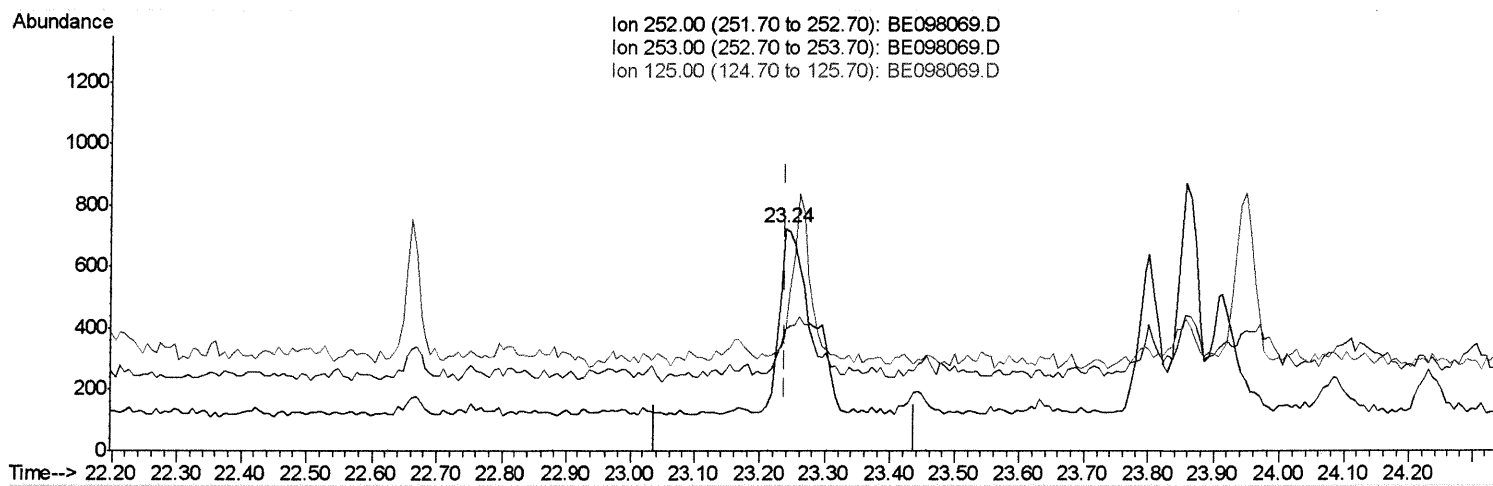

(21) Benzo(b)fluoranthene

23.237min (-0.000) 0.06ng/ul

response 2086

Ion	Exp%	Act%
252.00	100	100
253.00	23.90	54.62#
125.00	8.40	52.28#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102518\
Quantitation Report (Qedit)




Data File : BE098069.D
Acq On : 25 Oct 2018 23:31
Operator : SJ/JU
Sample : J5568-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AK5

Manual Integrations
APPROVED

Sohil
10/26/2018 3:47:46 PM

Quant Time: Oct 26 07:17:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 26 05:34:25 2018
Response via : Initial Calibration

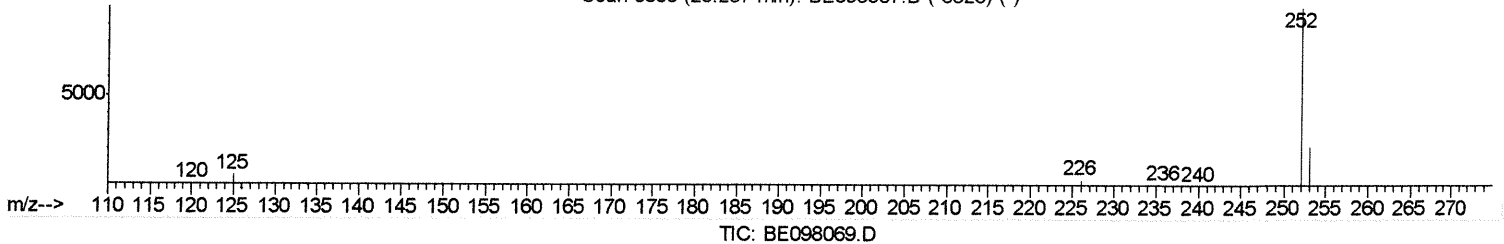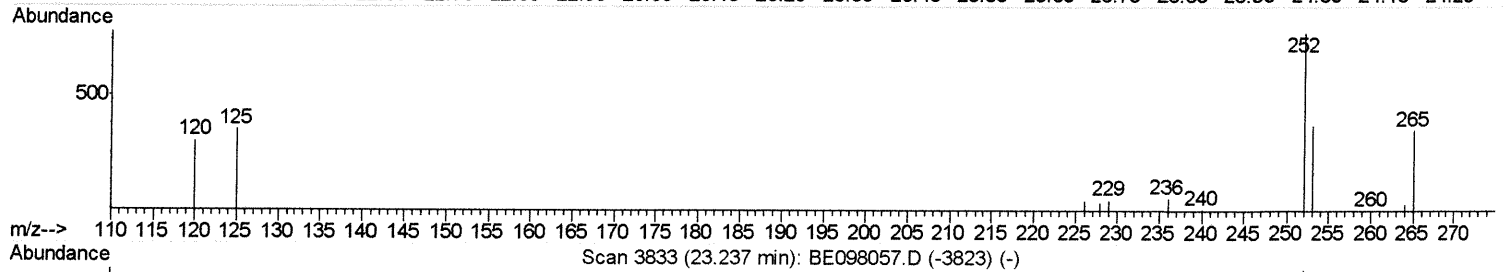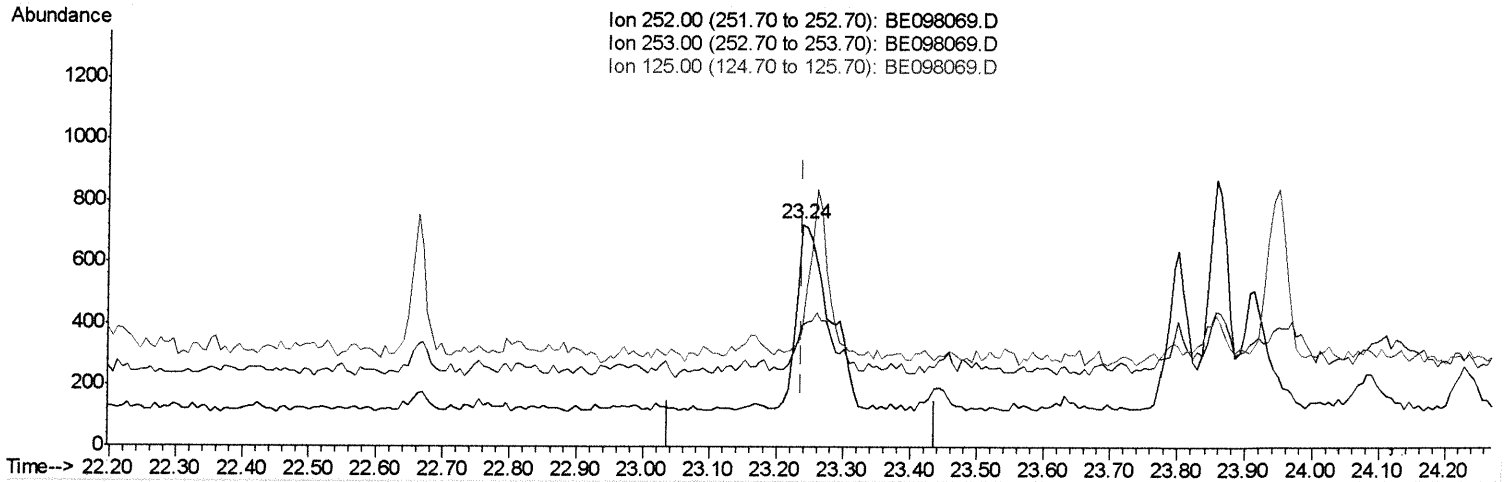

(21) Benzo(b)fluoranthene

23.237min (-0.000) 0.05ng/ul m> SA 10/24/18

response 1545

Ion	Exp%	Act%
252.00	100	100
253.00	23.90	54.62#
125.00	8.40	52.28#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102518\
 Quantitation Report (QT Reviewed)
 Data File : BE098069.D
 Acq On : 25 Oct 2018 23:31
 Operator : SJ/JU
 Sample : J5568-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AK5

Manual Integrations
 APPROVED

Sohil
 10/26/2018 3:47:46 PM

Quant Time: Oct 26 07:20:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 26 05:34:25 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	1335	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	6541	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	4599	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.29	188	10763	0.40	ng/ul	0.00
16) Chrysene-d12	21.47	240	14405	0.40	ng/ul	0.00
20) Perylene-d12	24.02	264	11841m>	0.40	ng/ul	0.00

SJ 10/29/18

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.27	152	2042	0.18	ng/ul	0.00
14) Fluoranthene-d10	19.32	212	5937	0.17	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
21) Benzo(b)fluoranthene	23.24	252	1545m>	0.047	ng/ul	

SJ 10/29/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed