

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102518\
Quantitation Report (QT Reviewed)


Data File : BE098075.D
Acq On : 26 Oct 2018 3:12
Operator : SJ/JU
Sample : J5567-21
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AJ7

Manual Integrations
APPROVED

Sohil
10/26/2018 3:47:52 PM

Quant Time: Oct 26 08:07:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 26 07:43:08 2018
Response via : Initial Calibration

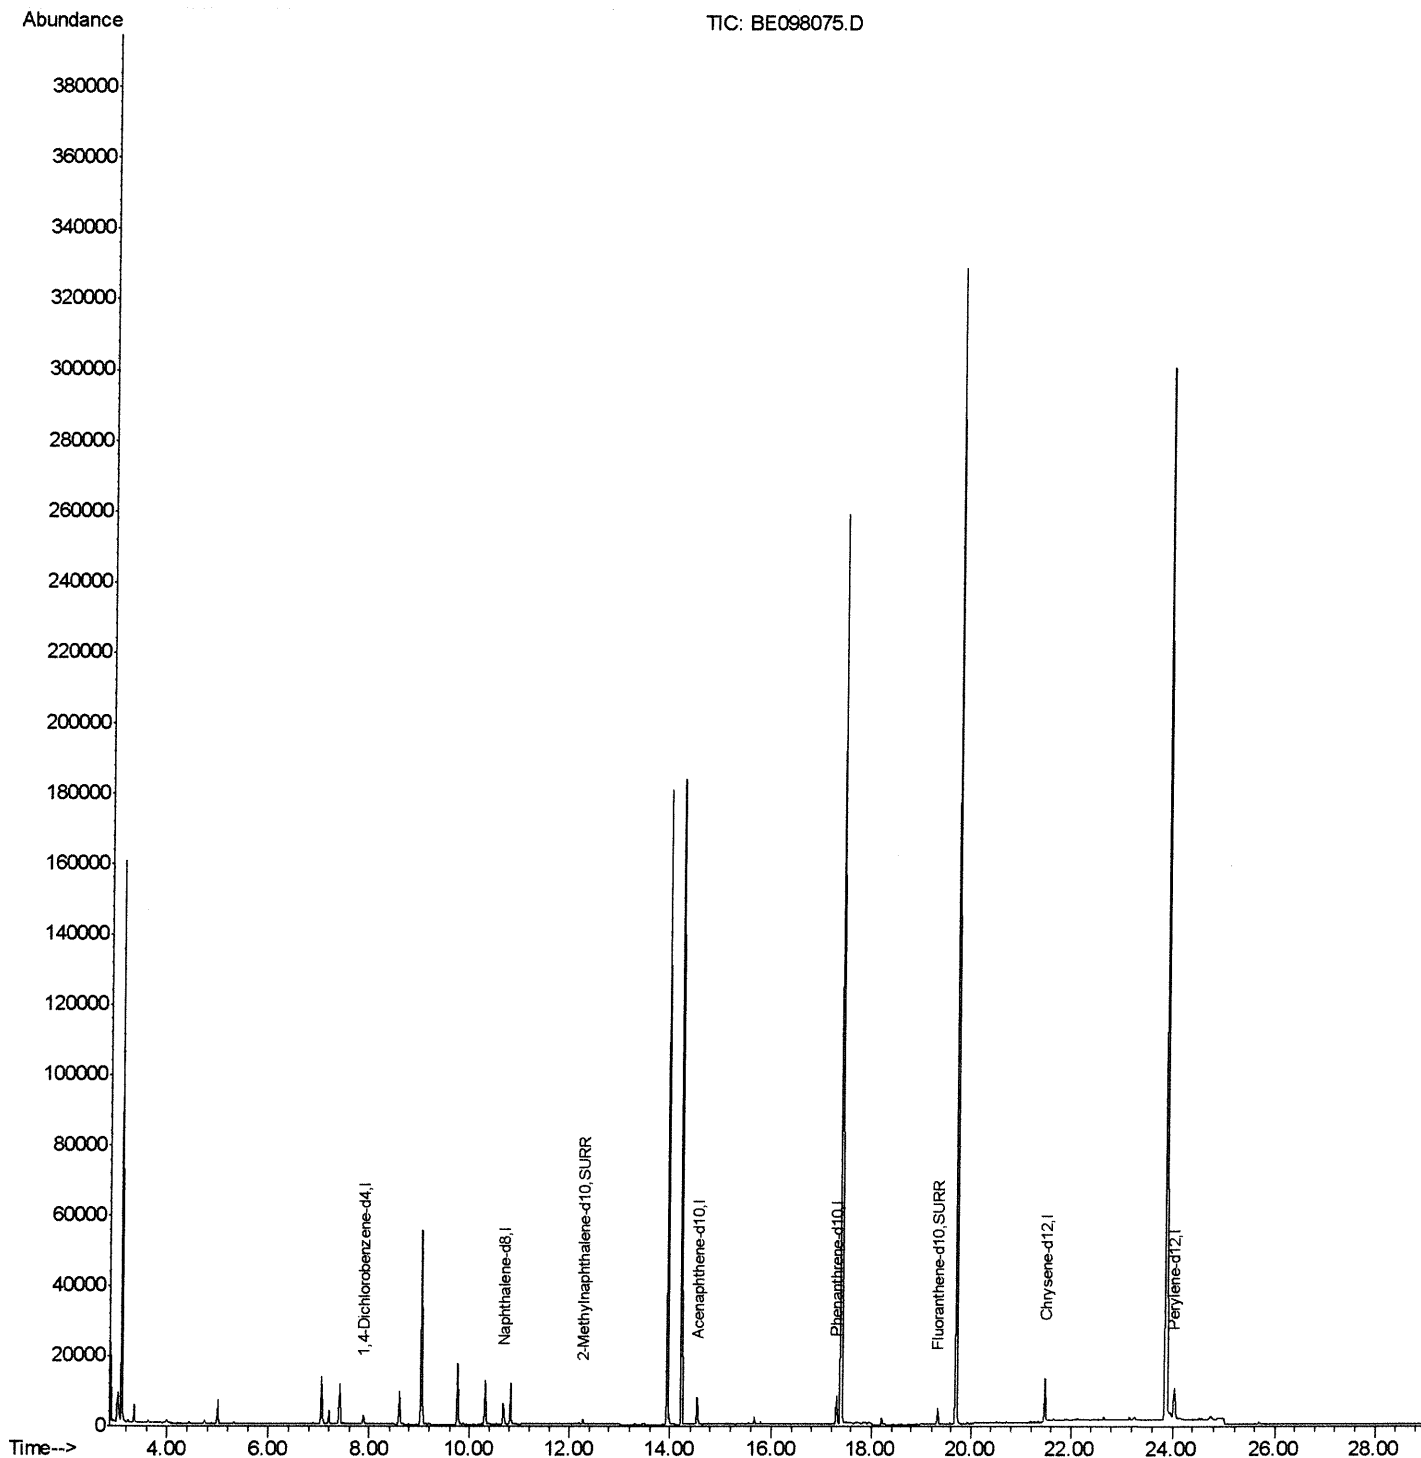

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102518\
Quantitation Report (Qedit)



Data File : BE098075.D
Acq On : 26 Oct 2018 3:12
Operator : SJ/JU
Sample : J5567-21
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AJ7

Manual Integrations
APPROVED

Sohil
10/26/2018 3:47:52 PM

Quant Time: Oct 26 07:45:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 26 07:43:08 2018
Response via : Initial Calibration

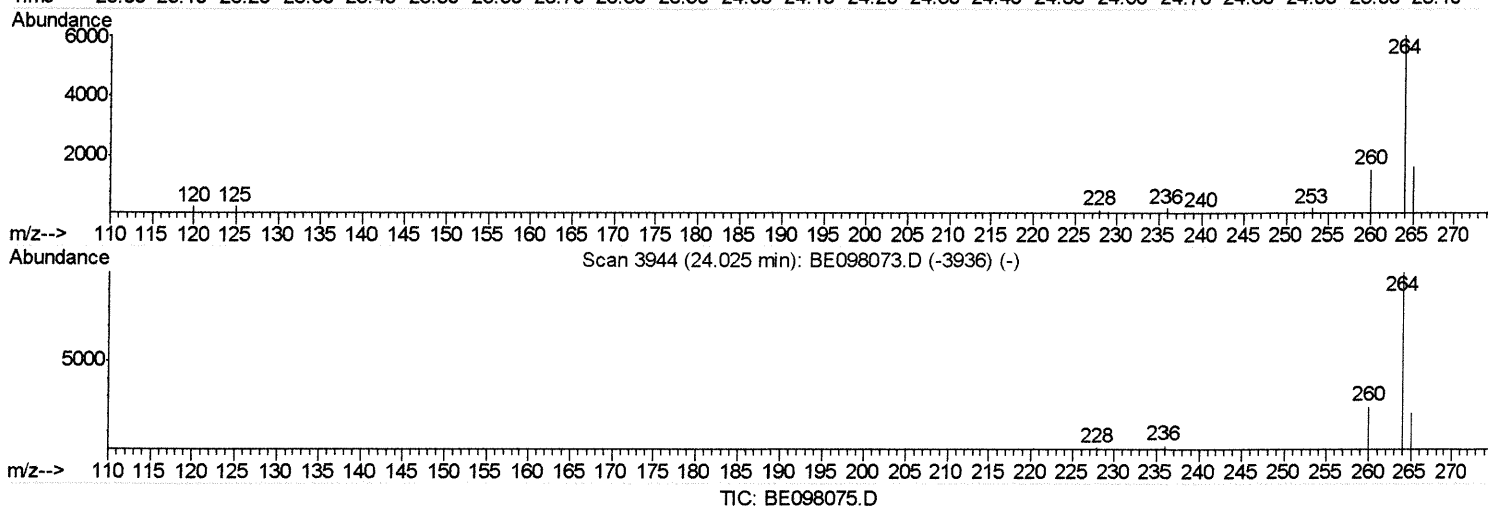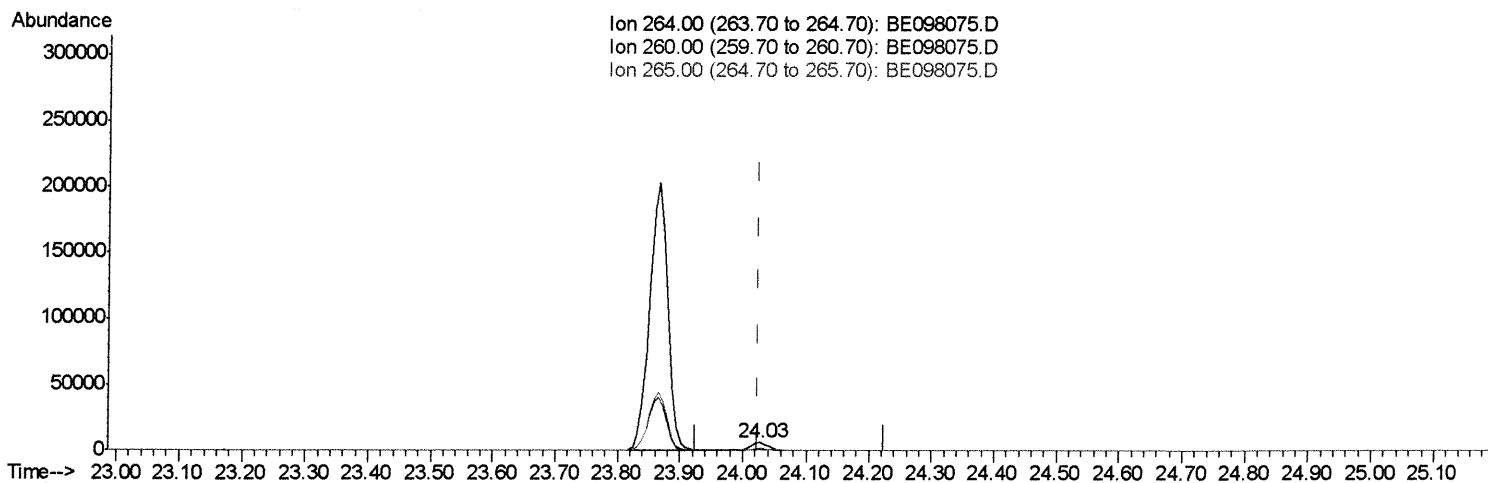

(20) Perylene-d12 (I)

24.027min (+0.002) 0.40ng/ul

response 13138

Ion	Exp%	Act%
264.00	100	100
260.00	25.20	25.38
265.00	28.00	27.26
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102518\
Quantitation Report (Qedit)




Data File : BE098075.D
Acq On : 26 Oct 2018 3:12
Operator : SJ/JU
Sample : J5567-21
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AJ7

Manual Integrations
APPROVED

Sohil
10/26/2018 3:47:52 PM

Quant Time: Oct 26 07:45:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 26 07:43:08 2018
Response via : Initial Calibration

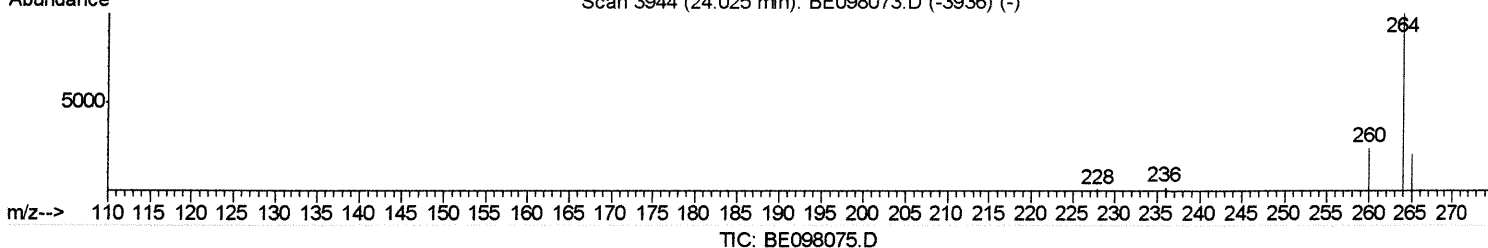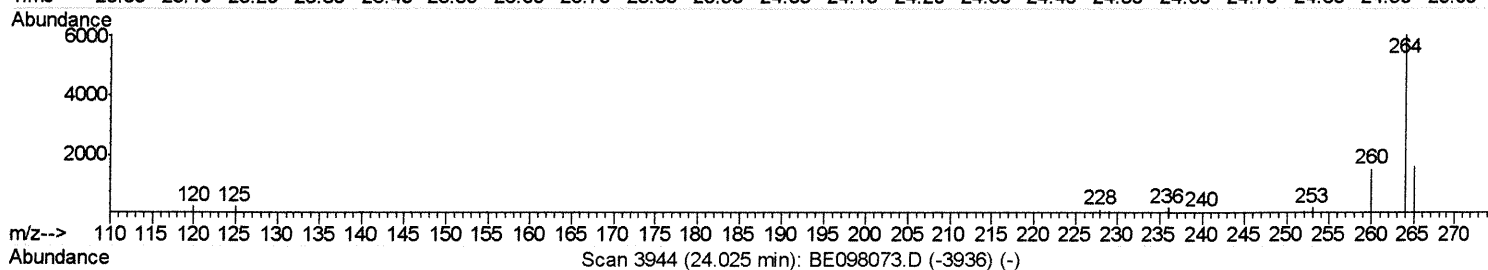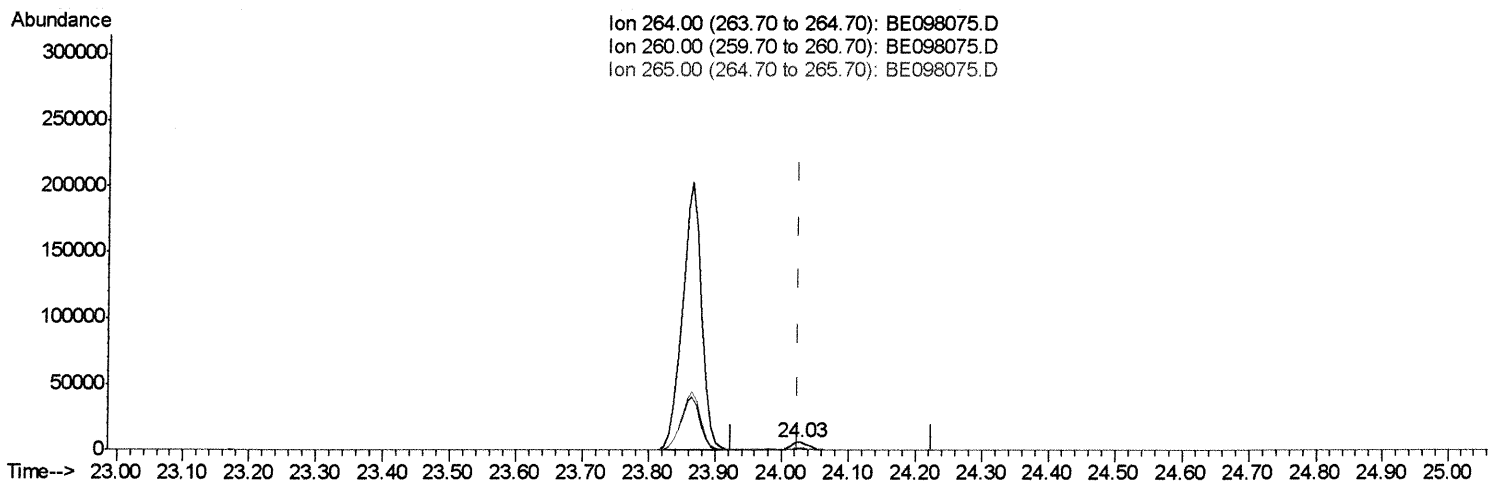

(20) Perylene-d12 (I)

24.027min (+0.002) 0.40ng/ul m > SJ 10/24/18

response 11310

Ion	Exp%	Act%
264.00	100	100
260.00	25.20	25.38
265.00	28.00	27.26
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102518\
Quantitation Report (QT Reviewed)

Data File : BE098075.D
Acq On : 26 Oct 2018 3:12
Operator : SJ/JU
Sample : J5567-21
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AJ7

Manual Integrations
APPROVED

Sohil
10/26/2018 3:47:52 PM

Quant Time: Oct 26 08:07:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 26 07:43:08 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.87	152	1269	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	6316	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.54	164	4478	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.30	188	10480	0.40	ng/ul	0.00
16) Chrysene-d12	21.47	240	14361	0.40	ng/ul	0.00
20) Perylene-d12	24.03	264	11310m	0.40	ng/ul	0.00

SJ 10/29/18

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.27	152	1641	0.15	ng/ul	0.00
14) Fluoranthene-d10	19.32	212	5378	0.16	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed