

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102518\
 Data File : BE098067.D
 Acq On : 25 Oct 2018 22:17
 Operator : SJ/JU
 Sample : J5568-11
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AK6

Manual Integrations
 APPROVED

Sohil
 10/26/2018 3:47:45 PM

Quant Time: Oct 26 07:09:01 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 26 05:34:25 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.87	152	1197	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	6149	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	4517	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.29	188	10508m	0.40	ng/ul	0.00
16) Chrysene-d12	21.47	240	11450m	0.40	ng/ul	0.00
20) Perylene-d12	24.02	264	10624m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.27	152	2709	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.32	212	8176m	0.24	ng/ul	0.00
Target Compounds						
21) Benzo(b)fluoranthene	23.24	252	1502m	0.051	ng/ul	Qvalue
23) Benzo(a)pyrene	23.91	252	973m	0.034	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102518\
Data File : BE098067.D
Acq On : 25 Oct 2018 22:17
Operator : SJ/JU
Sample : J5568-11
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
C0AK6

Manual Integrations
APPROVED

Sohil
10/26/2018 3:47:45 PM

Quant Time: Oct 26 07:09:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 26 05:34:25 2018
Response via : Initial Calibration

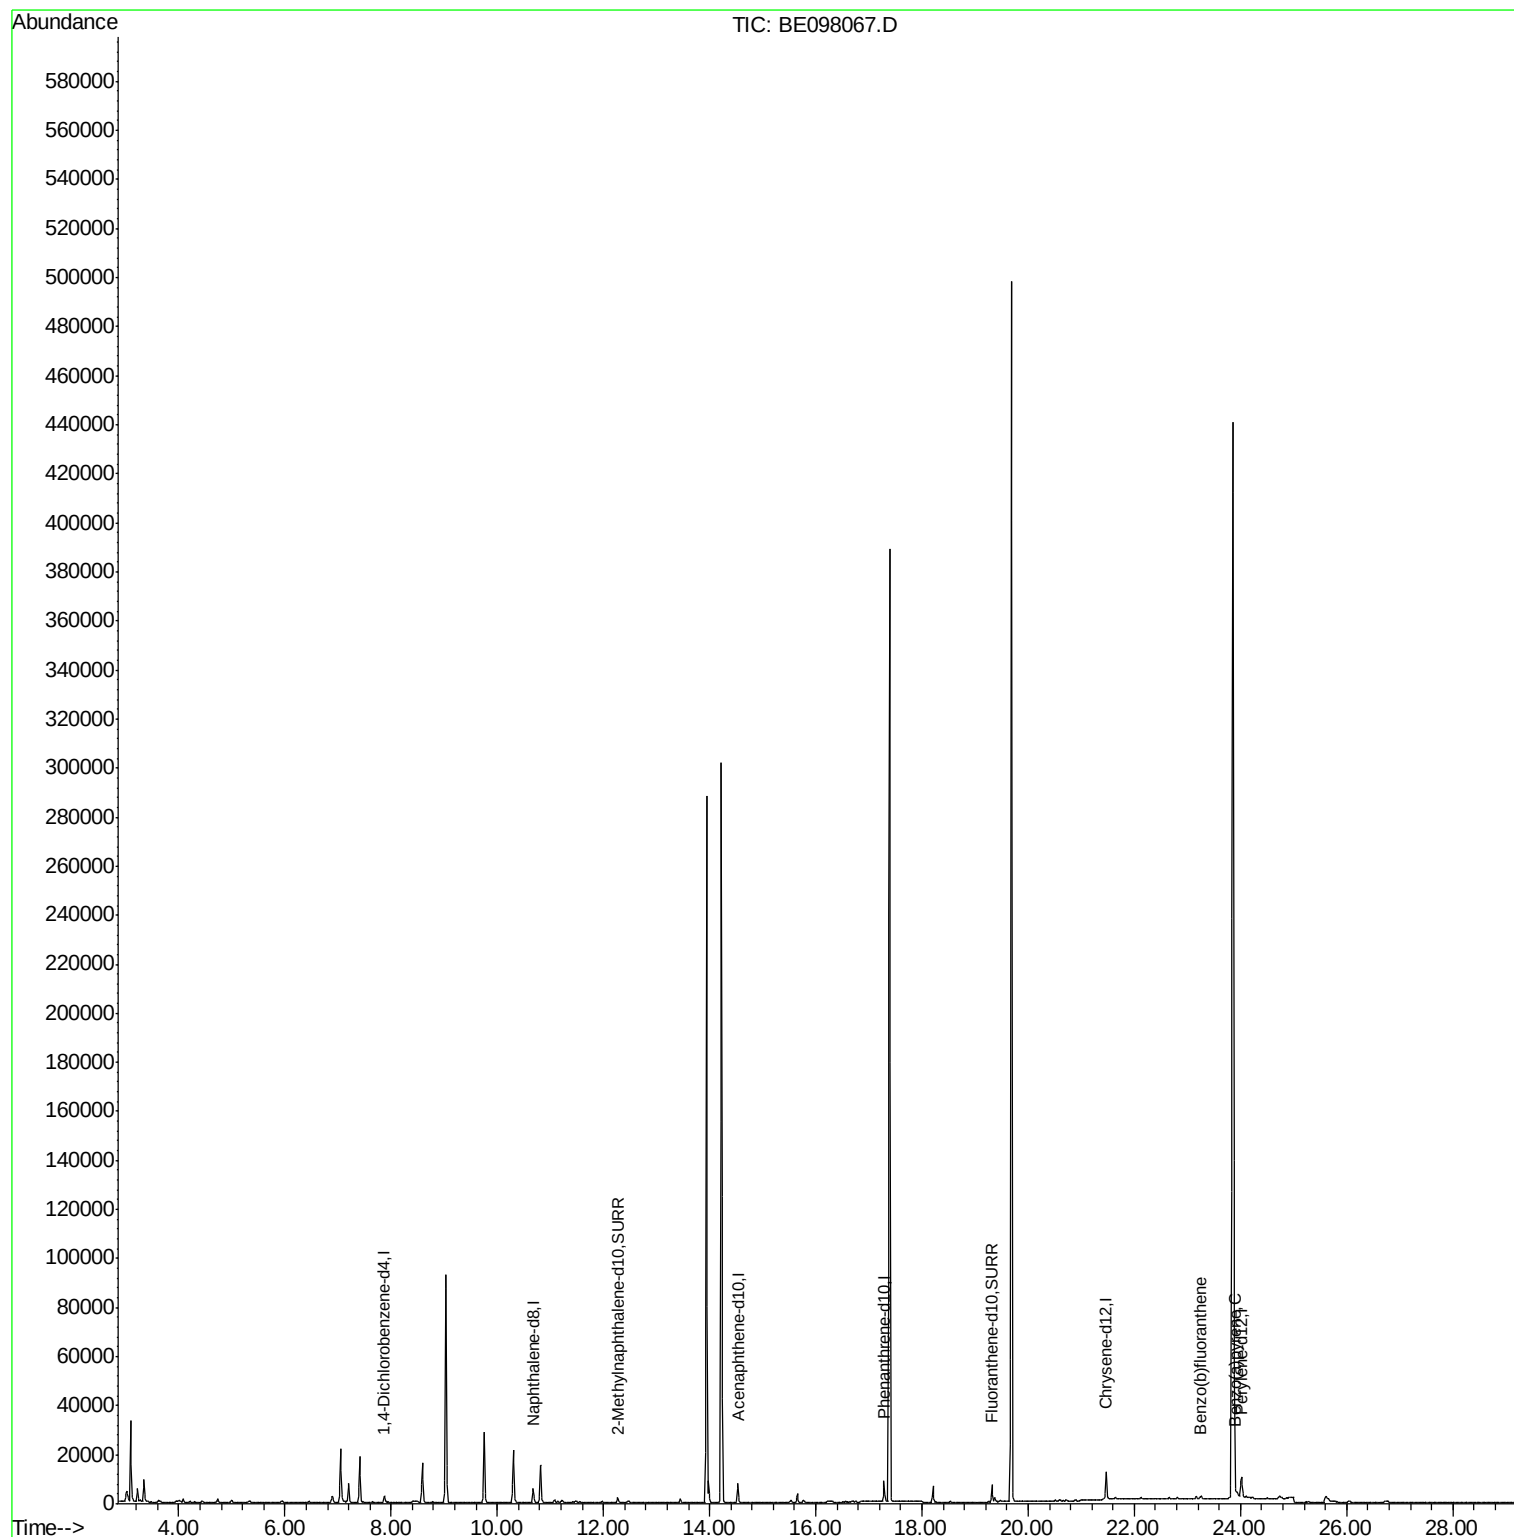

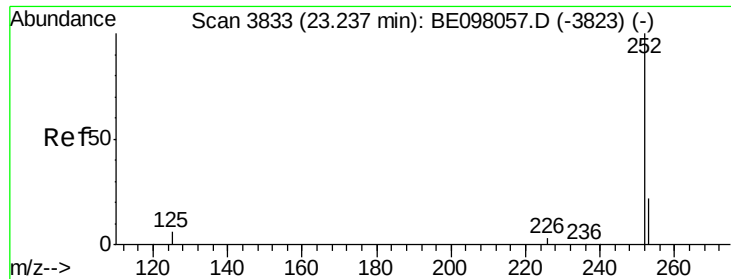





#21
Benzo(b)fluoranthene
Concen: 0.051 ng/ul m
RT: 23.24 min Scan# 3831
Delta R.T. 0.00 min
Lab File: BE098067.D
Acq: 25 Oct 2018 22:17

Instrument :
BNA_E
ClientSampled :
C0AK6

Tgt Ion	Ratio	Lower	Upper
252	100		
253	51.0	0.0	47.8#
125	68.7	0.0	16.8#

Manual Integrations
APPROVED

Sohil
10/26/2018 3:47:45 PM

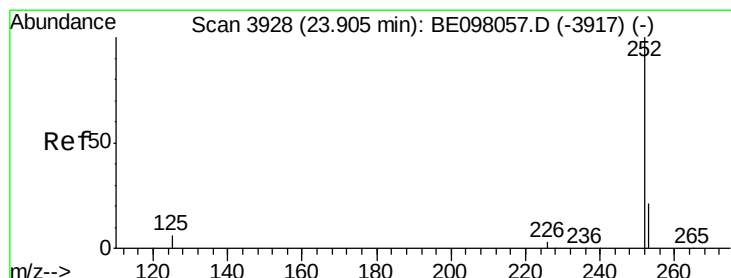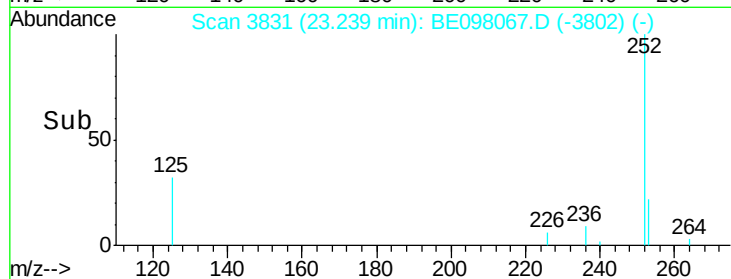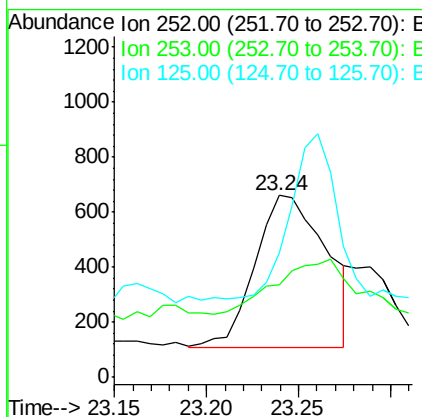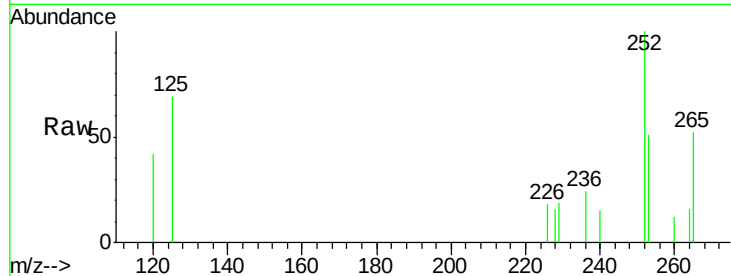

#23
Benzo(a)pyrene
Concen: 0.034 ng/ul m
RT: 23.91 min Scan# 3927
Delta R.T. 0.01 min
Lab File: BE098067.D
Acq: 25 Oct 2018 22:17

Tgt Ion	Ratio	Lower	Upper
252	100		
253	57.3	19.4	29.2#
125	65.3	7.8	11.8#

