

Data File : BE098102.D
Acq On : 26 Oct 2018 23:26
Operator : SJ/JU
Sample : J5568-02RE
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AJ9RE

Quant Time: Oct 27 00:38:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 27 00:33:42 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.87	152	1116	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	5651	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	4071	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.29	188	9831	0.40	ng/ul	0.00
16) Chrysene-d12	21.47	240	12786	0.40	ng/ul	0.00
20) Perylene-d12	24.02	264	11813	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.27	152	1063	0.11	ng/ul	0.00
14) Fluoranthene-d10	19.32	212	3032	0.09	ng/ul	0.00
Target Compounds						
21) Benzo(b)fluoranthene	23.24	252	1134	0.035	ng/ul#	10
22) Benzo(k)fluoranthene	23.24	252	1118	0.035	ng/ul#	11


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BE098102.D
Acq On : 26 Oct 2018 23:26
Operator : SJ/JU
Sample : J5568-02RE
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AJ9RE

Quant Time: Oct 27 00:38:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 27 00:33:42 2018
Response via : Initial Calibration

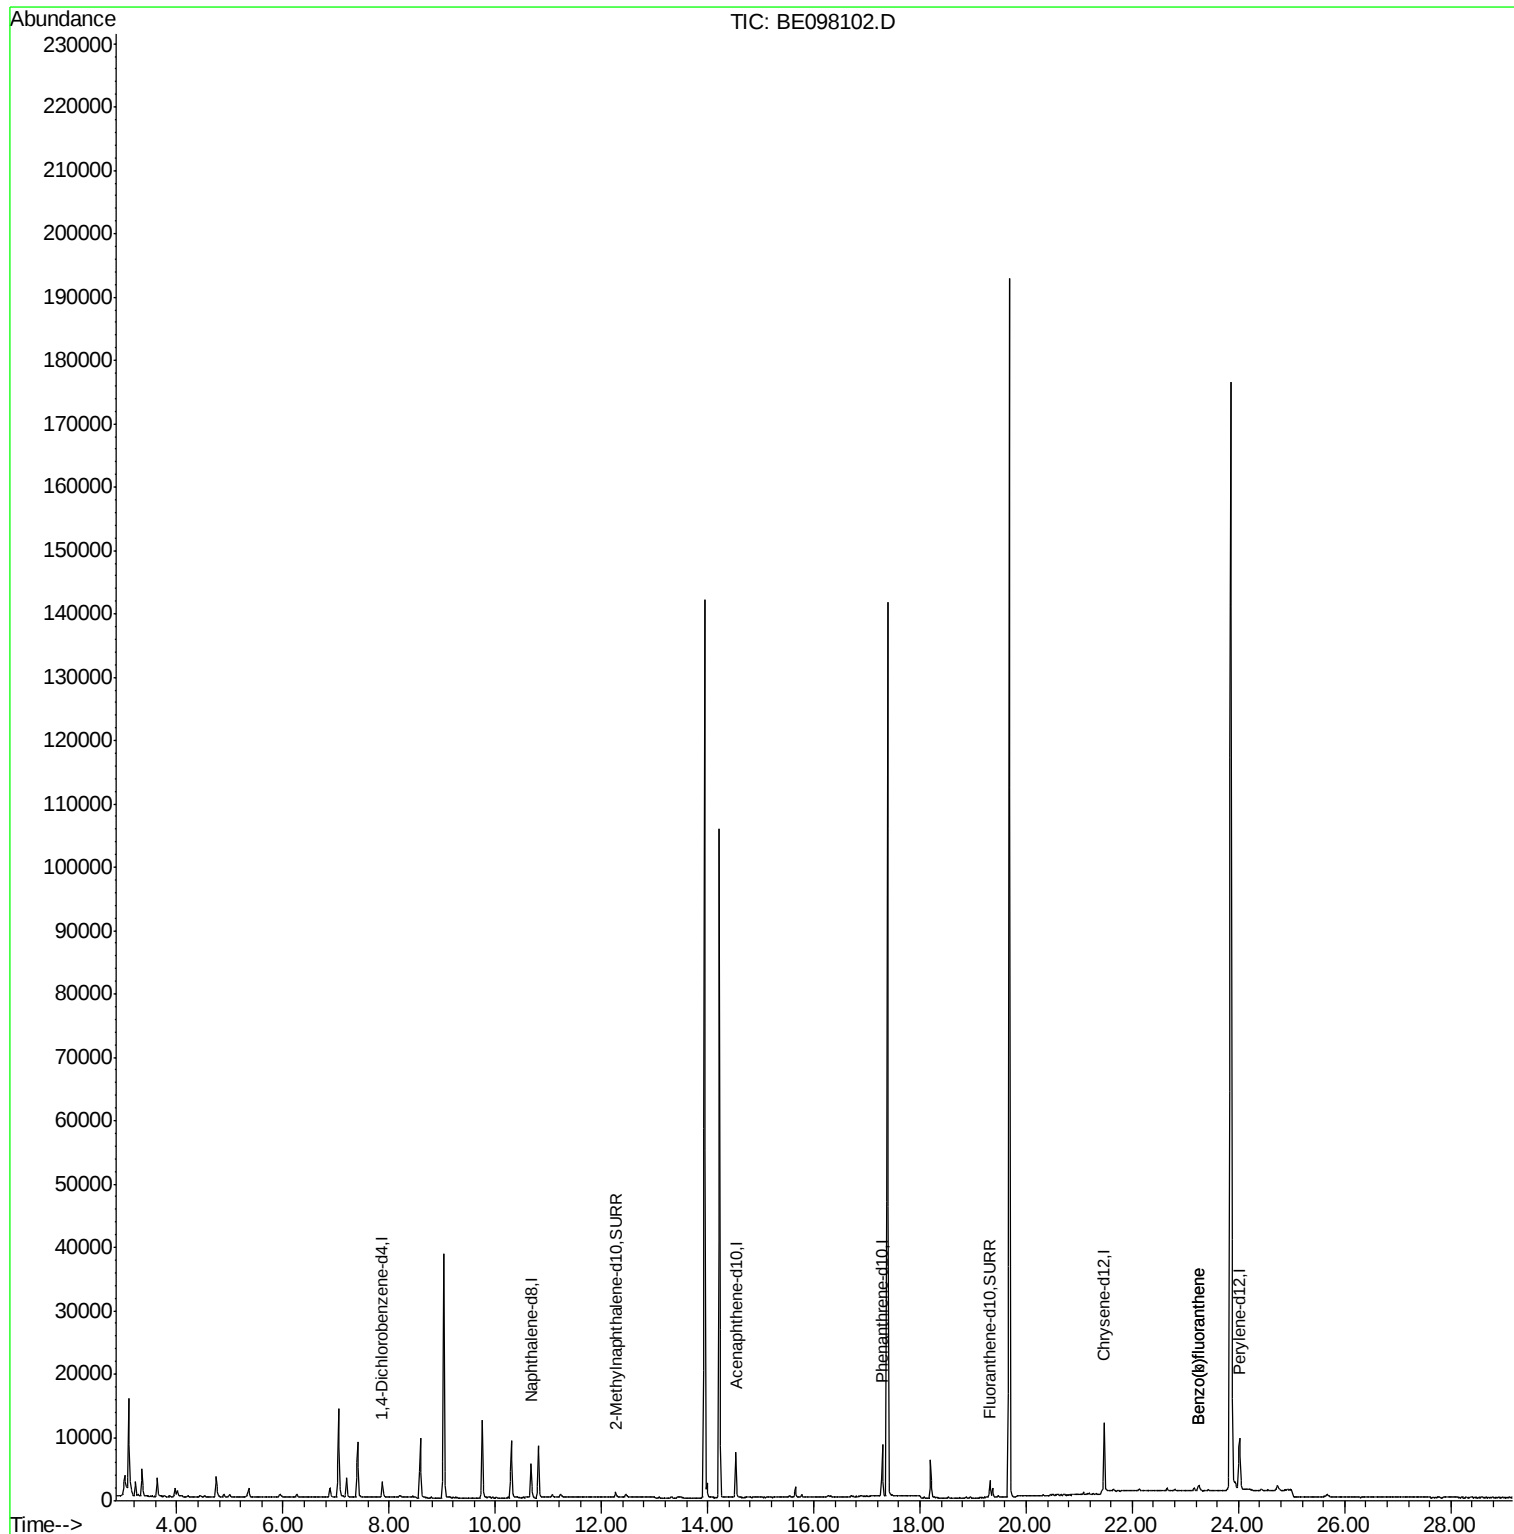

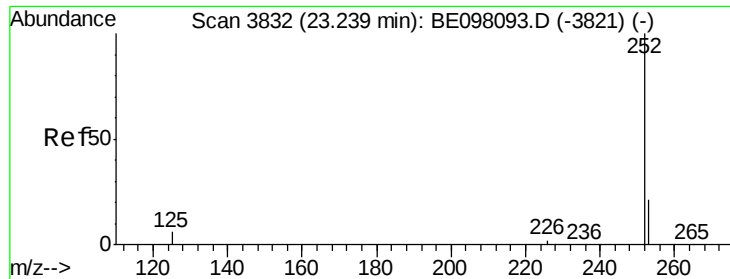

#21

Benzo(b)fluoranthene

Concen: 0.035 ng/ul

RT: 23.24 min Scan# 3832

Delta R.T. -0.00 min

Lab File: BE098102.D

Acq: 26 Oct 2018 23:26

Instrument :

BNA_E

ClientSampleId :

C0AJ9RE


Tgt Ion:252 Resp: 1134

Ion Ratio Lower Upper

252 100

253 56.2 0.0 47.8#




125 64.6 0.0 16.8#

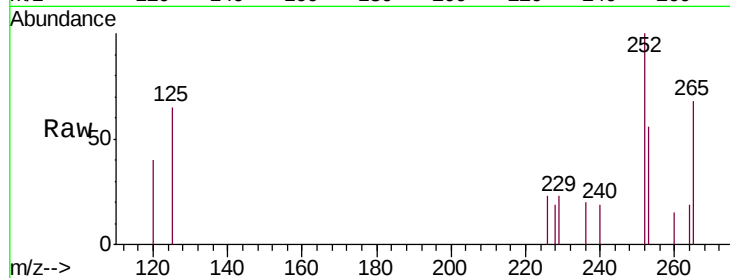

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

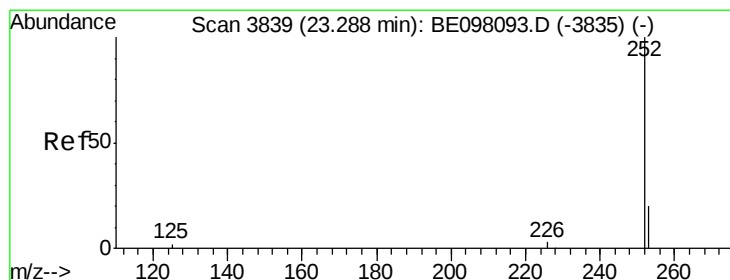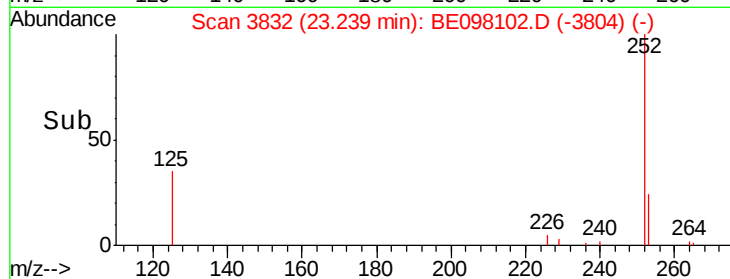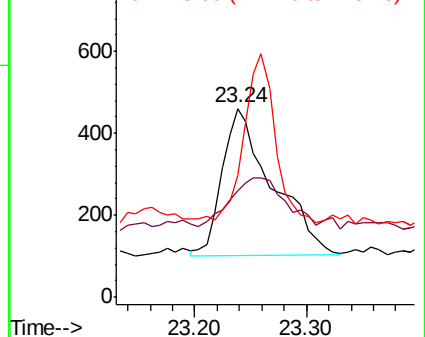

#22

Benzo(k)fluoranthene

Concen: 0.035 ng/ul

RT: 23.24 min Scan# 3832

Delta R.T. -0.05 min

Lab File: BE098102.D

Acq: 26 Oct 2018 23:26


Tgt Ion:252 Resp: 1118

Ion Ratio Lower Upper

252 100

253 56.2 19.3 28.9#

125 64.6 6.2 9.2#

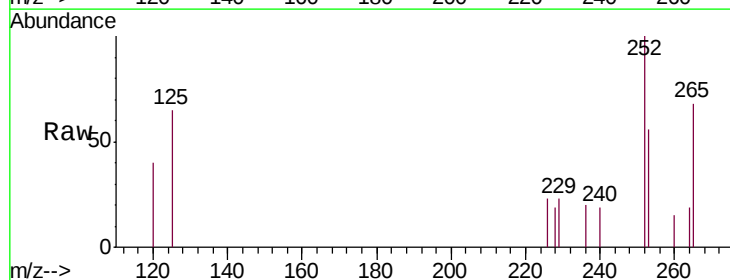

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

