

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102618\
Quantitation Report (Not Reviewed)

Data File : BE098105.D
Acq On : 27 Oct 2018 1:16
Operator : SJ/JU
Sample : J5568-13RE
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AK8RE

Quant Time: Oct 27 04:04:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 27 00:33:42 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.87	152	1136	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	5653	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	3910	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.29	188	9220	0.40	ng/ul	0.00
16) Chrysene-d12	21.47	240	12610	0.40	ng/ul	0.00
20) Perylene-d12	24.02	264	10913	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.27	152	965	0.10	ng/ul	0.00
14) Fluoranthene-d10	19.32	212	2494	0.08	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	16.98	266	17	0.035	ng/ul#	Qvalue 33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BE098105.D
Acq On : 27 Oct 2018 1:16
Operator : SJ/JU
Sample : J5568-13RE
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AK8RE

Quant Time: Oct 27 04:04:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 27 00:33:42 2018
Response via : Initial Calibration

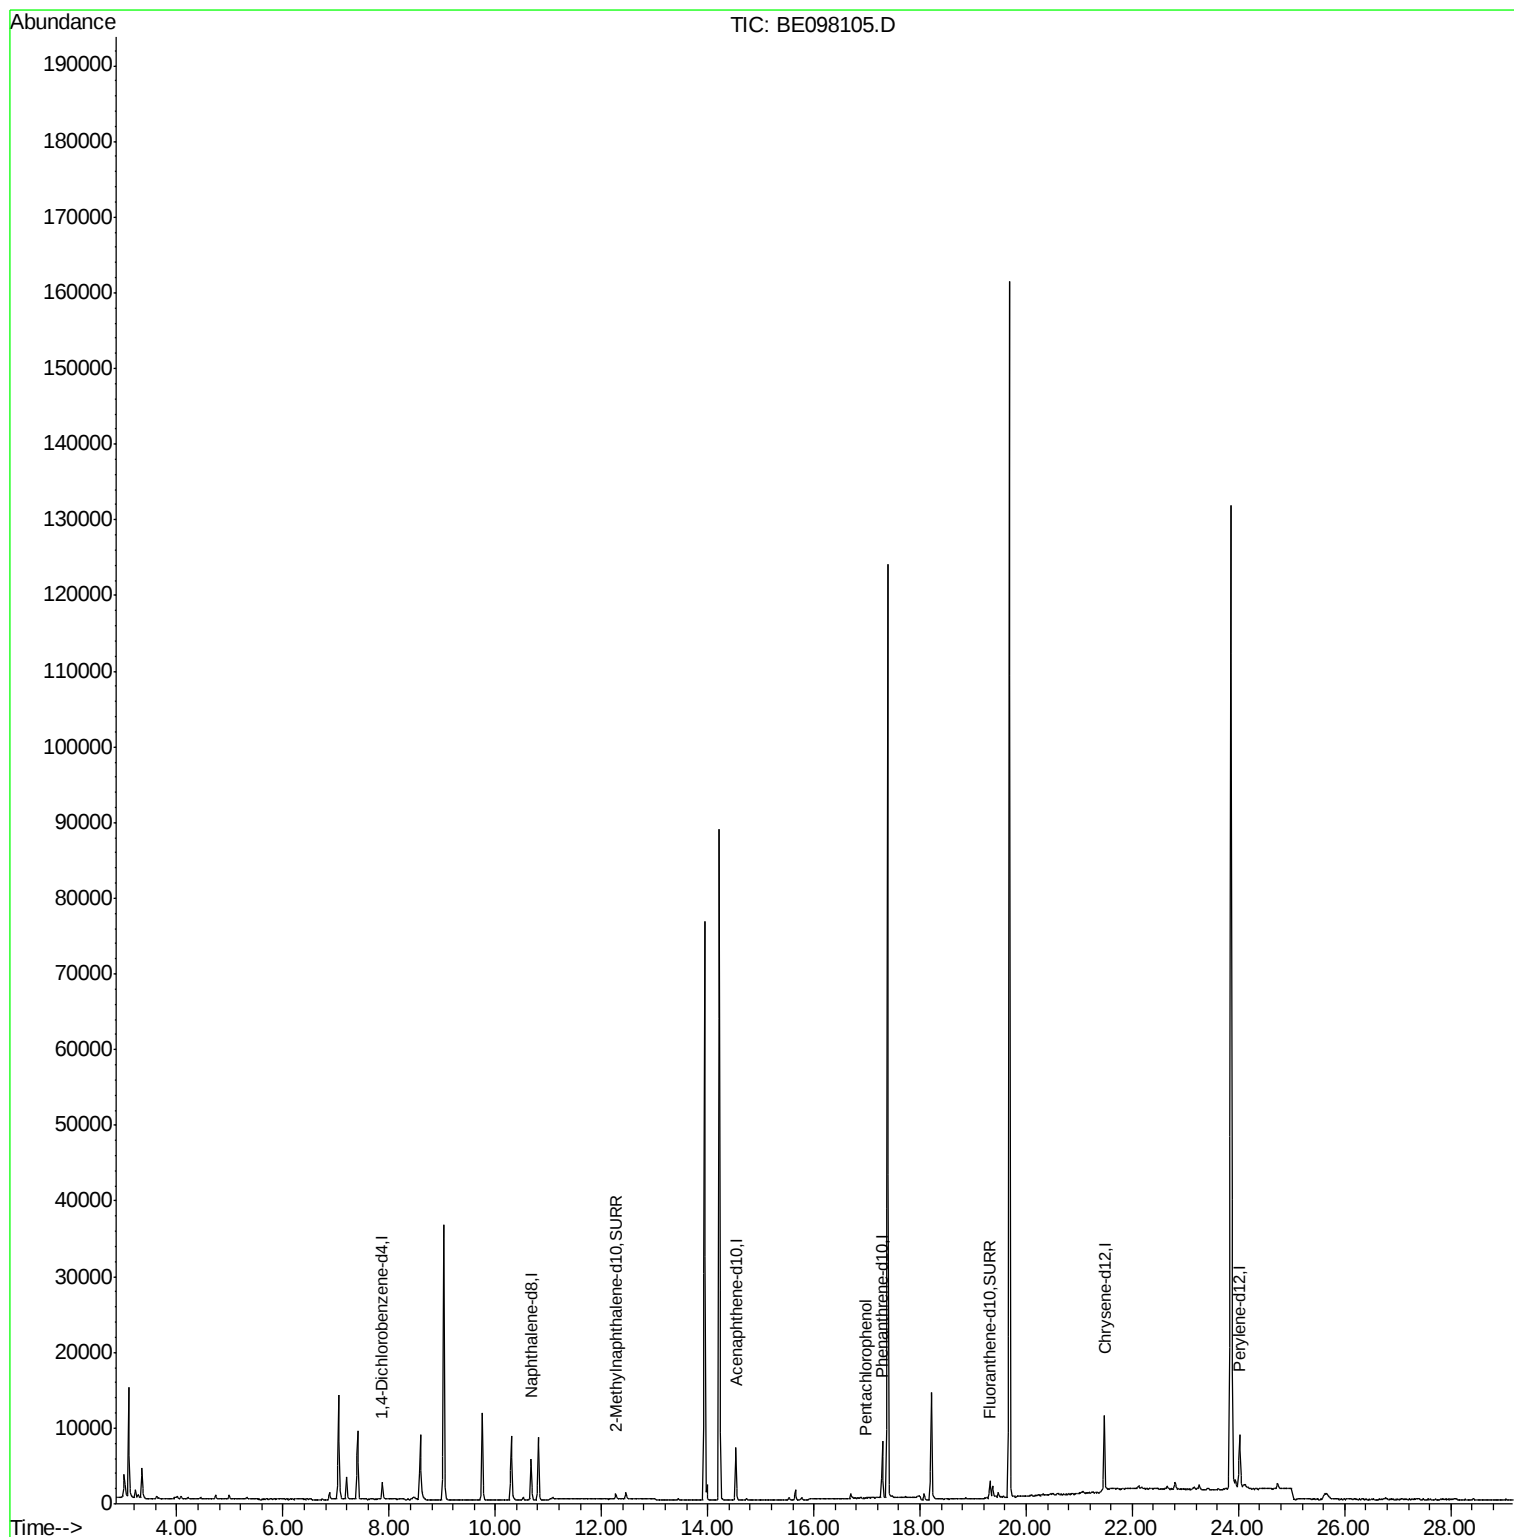

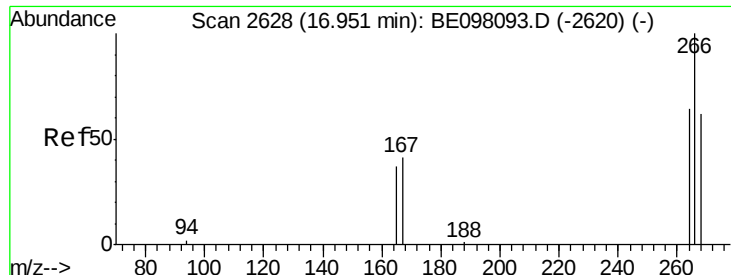

#11
 Pentachlorophenol
 Concen: 0.035 ng/ul
 RT: 16.98 min Scan# 2632
 Delta R.T. 0.03 min
 Lab File: BE098105.D
 Acq: 27 Oct 2018 1:16

Instrument :
 BNA_E
 ClientSampleId :
 C0AK8RE

Tgt Ion: 266 Resp: 17
 Ion Ratio Lower Upper
 266 100
 264 23.5 48.5 72.7#
 268 0.0 53.7 80.5#

