


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE102919\
 Data File : BE100693.D
 Acq On : 29 Oct 2019 13:10
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE101019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 23 16:49:33 2019

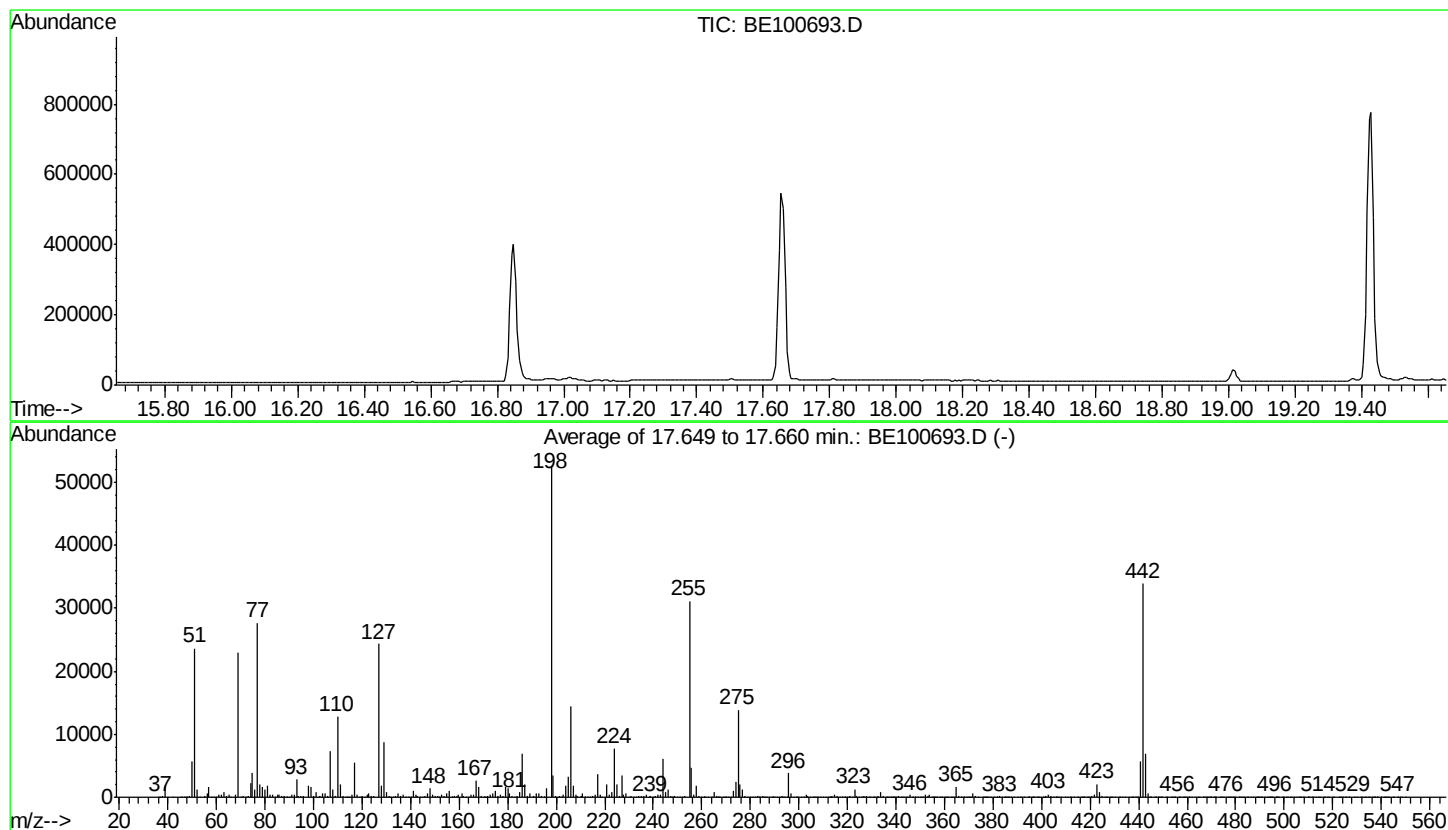

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2553

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.9	23648	PASS
68	69	0.00	2	1.6	360	PASS
69	198	0.00	100	43.7	22992	PASS
70	69	0.00	2	0.3	73	PASS
127	198	10	80	46.2	24317	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52672	PASS
199	198	5	9	6.7	3509	PASS
275	198	10	60	26.4	13915	PASS
365	198	1	100	3.3	1721	PASS
441	198	0.01	100	10.8	5708	PASS
442	198	50	100	64.3	33873	PASS
443	442	15	24	20.2	6834	PASS