
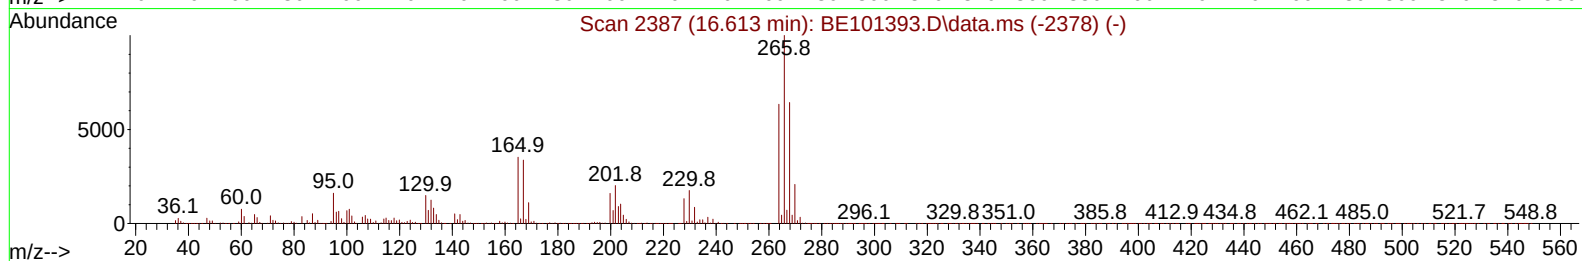
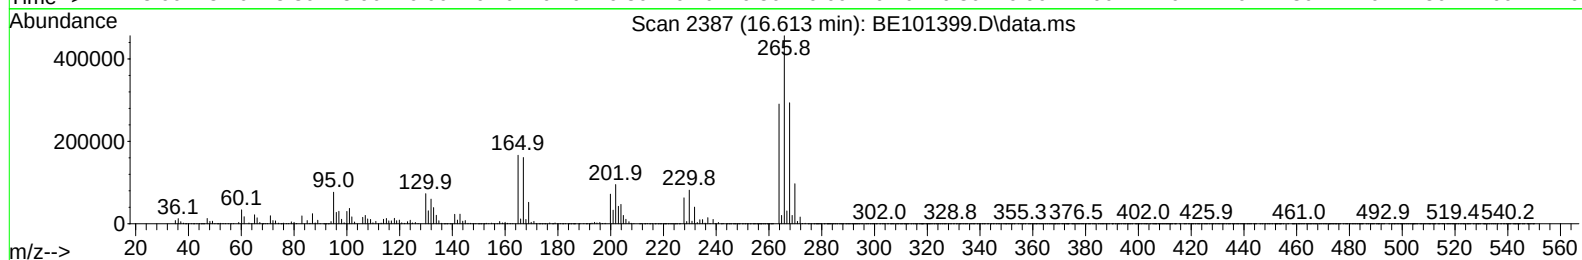


Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE102924\  
Data File : BE101399.D  
Acq On : 29 Oct 2024 10:04  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 11:47:14 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270-BE102824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Oct 29 01:26:30 2024  
Response via : Initial Calibration

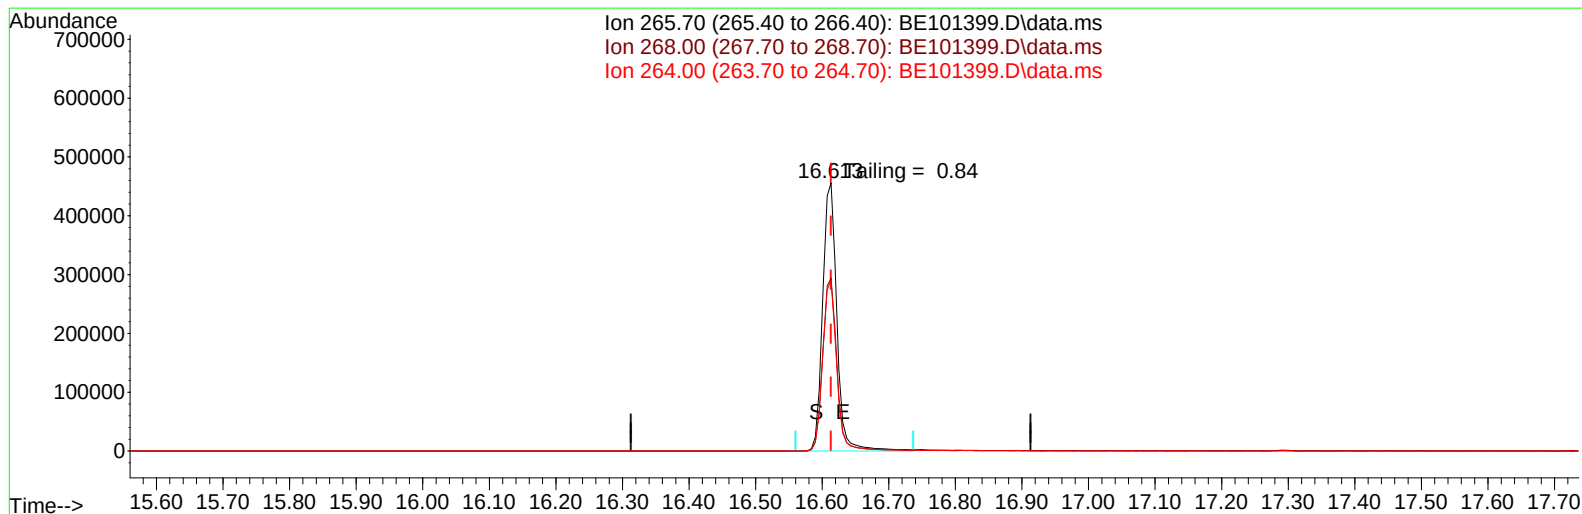

TIC: BE101399.D\data.ms

**(70) Pentachlorophenol (C)**




**16.613min (+ 0.000) 1523436.50 ng**

**response 677095**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.40  | 64.38  |
| 264.00 | 63.40  | 63.67  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE102924\  
Data File : BE101399.D  
Acq On : 29 Oct 2024 10:04  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 11:47:14 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270-BE102824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Oct 29 01:26:30 2024  
Response via : Initial Calibration

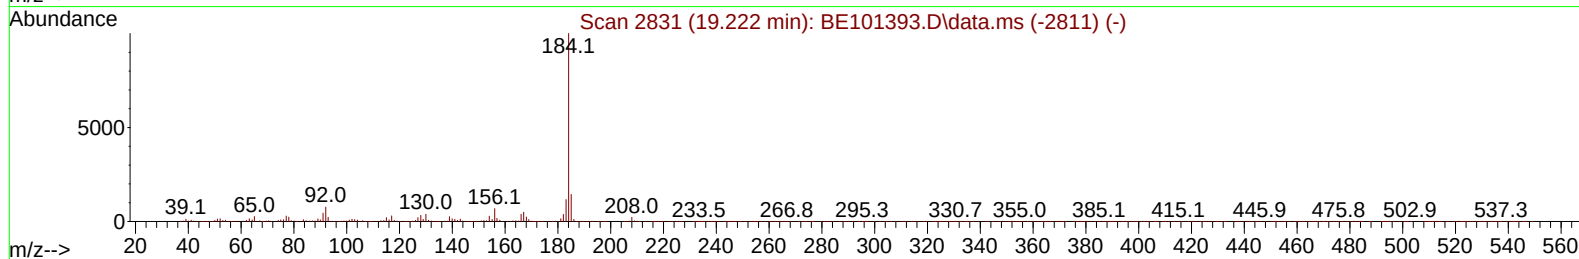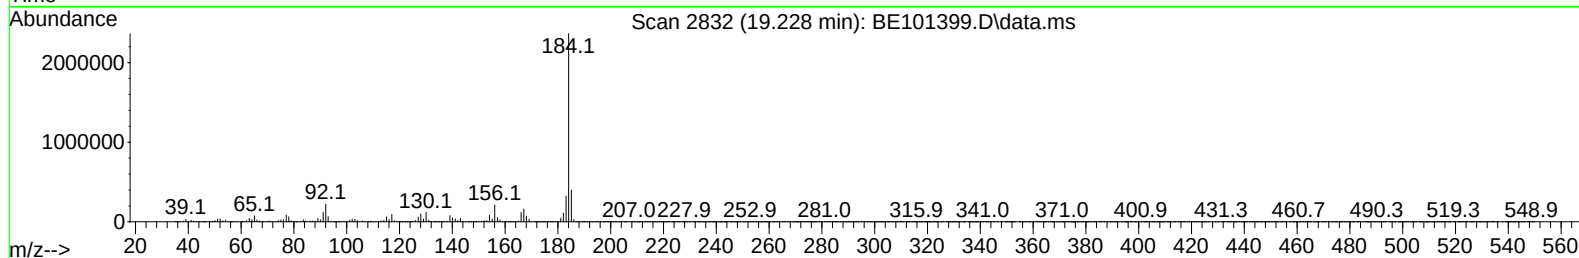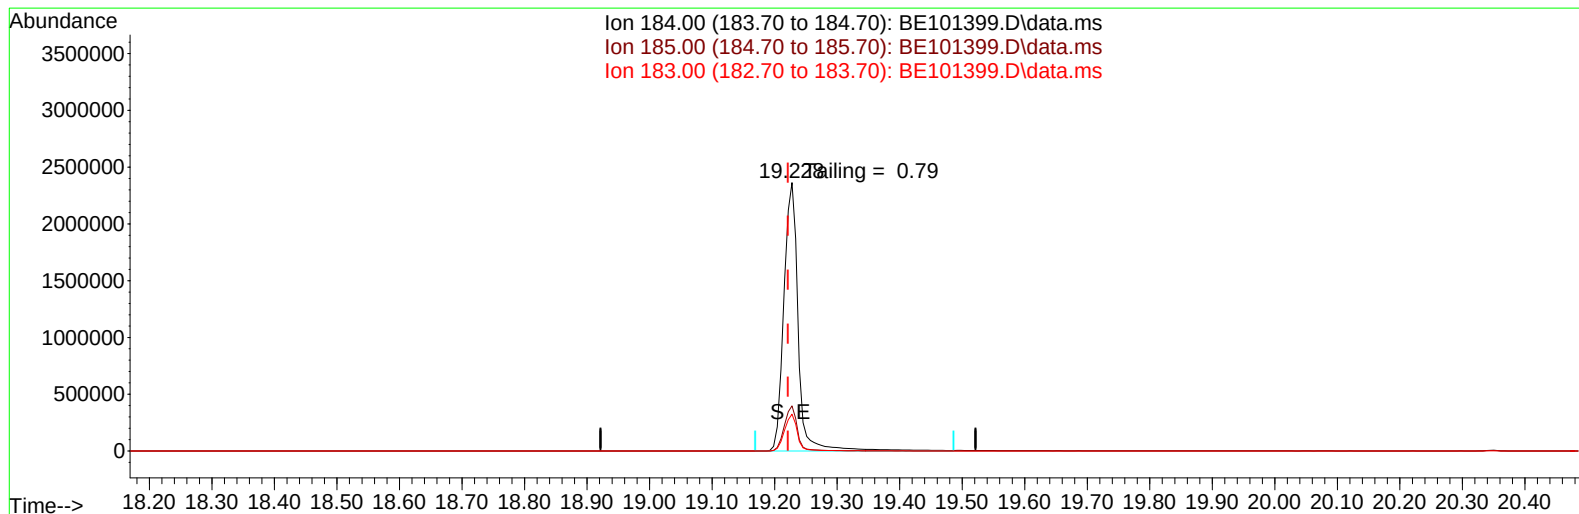

TIC: BE101399.D\data.ms

**(77) Benzidine**

19.228min (+ 0.006) 32410.12 ng

response 3791312

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 16.84  |
| 183.00 | 11.60  | 13.71  |
| 0.00   | 0.00   | 0.00   |