

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE102924\
Data File : BE101413.D
Acq On : 29 Oct 2024 18:40
Operator : RC/JU
Sample : PB164369BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164369BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BE101413.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.321	459	465	493	rBV	2271359	3514286	34.15%	8.572%
2	6.948	734	742	766	rBV	2055502	3573964	34.73%	8.717%
3	7.571	841	848	856	rBV	432045	675199	6.56%	1.647%
4	8.782	1044	1054	1074	rBV	1282549	2205558	21.43%	5.380%
5	10.339	1311	1319	1338	rBV	559660	993090	9.65%	2.422%
6	12.800	1730	1738	1763	rBV	3560093	5631837	54.72%	13.737%
7	14.175	1965	1972	1988	rBV	913596	1388776	13.49%	3.387%
8	15.685	2221	2229	2244	rBV	3178553	4832018	46.95%	11.786%
9	16.913	2431	2438	2448	rBV	1210799	1775047	17.25%	4.330%
10	19.510	2873	2880	2896	rBV	7433665	10291851	100.00%	25.103%
11	21.073	3140	3146	3162	rBV	2031691	2703136	26.26%	6.593%
12	23.359	3526	3535	3546	rBV	1680710	3413621	33.17%	8.326%




Sum of corrected areas: 40998383

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE102924\
Data File : BE101413.D
Acq On : 29 Oct 2024 18:40
Operator : RC/JU
Sample : PB164369BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164369BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

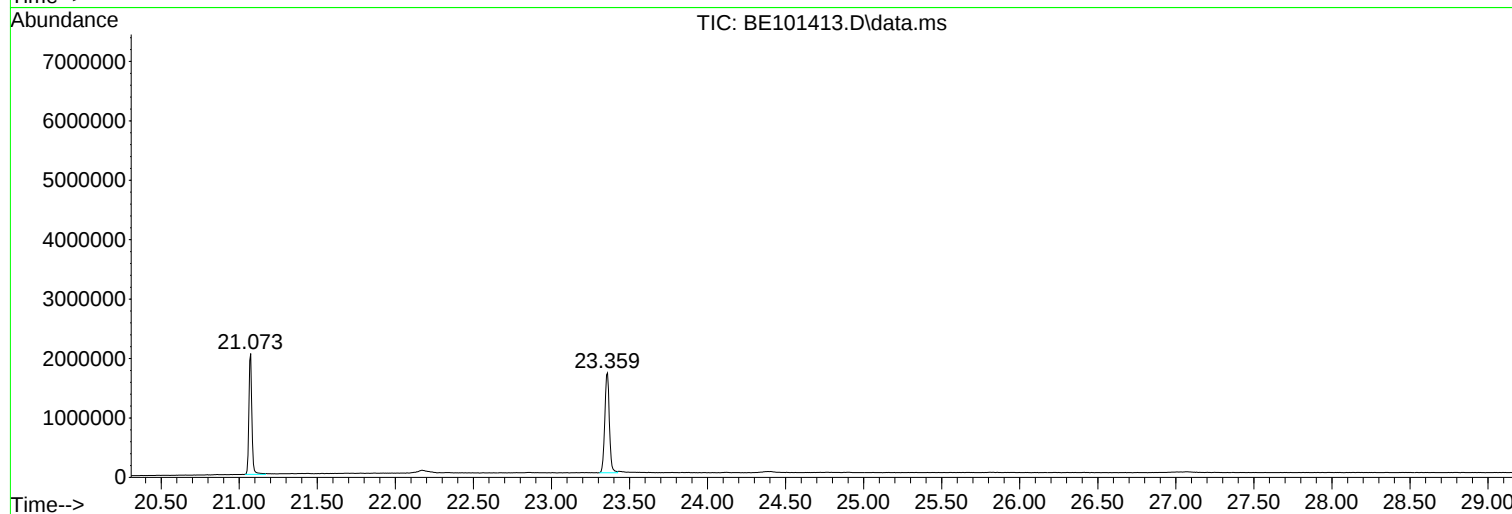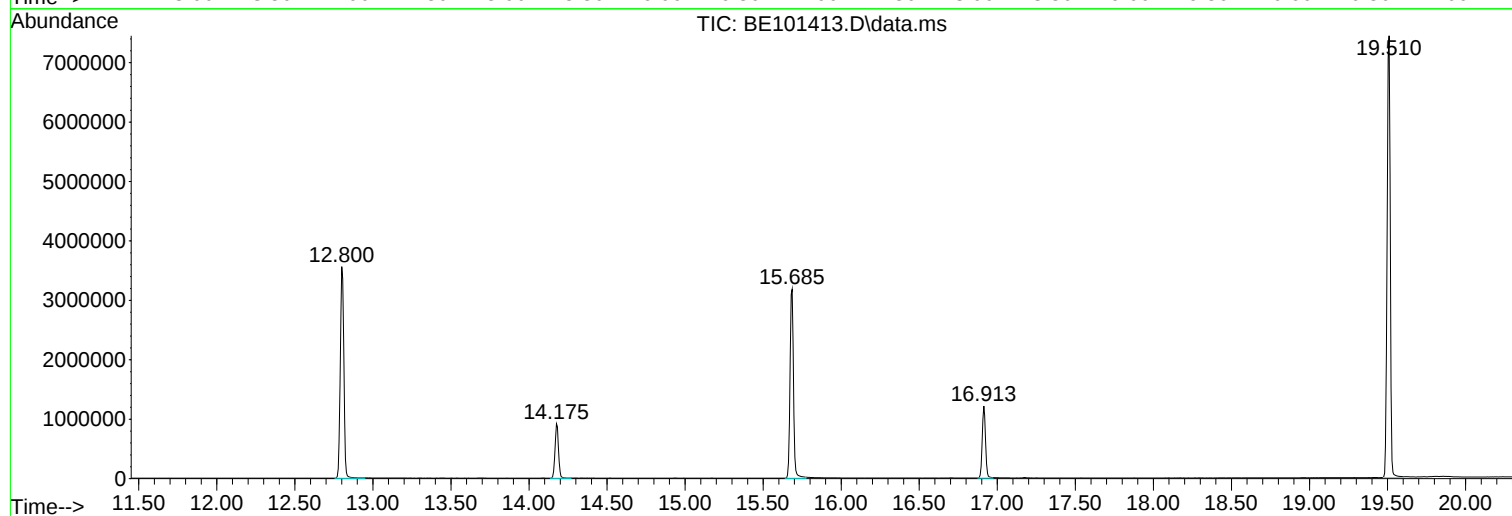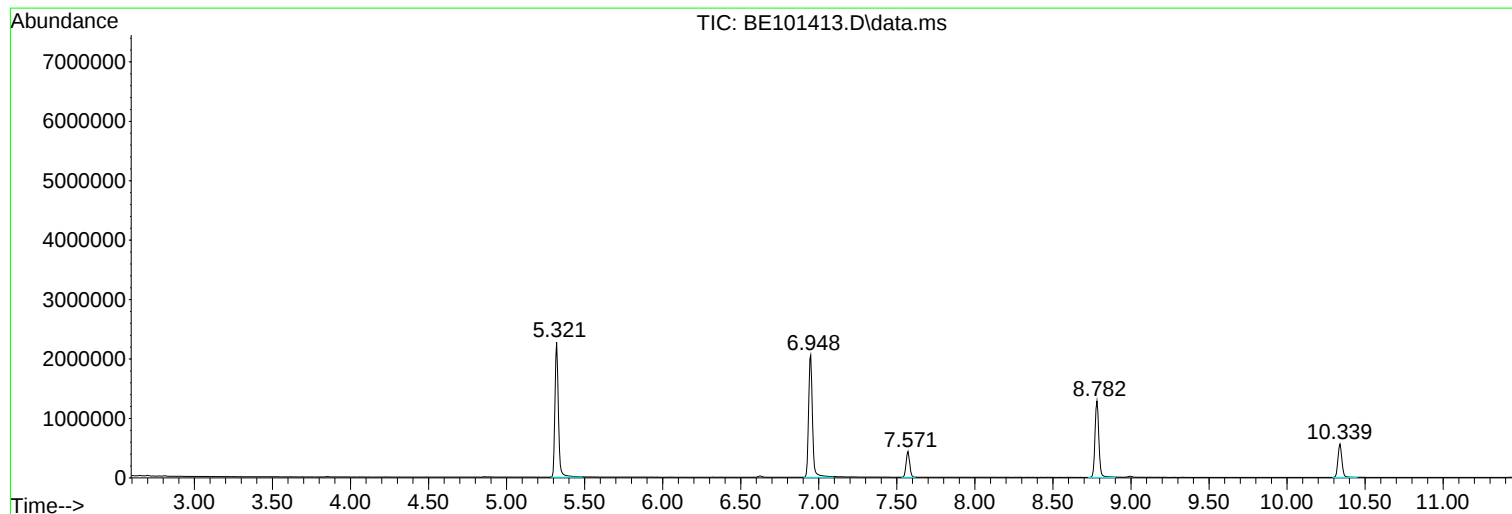

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE102924\
Data File : BE101413.D
Acq On : 29 Oct 2024 18:40
Operator : RC/JU
Sample : PB164369BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164369BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE102924\
Data File : BE101413.D
Acq On : 29 Oct 2024 18:40
Operator : RC/JU
Sample : PB164369BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164369BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------