
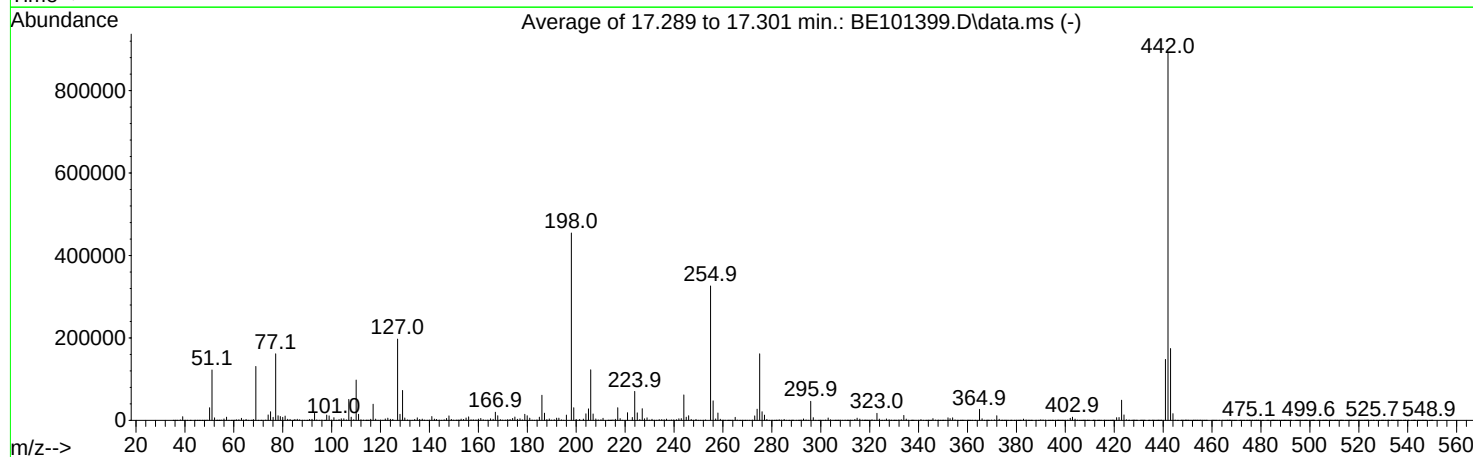


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE102924\
Data File : BE101399.D
Acq On : 29 Oct 2024 10:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 29 01:26:30 2024

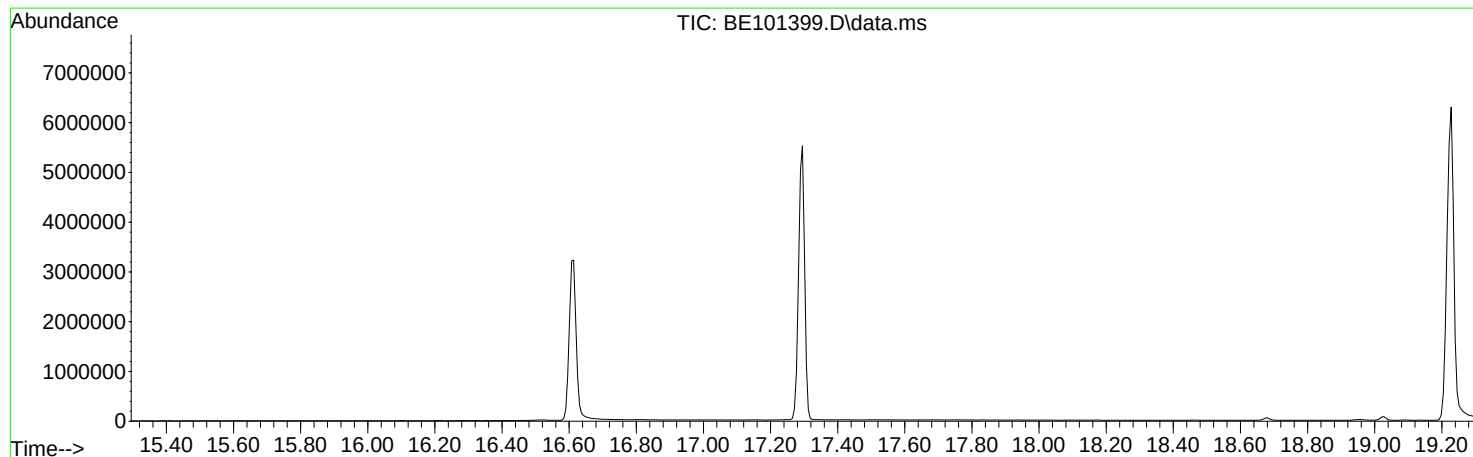




AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.9	122244	PASS
68	69	0.00	2	1.4	1866	PASS
69	198	0.00	100	28.8	130955	PASS
70	69	0.00	2	0.4	555	PASS
127	198	10	80	43.4	197224	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	454464	PASS
199	198	5	9	6.7	30635	PASS
275	198	10	60	35.6	161579	PASS
365	198	1	100	5.9	26756	PASS
441	198	0.01	100	32.5	147857	PASS
442	442	50	100	100.0	892479	PASS
443	442	15	24	19.5	174158	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE102924\
Data File : BE101399.D
Acq On : 29 Oct 2024 10:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Oct 29 11:47:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

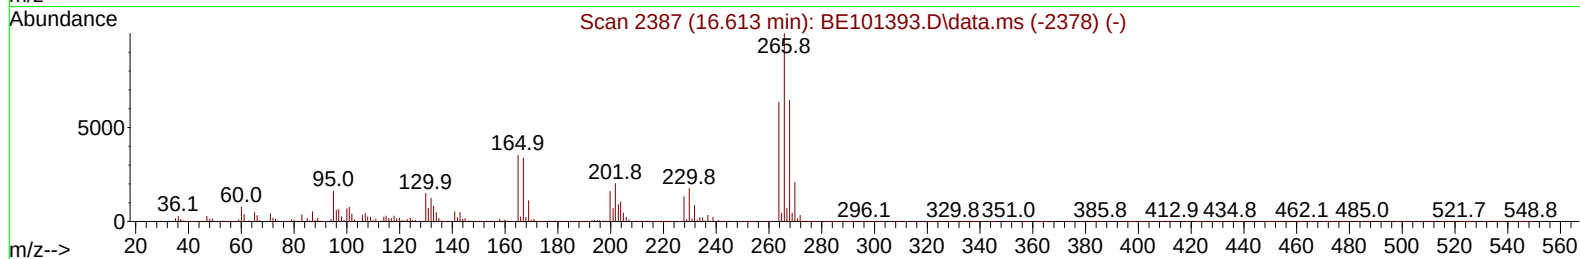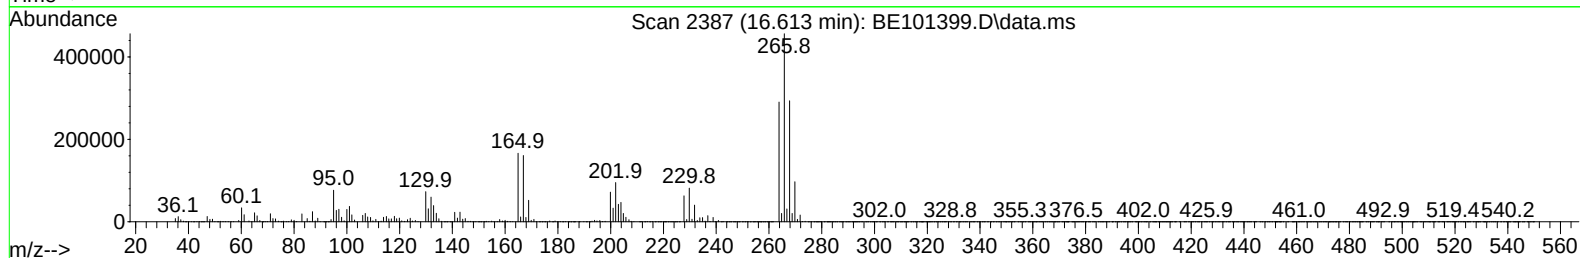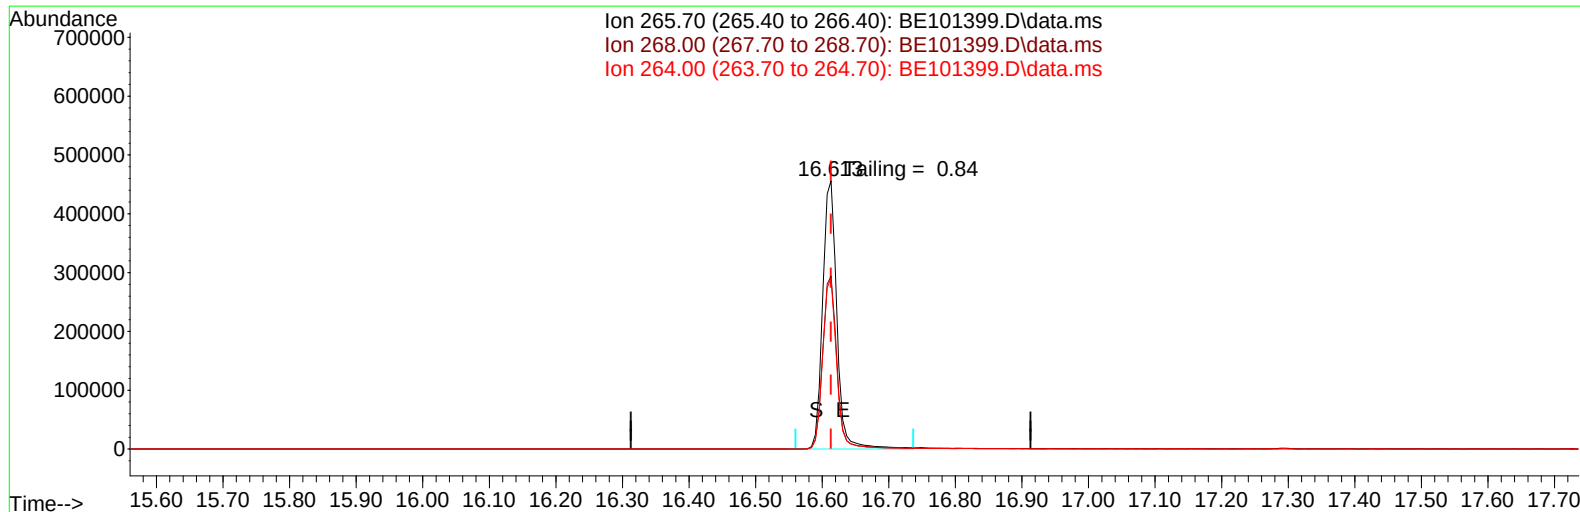

TIC: BE101399.D\data.ms

(70) Pentachlorophenol (C)

16.613min (+ 0.000) 1523436.50 ng




response 677095

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	64.38
264.00	63.40	63.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE102924\
Data File : BE101399.D
Acq On : 29 Oct 2024 10:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Oct 29 11:47:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

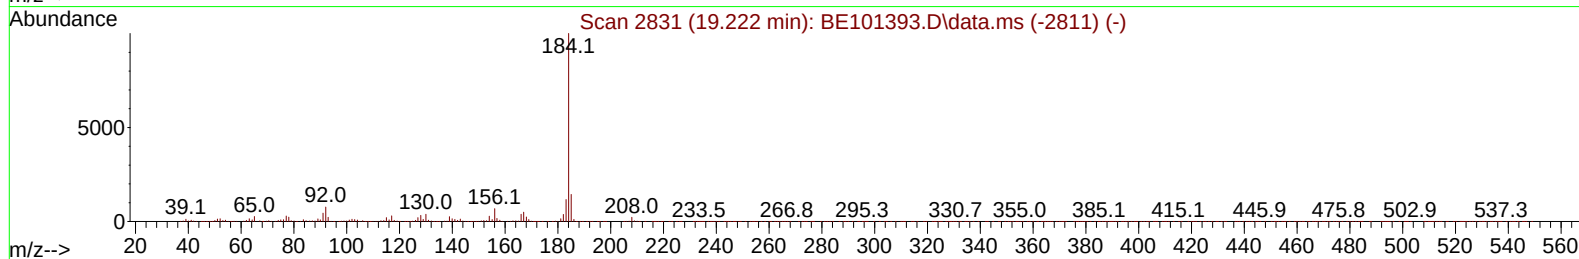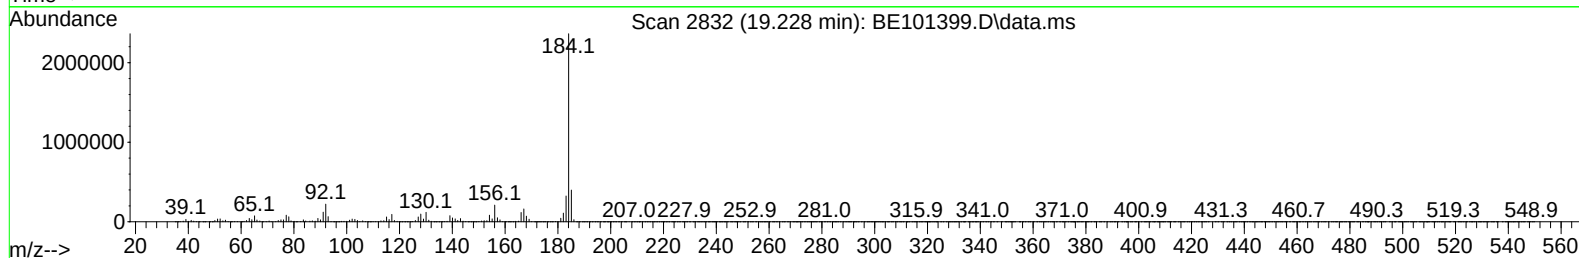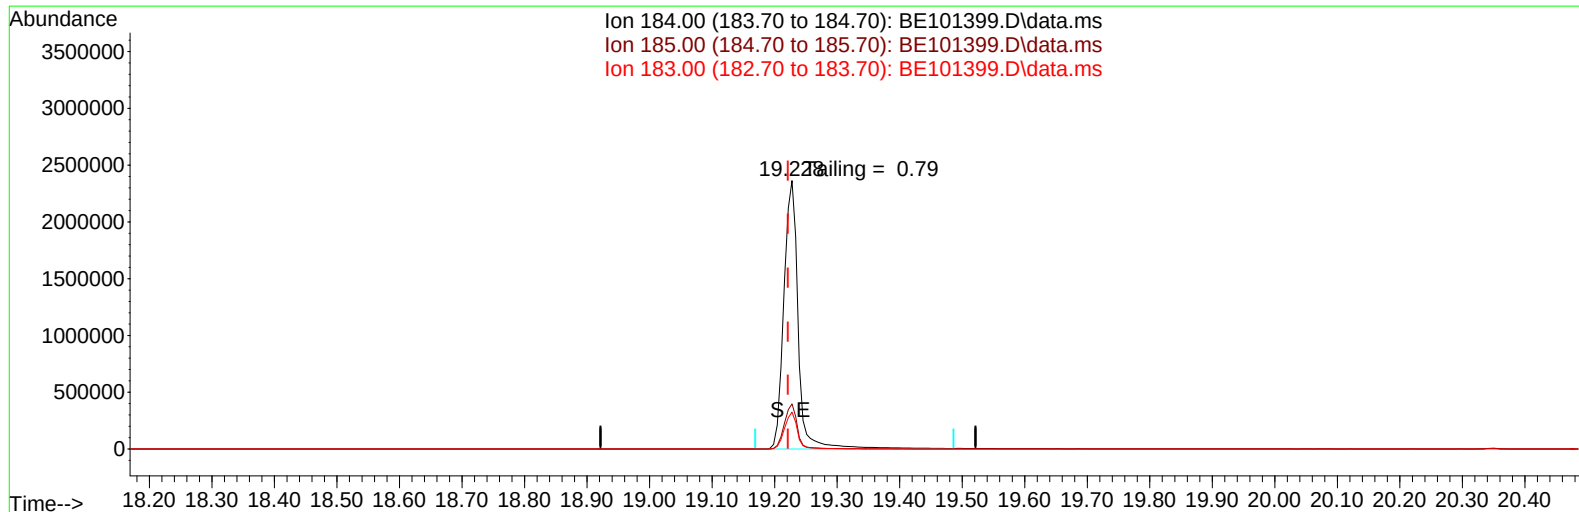

TIC: BE101399.D\data.ms

(77) Benzidine

19.228min (+ 0.006) 32410.12 ng

response 3791312

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	16.84
183.00	11.60	13.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/29/2024	BNA_E	<u>BE101399.D</u>
Compound Name	Response	Retention Time
DDT	1913621	20.35
DDD	61909	19.915
DDE	432	19.51
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
62341	1975962	3.15

Instrument :
BNA_E
ClientSampleId :
DFTPP