

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE103018\
 Data File : BE098110.D
 Acq On : 30 Oct 2018 12:15
 Operator : SJ/JU
 Sample : J5598-16DL 10X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Oct 30 12:54:42 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 30 01:14:11 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.87	152	1088	0.40	ng/ul	0.00
2) Naphthalene-d8	10.67	136	5464	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	3932	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.29	188	9567	0.40	ng/ul	0.00
16) Chrysene-d12	21.47	240	13629	0.40	ng/ul	0.00
20) Perylene-d12	24.02	264	10769	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.27	152	185	0.02	ng/ul	0.00
14) Fluoranthene-d10	19.32	212	551	0.02	ng/ul	0.00
Target Compounds				Ovalue		
3) Naphthalene	10.72	128	2100	0.161	ng/ul	96
5) 2-Methylnaphthalene	12.34	142	682	0.069	ng/ul	99
7) Acenaphthylene	14.25	152	1821	0.117	ng/ul#	94
11) Pentachlorophenol	16.96	266	17	0.034	ng/ul#	33
12) Phenanthrene	17.33	178	4773	0.216	ng/ul	99
13) Anthracene	17.42	178	3699	0.170	ng/ul	99
15) Fluoranthene	19.35	202	24674	0.876	ng/ul	99
17) Pyrene	19.71	202	31302	0.984	ng/ul	100
18) Benzo(a)anthracene	21.45	228	21463	0.536	ng/ul	98
19) Chrysene	21.50	228	33124	1.069	ng/ul	99
21) Benzo(b)fluoranthene	23.24	252	82337	2.760	ng/ul	98
22) Benzo(k)fluoranthene	23.24	252	82337	2.819	ng/ul	99
23) Benzo(a)pyrene	23.90	252	18572	0.647	ng/ul	97
24) Indeno(1,2,3-cd)pyrene	26.70	276	23361	0.710	ng/ul#	96
25) Dibenzo(a,h)anthracene	26.73	278	5758	0.210	ng/ul#	90
26) Benzo(a,h,i)perylene	27.54	276	19898	0.719	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE103018\
Data File : BE098110.D
Acq On : 30 Oct 2018 12:15
Operator : SJ/JU
Sample : J5598-16DL 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Oct 30 12:54:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 30 01:14:11 2018
Response via : Initial Calibration

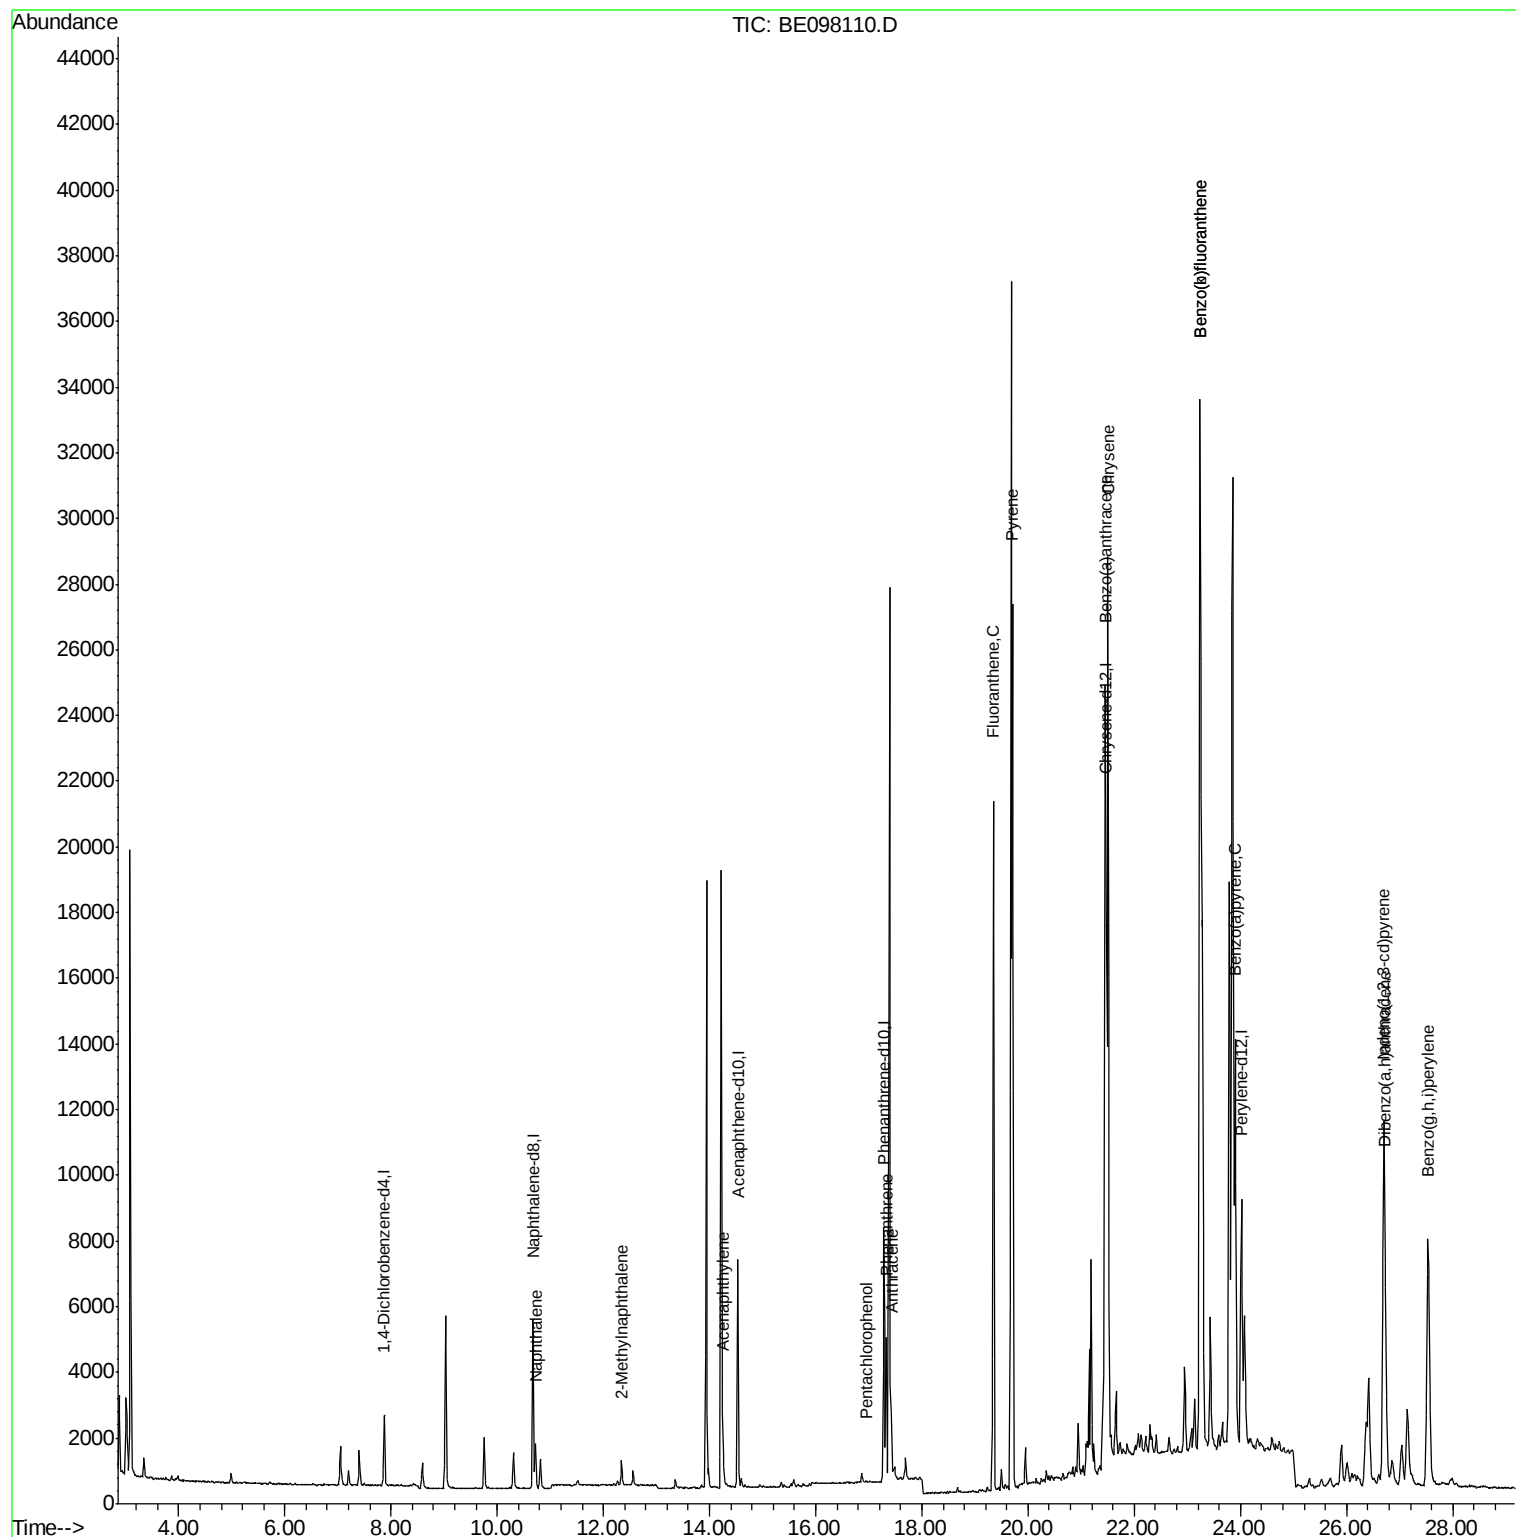

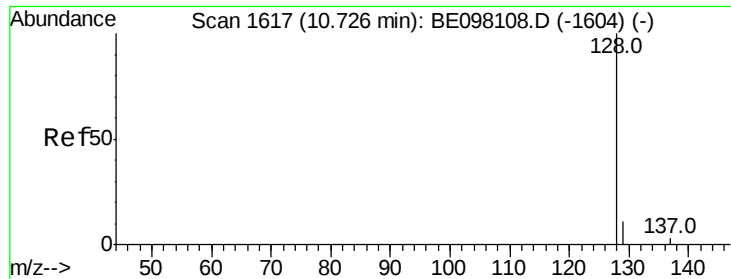

#3

Naphthalene

Concen: 0.161 ng/ul

RT: 10.72 min Scan# 1616

Delta R.T. -0.00 min

Lab File: BE098110.D

Acq: 30 Oct 2018 12:15

Instrument :

BNA_E

ClientSampleId :


Tot Ion:128 Resp: 2100

Ion Ratio Lower Upper

128 100

129 14.6 10.5 15.7




127 0.0 0.0 0.0



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

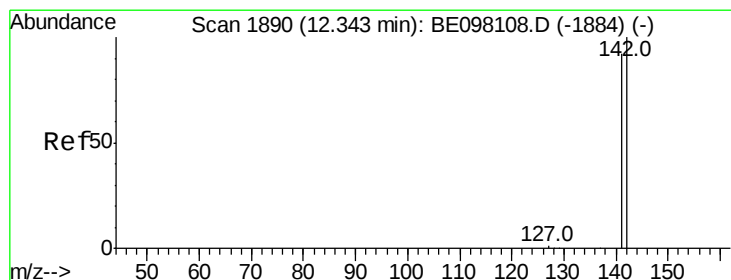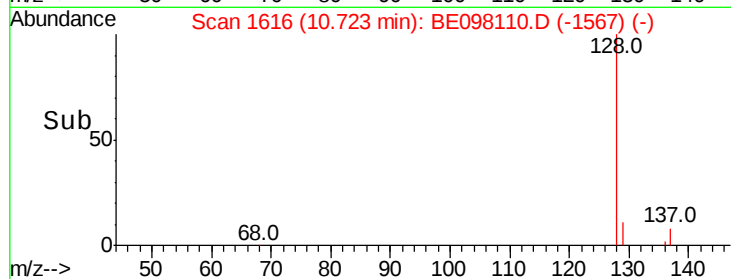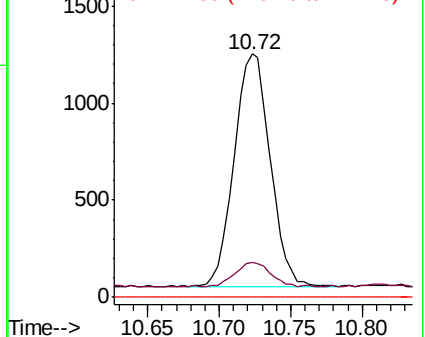

#5

2-Methylnaphthalene

Concen: 0.069 ng/ul

RT: 12.34 min Scan# 1890

Delta R.T. -0.00 min

Lab File: BE098110.D


Acq: 30 Oct 2018 12:15

Tgt Ion:142 Resp: 682

Ion Ratio Lower Upper



142 100


141 91.8 72.5 108.7



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

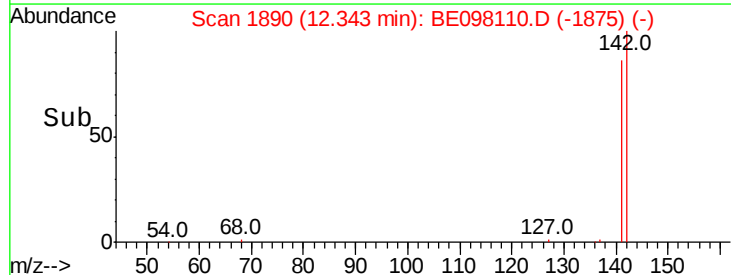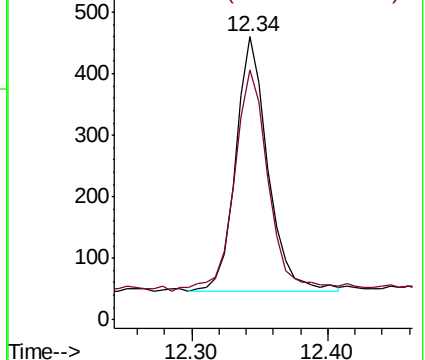

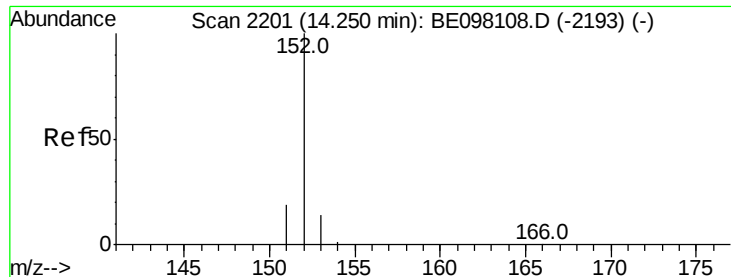

#7

Acenaphthylene

Concen: 0.117 ng/ul

RT: 14.25 min Scan# 2200

Delta R.T. -0.00 min

Lab File: BE098110.D

Acq: 30 Oct 2018 12:15

Instrument :

BNA_E

ClientSampled :


Tot Ion:152 Resp: 1821

Ion Ratio Lower Upper

152 100

151 24.1 17.3 25.9




153 18.2 11.9 17.9#



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

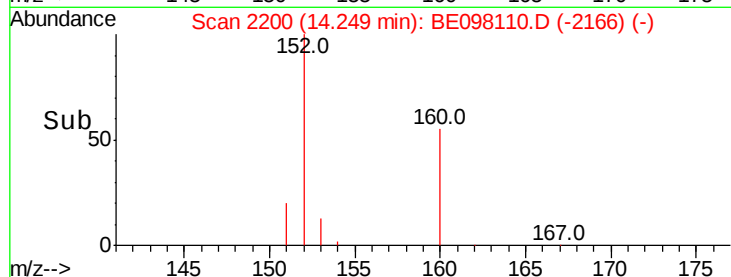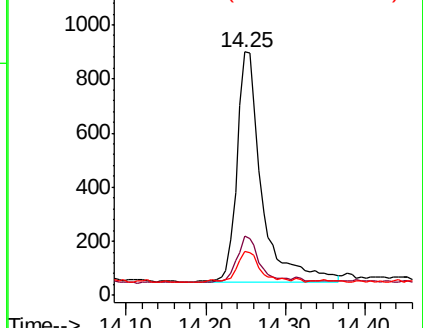

#11

Pentachlorophenol

Concen: 0.034 ng/ul

RT: 16.96 min Scan# 2629

Delta R.T. 0.01 min

Lab File: BE098110.D

Acq: 30 Oct 2018 12:15


Tgt Ion:266 Resp: 17

Ion Ratio Lower Upper

266 100

264 23.5 48.5 72.7#



268 0.0 53.7 80.5#




Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

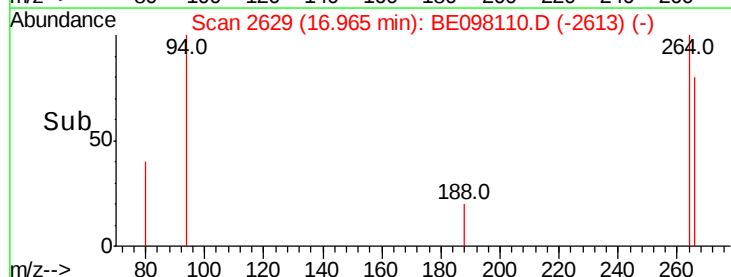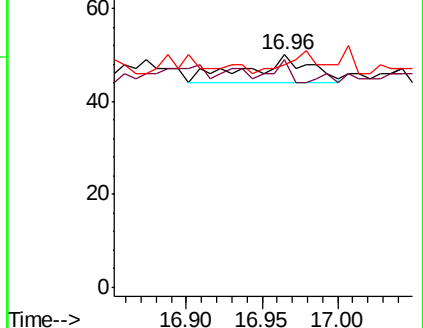

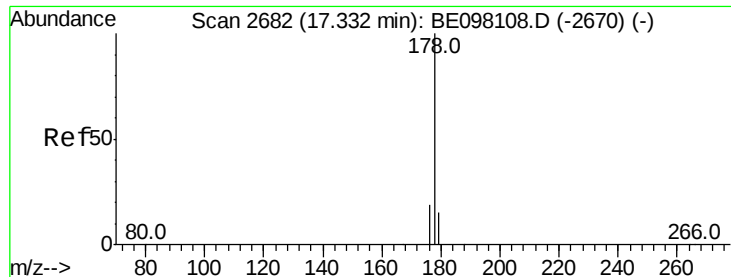

#12

Phenanthrene

Concen: 0.216 ng/ul

RT: 17.33 min Scan# 2681

Delta R.T. -0.00 min

Lab File: BE098110.D

Acq: 30 Oct 2018 12:15

Instrument :

BNA_E

ClientSampleId :


Tot Ion:178 Resp: 4773

Ion Ratio Lower Upper

178 100

179 16.8 13.0 19.4




176 19.7 15.7 23.5

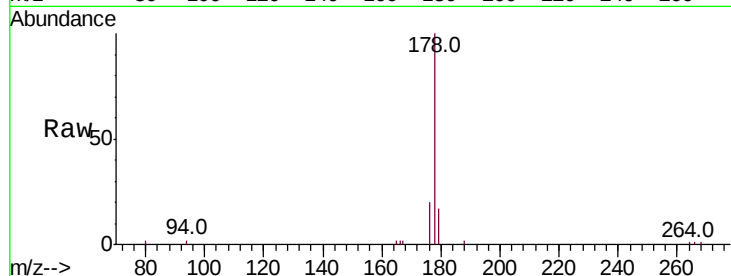

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

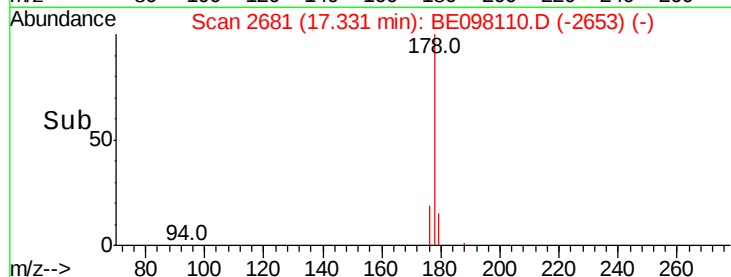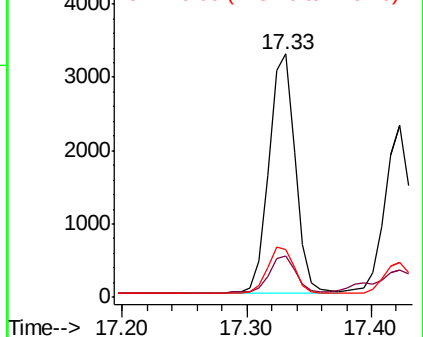

#13

Anthracene

Concen: 0.170 ng/ul

RT: 17.42 min Scan# 2694

Delta R.T. -0.00 min

Lab File: BE098110.D

Acq: 30 Oct 2018 12:15


Tgt Ion:178 Resp: 3699

Ion Ratio Lower Upper

178 100

179 16.0 12.6 19.0



176 20.4 15.6 23.4




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

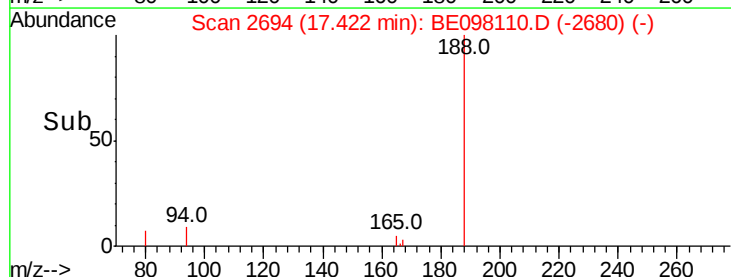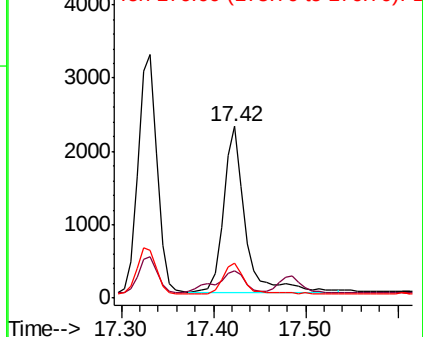


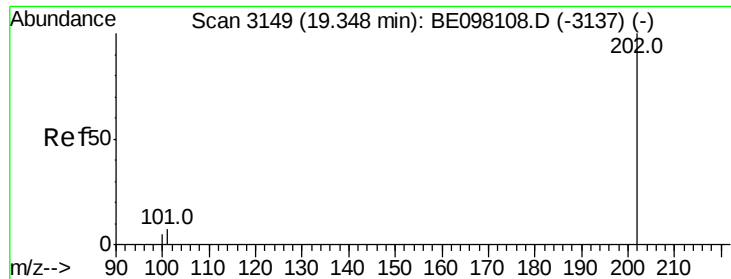




#15
Fluoranthene
Concen: 0.876 ng/ul
RT: 19.35 min Scan# 3149
Delta R.T. 0.00 min
Lab File: BE098110.D
Acq: 30 Oct 2018 12:15

Instrument :
BNA_E
ClientSampleId :

Tot Ion:202 Resp: 24674
Ion Ratio Lower Upper
202 100
101 6.9 0.0 27.5
100 6.1 0.0 26.0

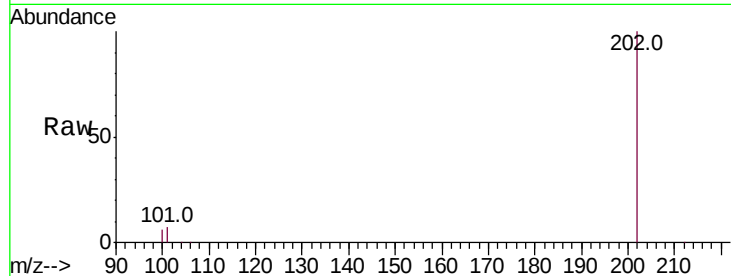


Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): BE

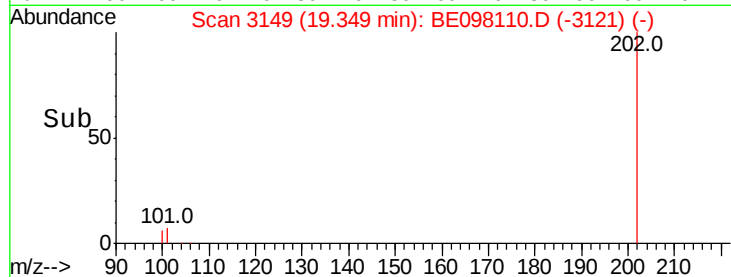
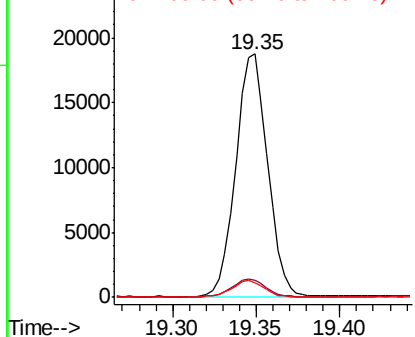



#17
Pyrene
Concen: 0.984 ng/ul
RT: 19.71 min Scan# 3250
Delta R.T. -0.00 min
Lab File: BE098110.D
Acq: 30 Oct 2018 12:15

Tgt Ion:202 Resp: 31302
Ion Ratio Lower Upper
202 100
101 8.5 6.9 10.3
100 7.5 6.0 9.0



Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): BE

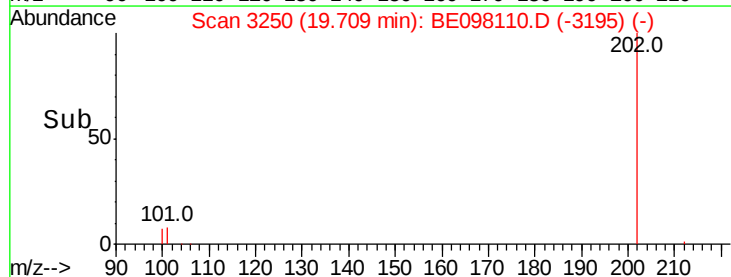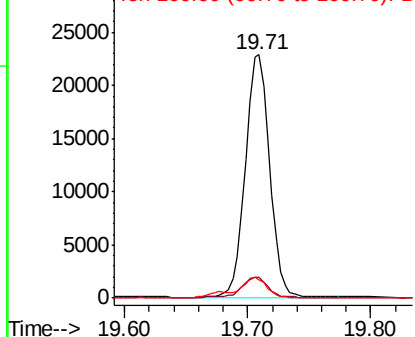

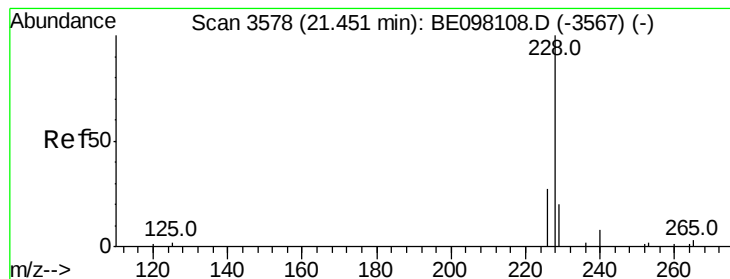

#18

Benzo(a)anthracene

Concen: 0.536 ng/ul

RT: 21.45 min Scan# 3577

Delta R.T. 0.00 min

Lab File: BE098110.D

Acq: 30 Oct 2018 12:15

Instrument :

BNA_E

ClientSampleId :


Tot Ion:228 Resp: 21463

Ion Ratio Lower Upper

228 100

229 21.7 16.1 24.1

226 28.6 22.2 33.4



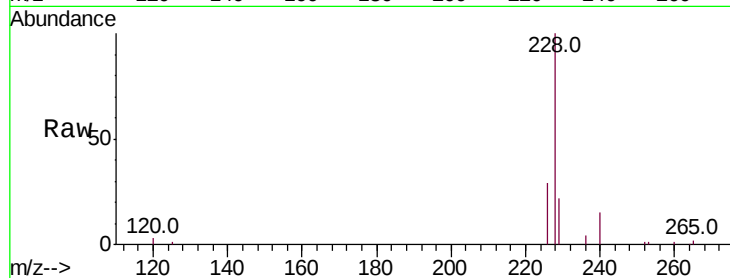


Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

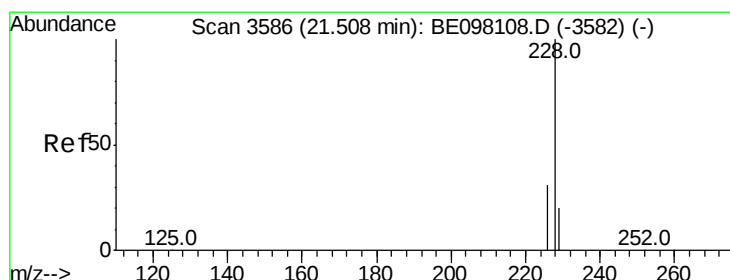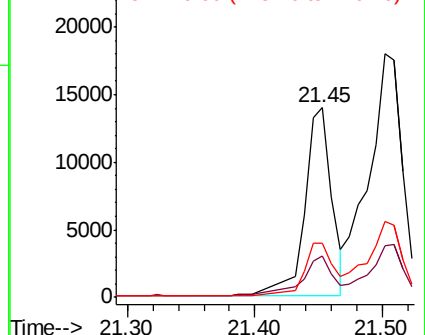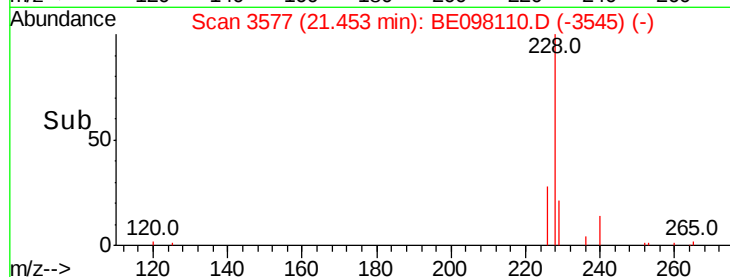

#19

Chrysene

Concen: 1.069 ng/ul

RT: 21.50 min Scan# 3584

Delta R.T. -0.01 min

Lab File: BE098110.D

Acq: 30 Oct 2018 12:15


Tgt Ion:228 Resp: 33124

Ion Ratio Lower Upper

228 100

226 31.3 24.6 37.0

229 21.0 16.4 24.6


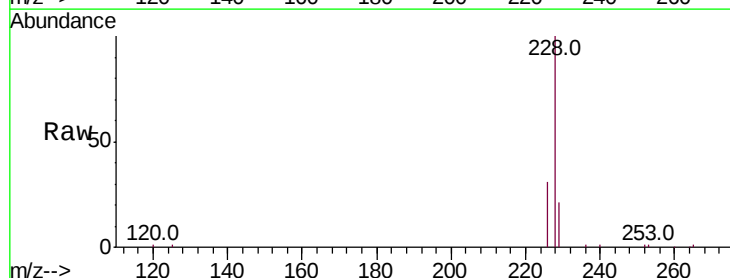



Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E



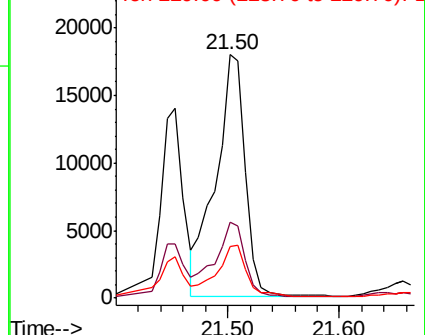
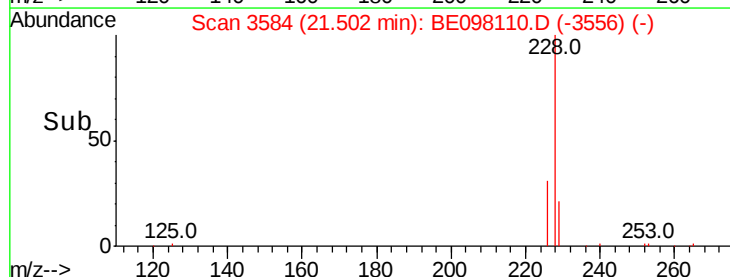


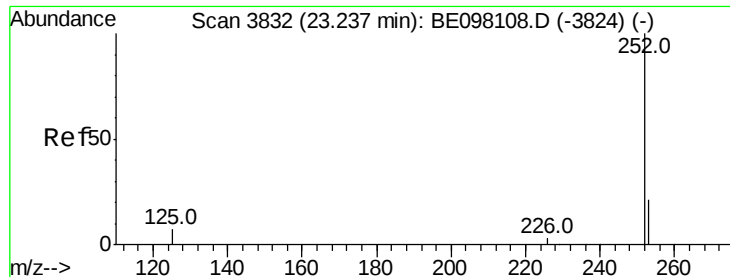

#21
Benzo(b)fluoranthene
Concen: 2.760 ng/ul
RT: 23.24 min Scan# 3831
Delta R.T. 0.00 min
Lab File: BE098110.D
Acq: 30 Oct 2018 12:15




Instrument :
BNA_E
ClientSampleId :


Tot Ion:252 Resp: 82337
Ion Ratio Lower Upper
252 100
253 23.2 0.0 47.8
125 7.7 0.0 16.8

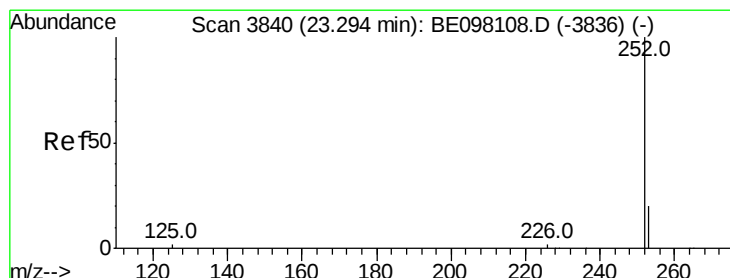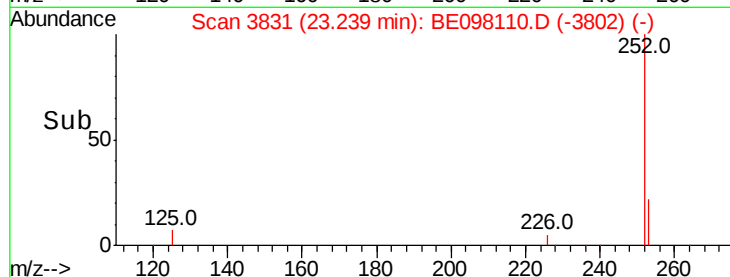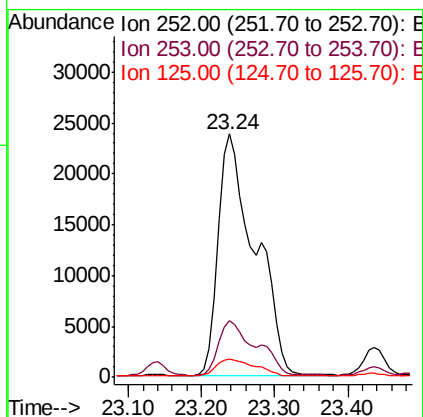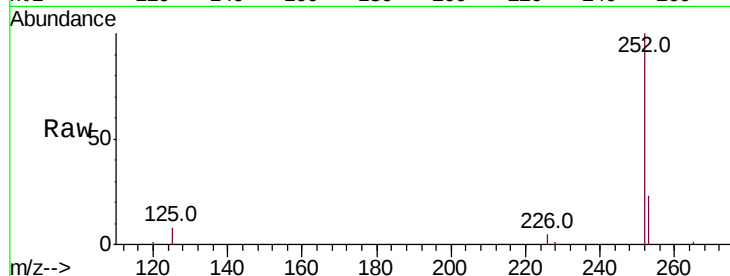

#22
Benzo(k)fluoranthene
Concen: 2.819 ng/ul
RT: 23.24 min Scan# 3831
Delta R.T. -0.05 min
Lab File: BE098110.D
Acq: 30 Oct 2018 12:15

Tgt Ion:252 Resp: 82337
Ion Ratio Lower Upper
252 100
253 23.2 19.3 28.9
125 7.7 6.2 9.2

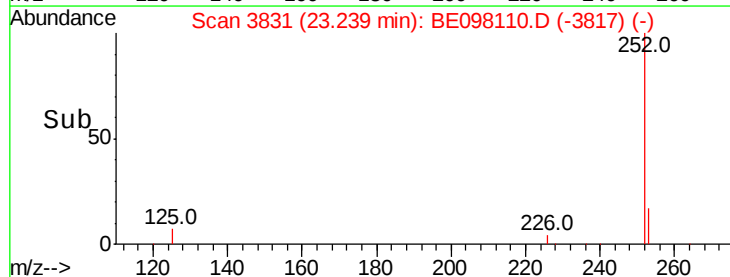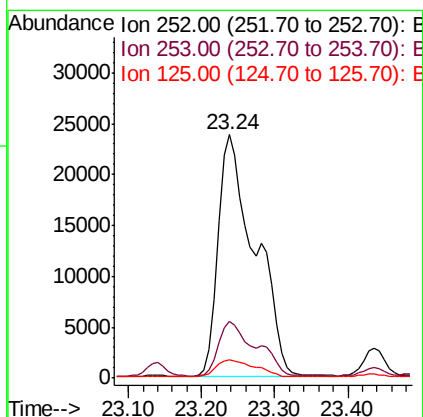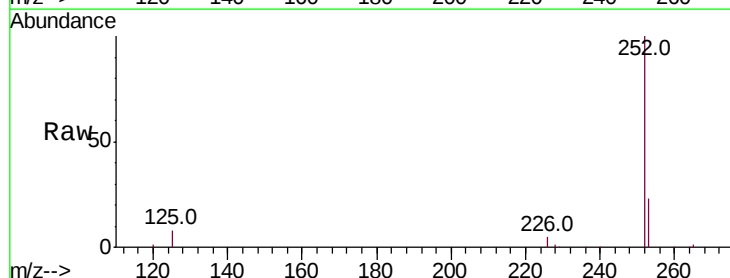

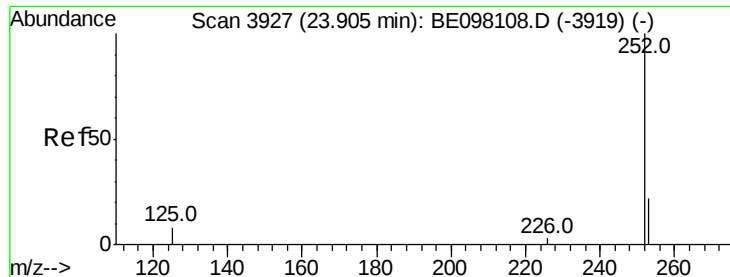

#23

Benzo(a)pyrene

Concen: 0.647 ng/ul

RT: 23.90 min Scan# 3925

Delta R.T. -0.01 min

Lab File: BE098110.D

Acq: 30 Oct 2018 12:15

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 18572

Ion Ratio Lower Upper

252 100

253 25.8 19.4 29.2




125 8.5 7.8 11.8

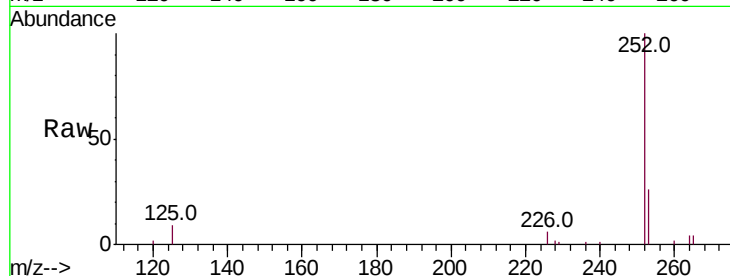

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

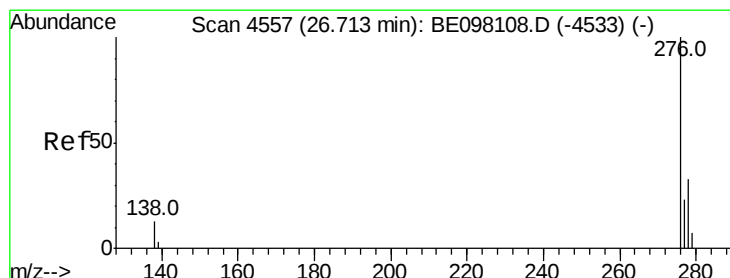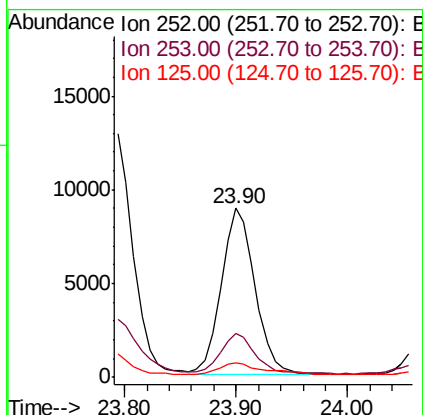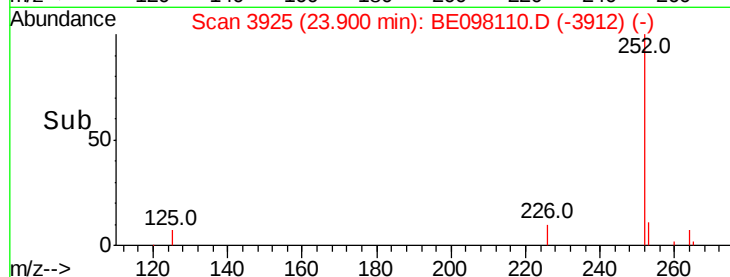

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.710 ng/ul

RT: 26.70 min Scan# 4553

Delta R.T. -0.01 min

Lab File: BE098110.D

Acq: 30 Oct 2018 12:15


Tgt Ion:276 Resp: 23361

Ion Ratio Lower Upper

276 100

138 13.1 11.8 17.8



227 0.0 0.0 0.0

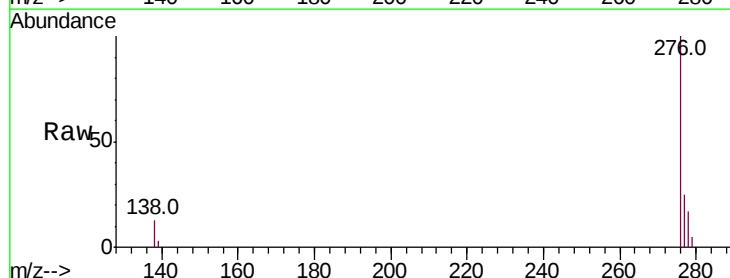


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E

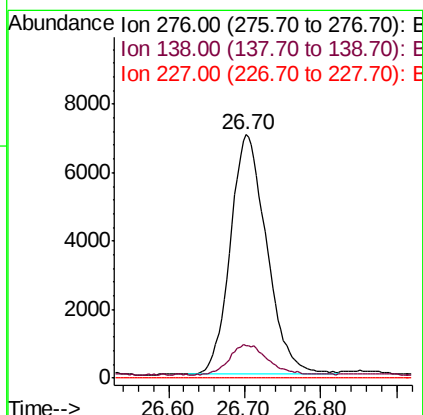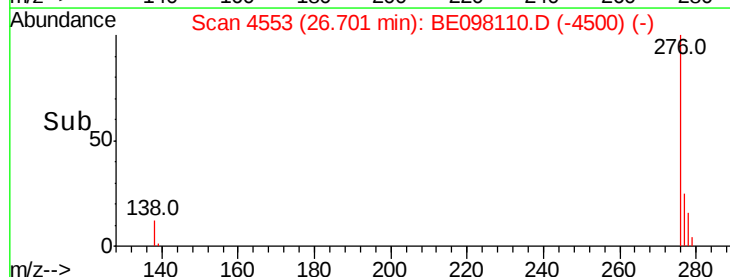




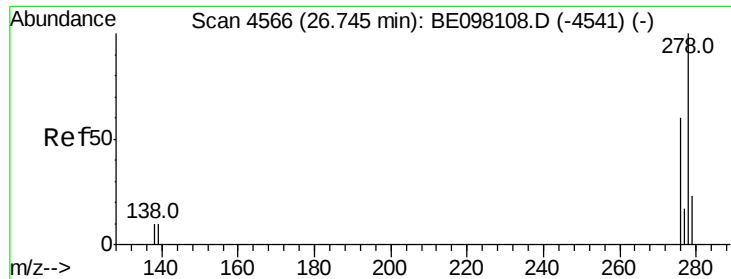


#25
Dibenzo(a,h)anthracene
Concen: 0.210 ng/ul
RT: 26.73 min Scan# 4561
Delta R.T. -0.02 min
Lab File: BE098110.D
Acq: 30 Oct 2018 12:15

Instrument :
BNA_E
ClientSampleId :

Tot Ion:278 Resp: 5758

Ion	Ratio	Lower	Upper
278	100		
139	16.8	10.0	15.0#
279	30.1	20.3	30.5

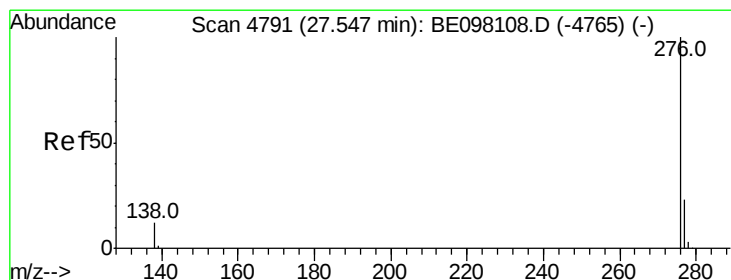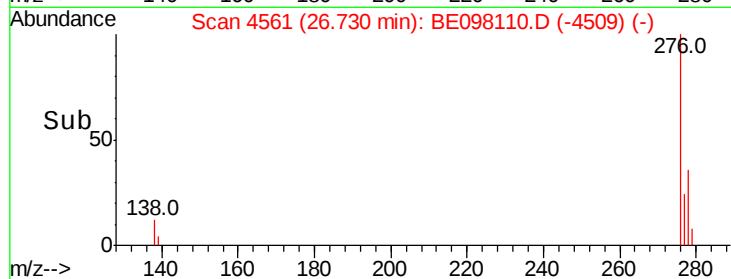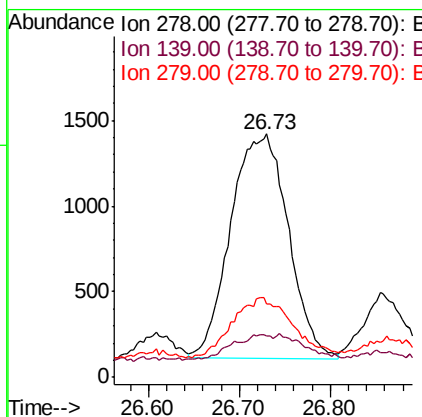

#26
Benzo(g,h,i)perylene
Concen: 0.719 ng/ul
RT: 27.54 min Scan# 4787
Delta R.T. -0.01 min
Lab File: BE098110.D
Acq: 30 Oct 2018 12:15

Tgt Ion:276 Resp: 19898

Ion	Ratio	Lower	Upper
276	100		
138	14.9	11.6	17.4
277	24.6	20.8	31.2

