

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE103118\
 Data File : BE098122.D
 Acq On : 31 Oct 2018 18:52
 Operator : SJ/JU
 Sample : J5701-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A40C0

Manual Integrations
 APPROVED

Sohil
 11/1/2018 11:08:03 AM

Quant Time: Nov 01 02:31:53 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 01 02:11:37 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.87	152	1043	0.40	ng/ul	0.00
2) Naphthalene-d8	10.67	136	4948	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	3643	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.28	188	7991m	0.40	ng/ul	0.00
16) Chrysene-d12	21.47	240	8744m	0.40	ng/ul	0.00
20) Perylene-d12	24.02	264	8056m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.27	152	3697	0.42	ng/ul	0.00
14) Fluoranthene-d10	19.31	212	10904m	0.42	ng/ul	0.00
Target Compounds						
8) Acenaphthene	14.61	153	1837	0.171	ng/ul#	24

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE103118\
Data File : BE098122.D
Acq On : 31 Oct 2018 18:52
Operator : SJ/JU
Sample : J5701-01
Misc :
ALS Vial : 10 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
A40C0

Quant Time: Nov 01 02:31:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 01 02:11:37 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
11/1/2018 11:08:03 AM

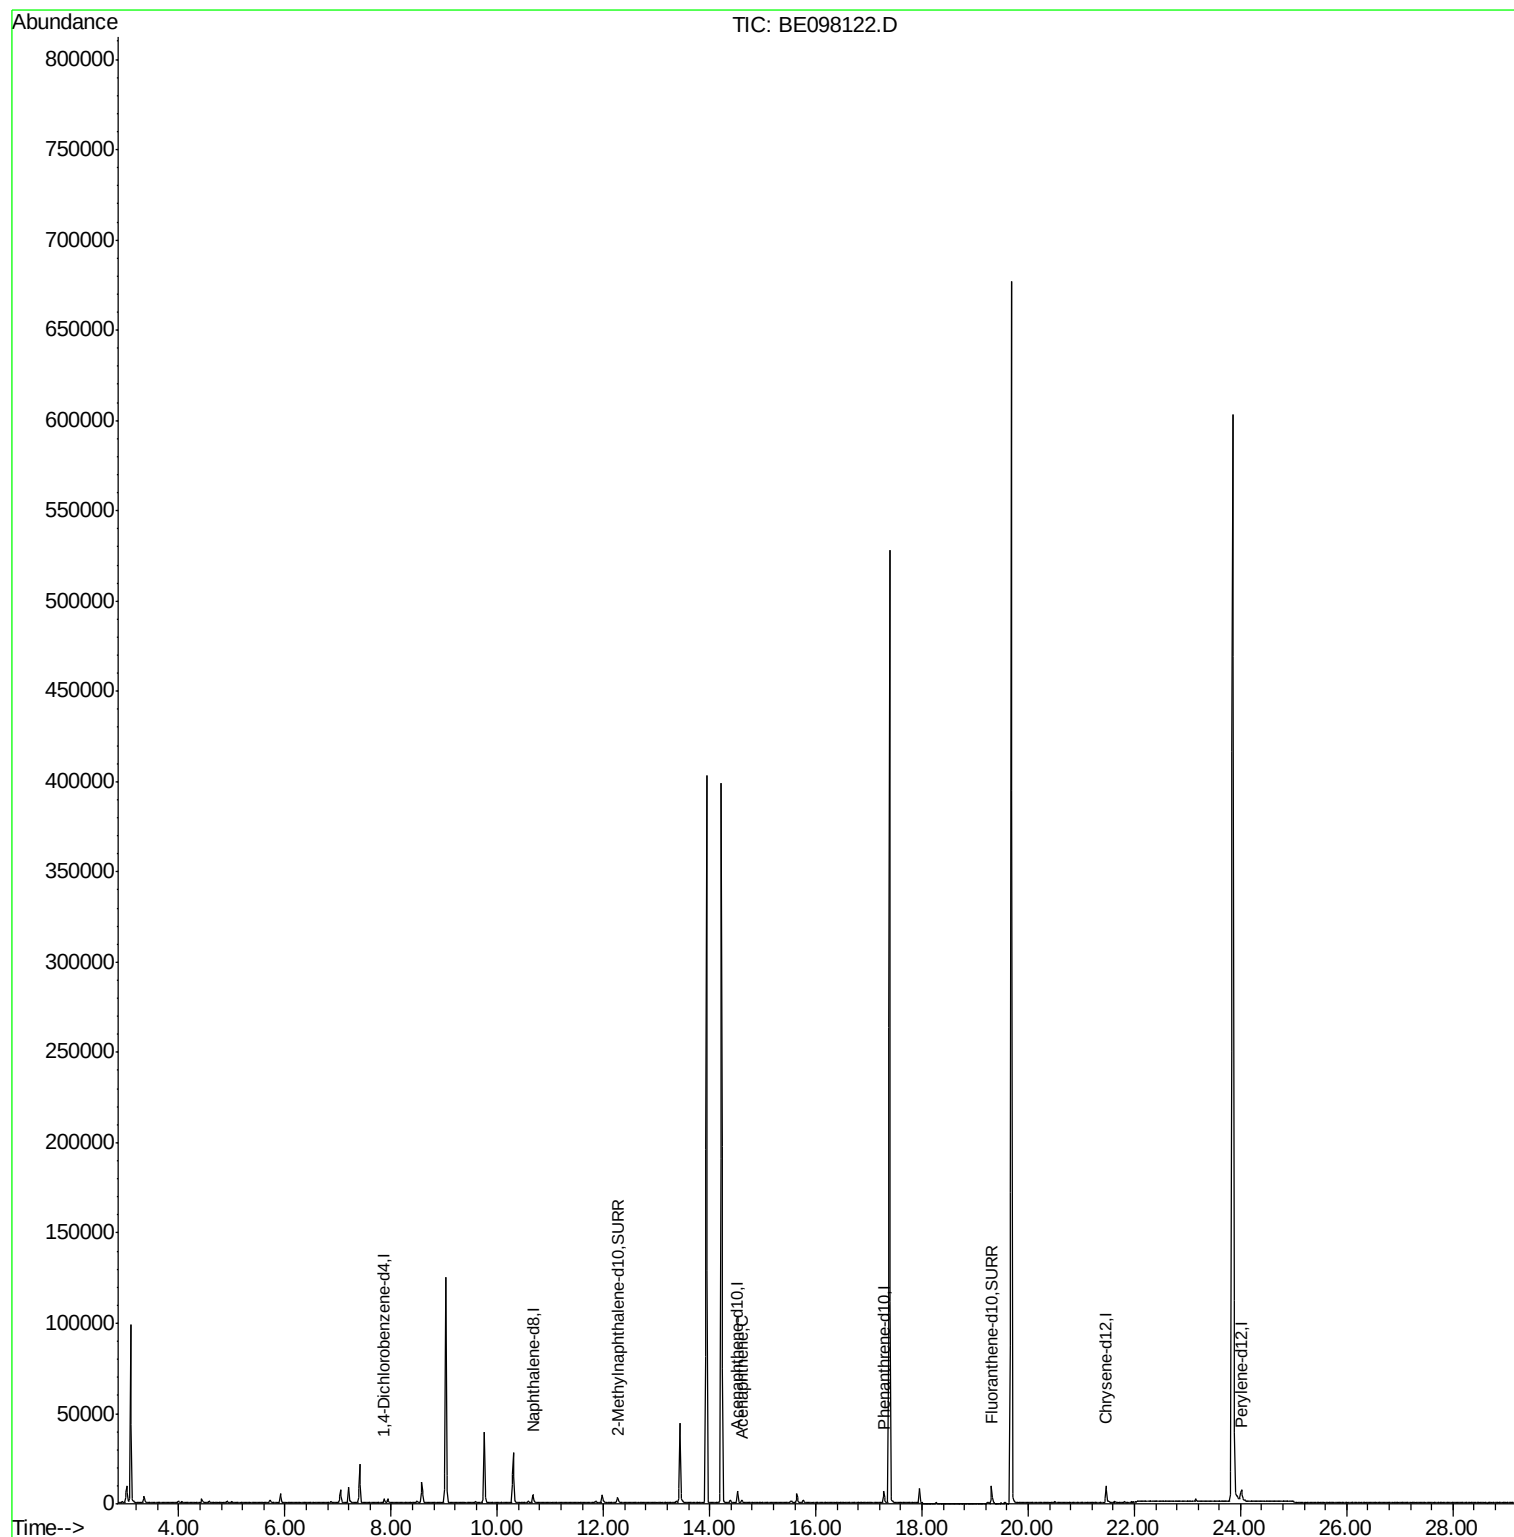

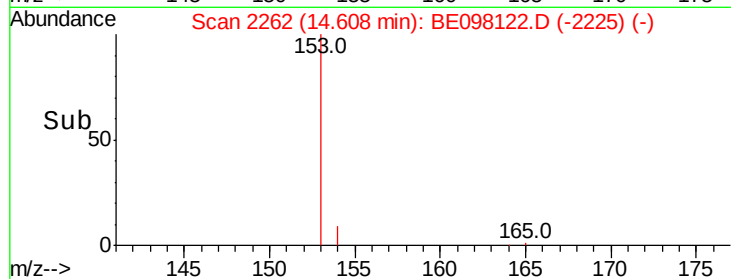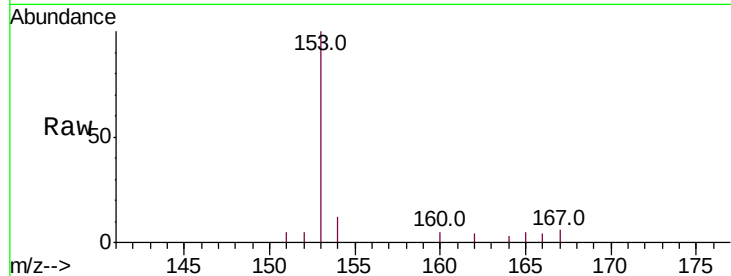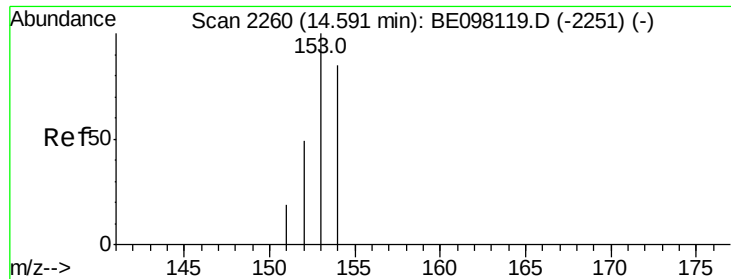

#8

Acenaphthene

Concen: 0.171 ng/ul

RT: 14.61 min Scan# 2262

Delta R.T. 0.02 min

Lab File: BE098122.D

Acq: 31 Oct 2018 18:52

Instrument :

BNA_E

ClientSampleId :

A40C0

Tot Ion:153 Resp: 1837

Ion Ratio Lower Upper

153 100

152 5.0 39.4 59.0#

154 11.8 70.5 105.7#

Manual Integrations

APPROVED

Sohil

11/1/2018 11:08:03 AM

