

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE103118\
 Data File : BE098123.D
 Acq On : 31 Oct 2018 19:31
 Operator : SJ/JU
 Sample : J5701-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A40C1

Manual Integrations
 APPROVED

Sohil
 11/1/2018 11:08:03 AM

Quant Time: Nov 01 02:34:21 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 01 02:11:37 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.87	152	996	0.40	ng/ul	0.00
2) Naphthalene-d8	10.67	136	4835	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	3638	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.29	188	8099m	0.40	ng/ul	0.00
16) Chrysene-d12	21.47	240	8561m	0.40	ng/ul	0.00
20) Perylene-d12	24.01	264	8028m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.27	152	3371	0.39	ng/ul	0.00
14) Fluoranthene-d10	19.32	212	9951m	0.38	ng/ul	0.00
Target Compounds						
8) Acenaphthene	14.61	153	1449	0.135	ng/ul#	Ovalue 26

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE103118\
Data File : BE098123.D
Acq On : 31 Oct 2018 19:31
Operator : SJ/JU
Sample : J5701-02
Misc :
ALS Vial : 11 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
A40C1

Quant Time: Nov 01 02:34:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 01 02:11:37 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
11/1/2018 11:08:03 AM



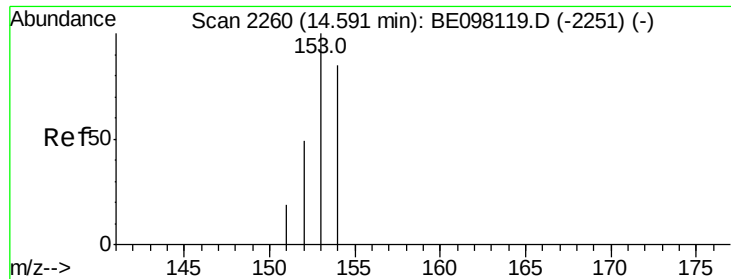

#8

Acenaphthene

Concen: 0.135 ng/ul

RT: 14.61 min Scan# 2262

Delta R.T. 0.02 min

Lab File: BE098123.D

Acq: 31 Oct 2018 19:31

Instrument :

BNA_E

ClientSampleId :

A40C1

Tot Ion:153 Resp: 1449

Ion Ratio Lower Upper

153 100

152 6.1 39.4 59.0#

154 13.2 70.5 105.7#

Manual Integrations

APPROVED

Sohil

11/1/2018 11:08:03 AM

