


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE110118\
Data File : BE098144.D
Acq On : 1 Nov 2018 13:40
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 11:02:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 01 13:00:52 2018
Response via : Initial Calibration

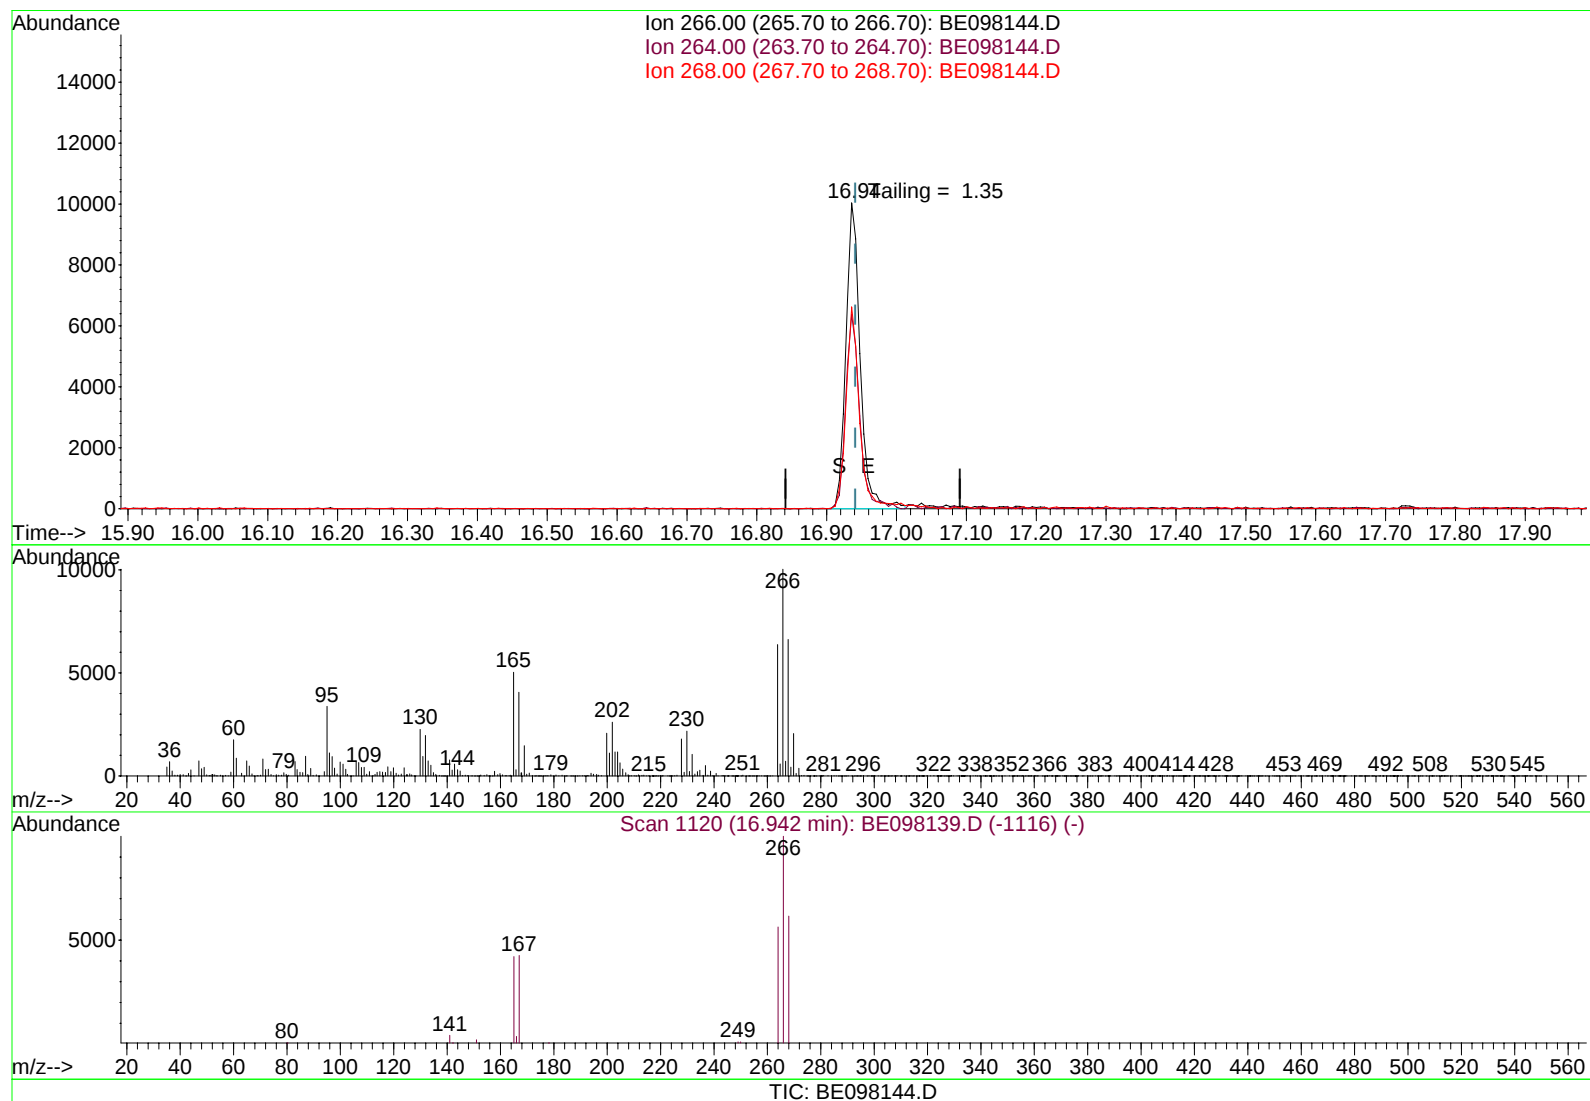

(22) Pentachlorophenol

16.936min (-0.005) 18695.53ng

response 14090

Ion	Exp%	Act%
266.00	100	100
264.00	64.10	63.51
268.00	62.60	65.99
0.00	0.00	0.00