


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE110118\
Data File : BE098136.D
Acq On : 1 Nov 2018 8:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE110118.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 01 13:00:52 2018

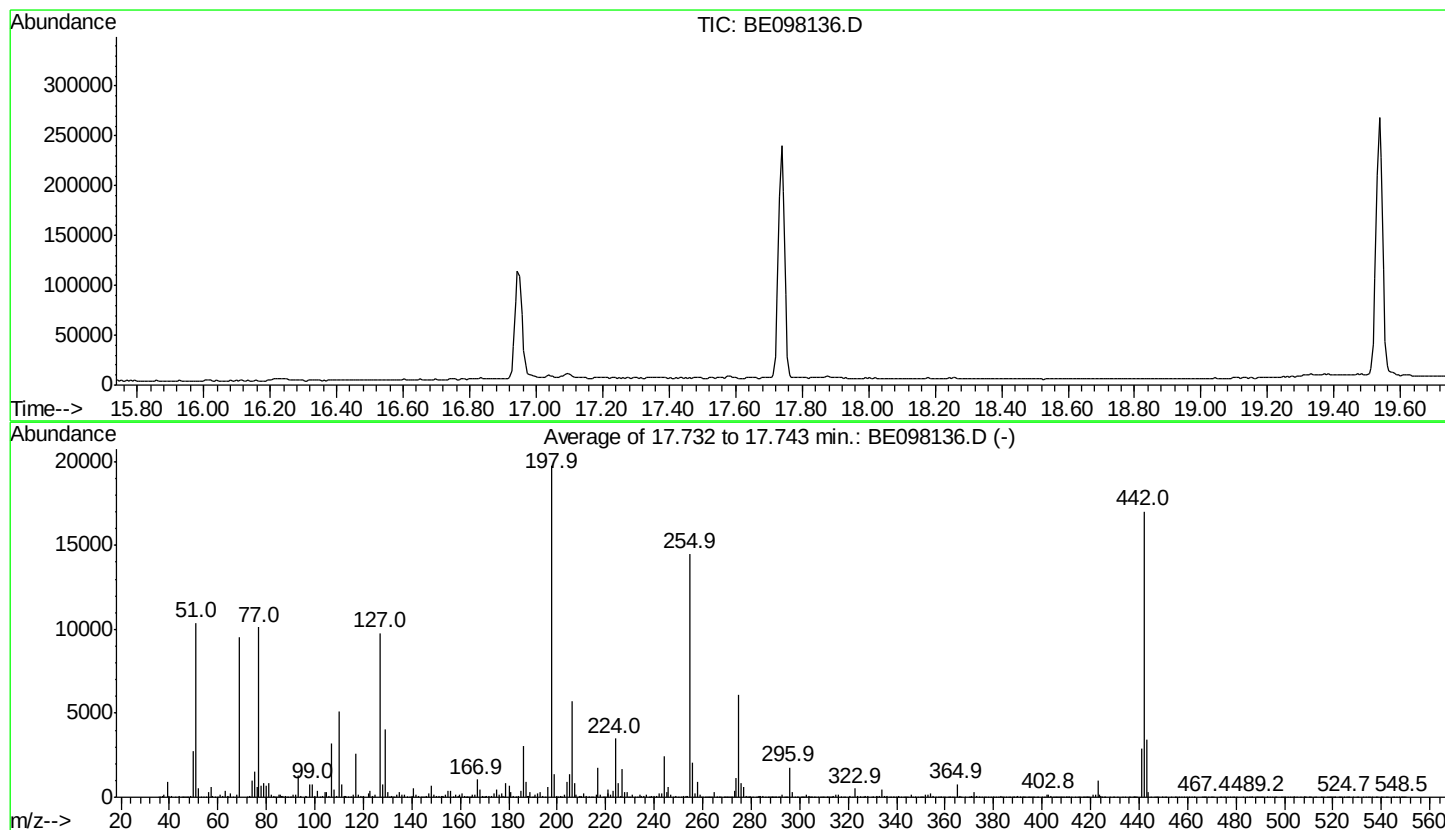

AutoFind: Scans 2577, 2578, 2579; Background Corrected with Scan 2570

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.6	10399	PASS
68	69	0.00	2	1.7	162	PASS
69	198	0.00	100	48.1	9501	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.5	9774	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19757	PASS
199	198	5	9	7.1	1401	PASS
275	198	10	60	30.8	6085	PASS
365	198	1	100	4.0	784	PASS
441	198	0.01	100	14.7	2913	PASS
442	198	50	100	86.3	17044	PASS
443	442	15	24	20.2	3446	PASS