


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE110118\
 Data File : BE098144.D
 Acq On : 1 Nov 2018 13:40
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE110118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 01 13:00:52 2018

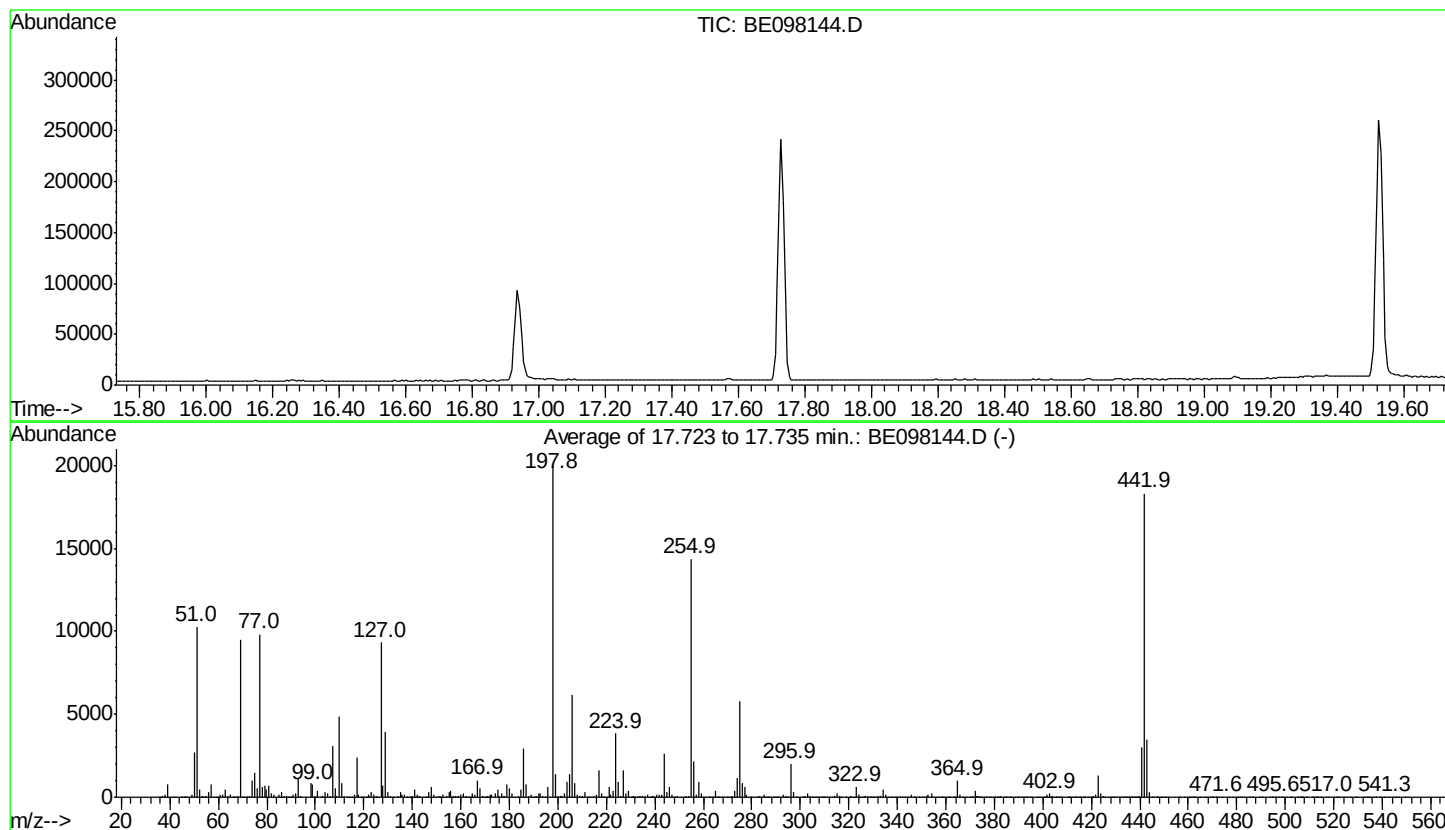

AutoFind: Scans 2576, 2577, 2578; Background Corrected with Scan 2569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.4	10273	PASS
68	69	0.00	2	0.5	52	PASS
69	198	0.00	100	47.5	9493	PASS
70	69	0.00	2	0.4	39	PASS
127	198	10	80	46.7	9337	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19995	PASS
199	198	5	9	7.1	1427	PASS
275	198	10	60	29.0	5808	PASS
365	198	1	100	4.9	989	PASS
441	198	0.01	100	15.1	3010	PASS
442	198	50	100	91.6	18313	PASS
443	442	15	24	19.1	3501	PASS