


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE110518\
Data File : BE098152.D
Acq On : 5 Nov 2018 9:05
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE110118.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 01 13:00:52 2018

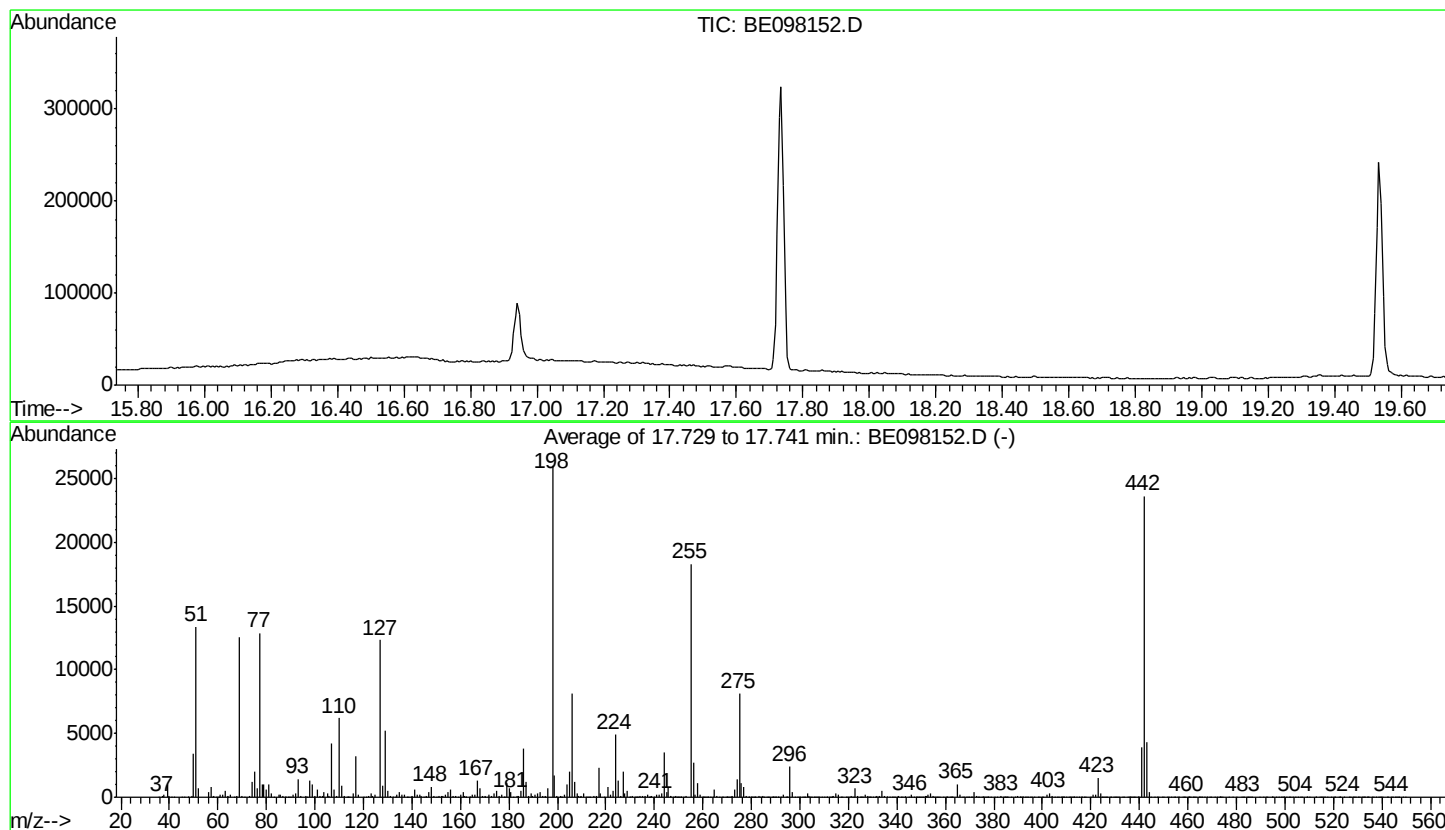

AutoFind: Scans 2577, 2578, 2579; Background Corrected with Scan 2569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.5	13382	PASS
68	69	0.00	2	0.9	112	PASS
69	198	0.00	100	48.1	12504	PASS
70	69	0.00	2	0.8	100	PASS
127	198	10	80	47.4	12324	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26008	PASS
199	198	5	9	6.5	1687	PASS
275	198	10	60	31.2	8115	PASS
365	198	1	100	4.0	1036	PASS
441	198	0.01	100	15.0	3914	PASS
442	198	50	100	90.8	23626	PASS
443	442	15	24	18.1	4284	PASS