


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE110718\
Data File : BE098164.D
Acq On : 7 Nov 2018 9:04
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE110118.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 01 13:00:52 2018

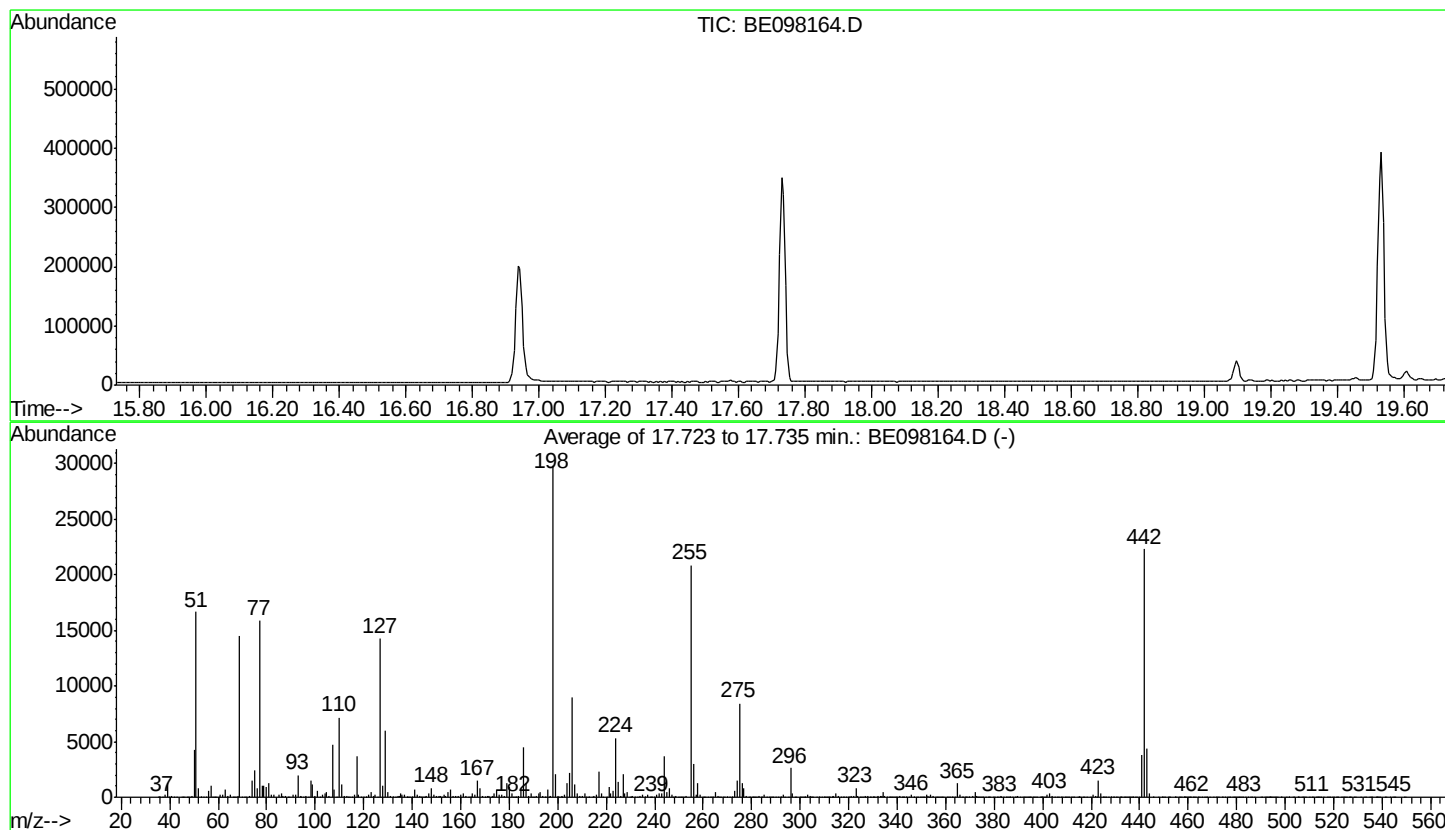

AutoFind: Scans 2576, 2577, 2578; Background Corrected with Scan 2569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.9	16659	PASS
68	69	0.00	2	0.7	106	PASS
69	198	0.00	100	48.7	14535	PASS
70	69	0.00	2	0.4	53	PASS
127	198	10	80	47.8	14269	PASS
197	198	0.00	2	0.2	65	PASS
198	198	100	100	100.0	29823	PASS
199	198	5	9	7.0	2096	PASS
275	198	10	60	28.2	8417	PASS
365	198	1	100	4.1	1223	PASS
441	198	0.01	100	12.7	3774	PASS
442	198	50	100	74.7	22290	PASS
443	442	15	24	19.5	4337	PASS