


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE110719\
 Data File : BE100699.D
 Acq On : 7 Nov 2019 13:18
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE101019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 23 16:49:33 2019

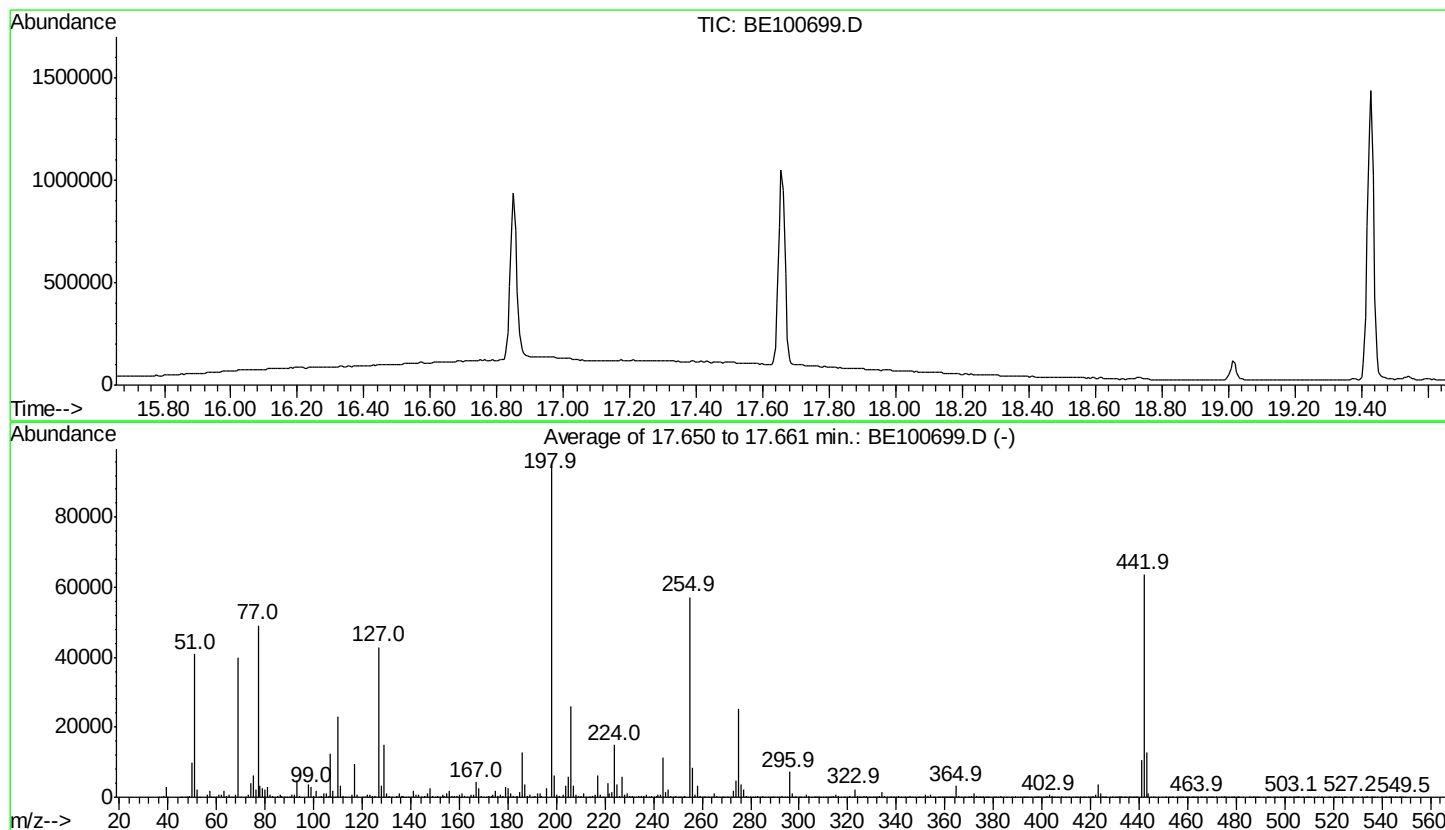

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	40927	PASS
68	69	0.00	2	1.5	604	PASS
69	198	0.00	100	42.1	39886	PASS
70	69	0.00	2	0.5	192	PASS
127	198	10	80	45.2	42835	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	94757	PASS
199	198	5	9	6.5	6189	PASS
275	198	10	60	26.8	25376	PASS
365	198	1	100	3.3	3152	PASS
441	198	0.01	100	11.1	10524	PASS
442	198	50	100	67.0	63501	PASS
443	442	15	24	20.0	12686	PASS