


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE110818\
Data File : BE098178.D
Acq On : 8 Nov 2018 8:53
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE110118.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 01 13:00:52 2018

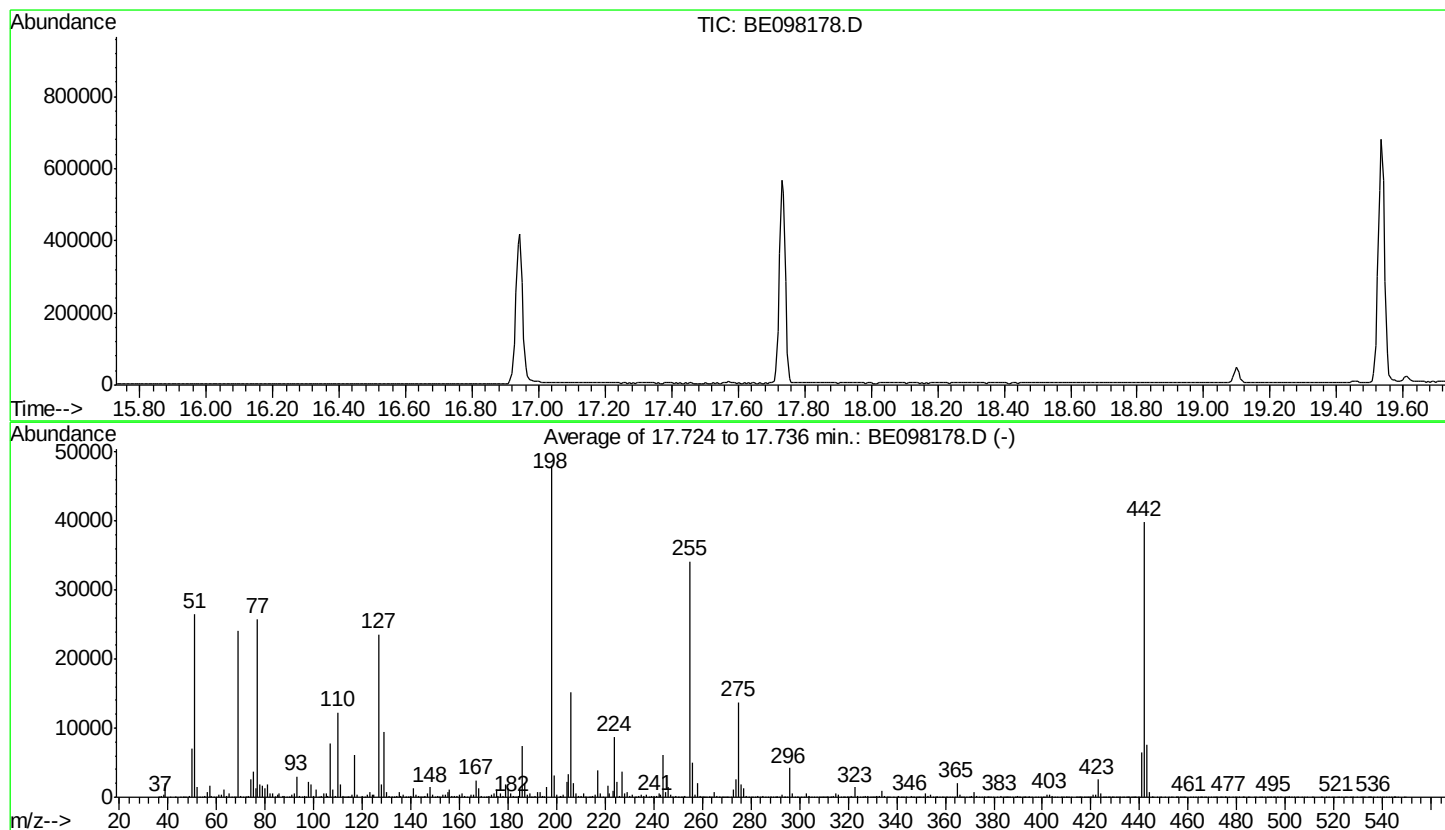

AutoFind: Scans 2576, 2577, 2578; Background Corrected with Scan 2568

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.3	26530	PASS
68	69	0.00	2	0.4	98	PASS
69	198	0.00	100	50.3	24153	PASS
70	69	0.00	2	0.5	120	PASS
127	198	10	80	49.2	23631	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48002	PASS
199	198	5	9	6.5	3107	PASS
275	198	10	60	28.7	13786	PASS
365	198	1	100	4.4	2089	PASS
441	198	0.01	100	13.4	6420	PASS
442	198	50	100	83.0	39853	PASS
443	442	15	24	19.2	7653	PASS