
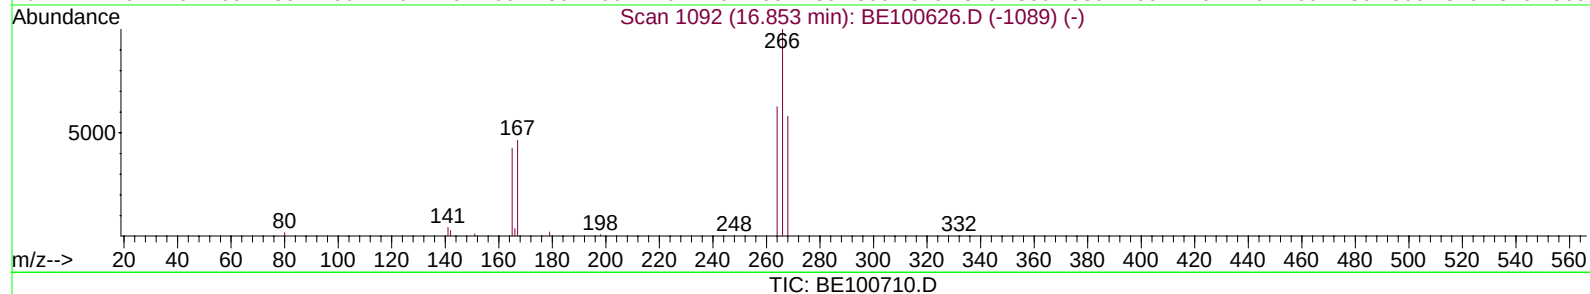
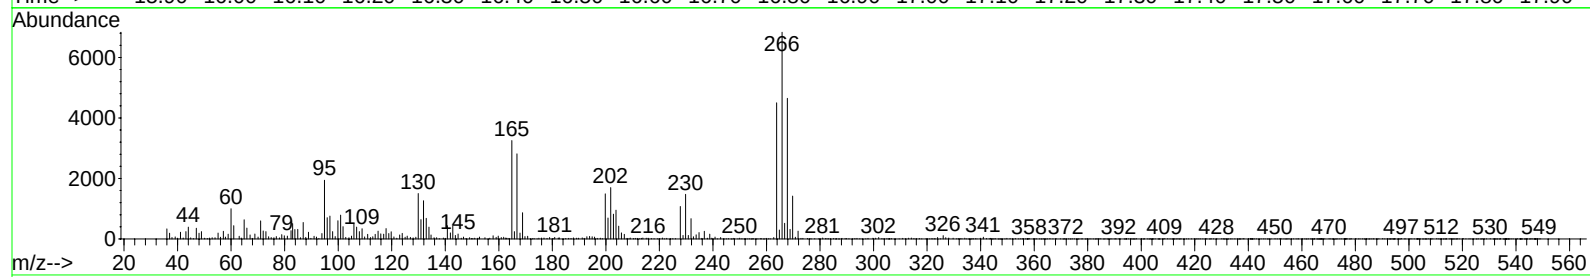


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE110819\  
Data File : BE100710.D  
Acq On : 8 Nov 2019 10:12  
Operator : JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 08 12:35:06 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE101019.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Oct 23 16:49:33 2019  
Response via : Initial Calibration

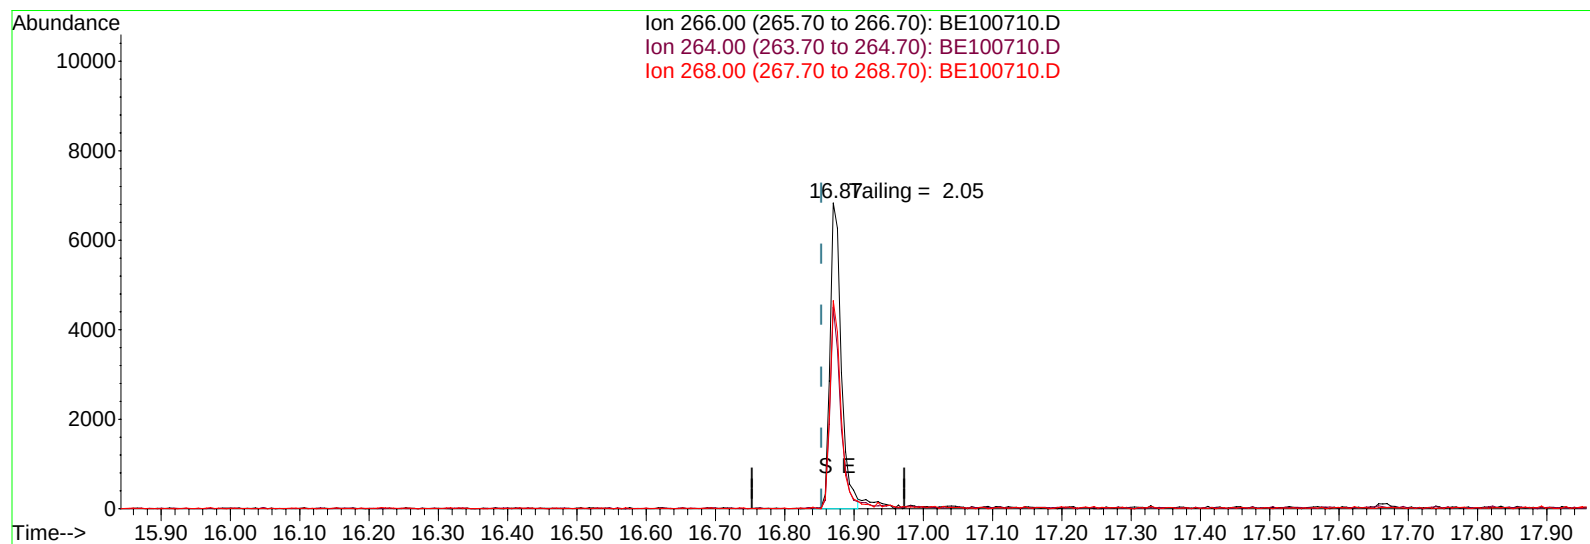

TIC: BE100710.D

(22) Pentachlorophenol

16.870min (+0.017) 3694.52ng

response 8078

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 266.00 | 100   | 100   |
| 264.00 | 65.30 | 65.90 |
| 268.00 | 66.40 | 68.04 |
| 0.00   | 0.00  | 0.00  |