


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE110819\
Data File : BE100710.D
Acq On : 8 Nov 2019 10:12
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE101019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 23 16:49:33 2019

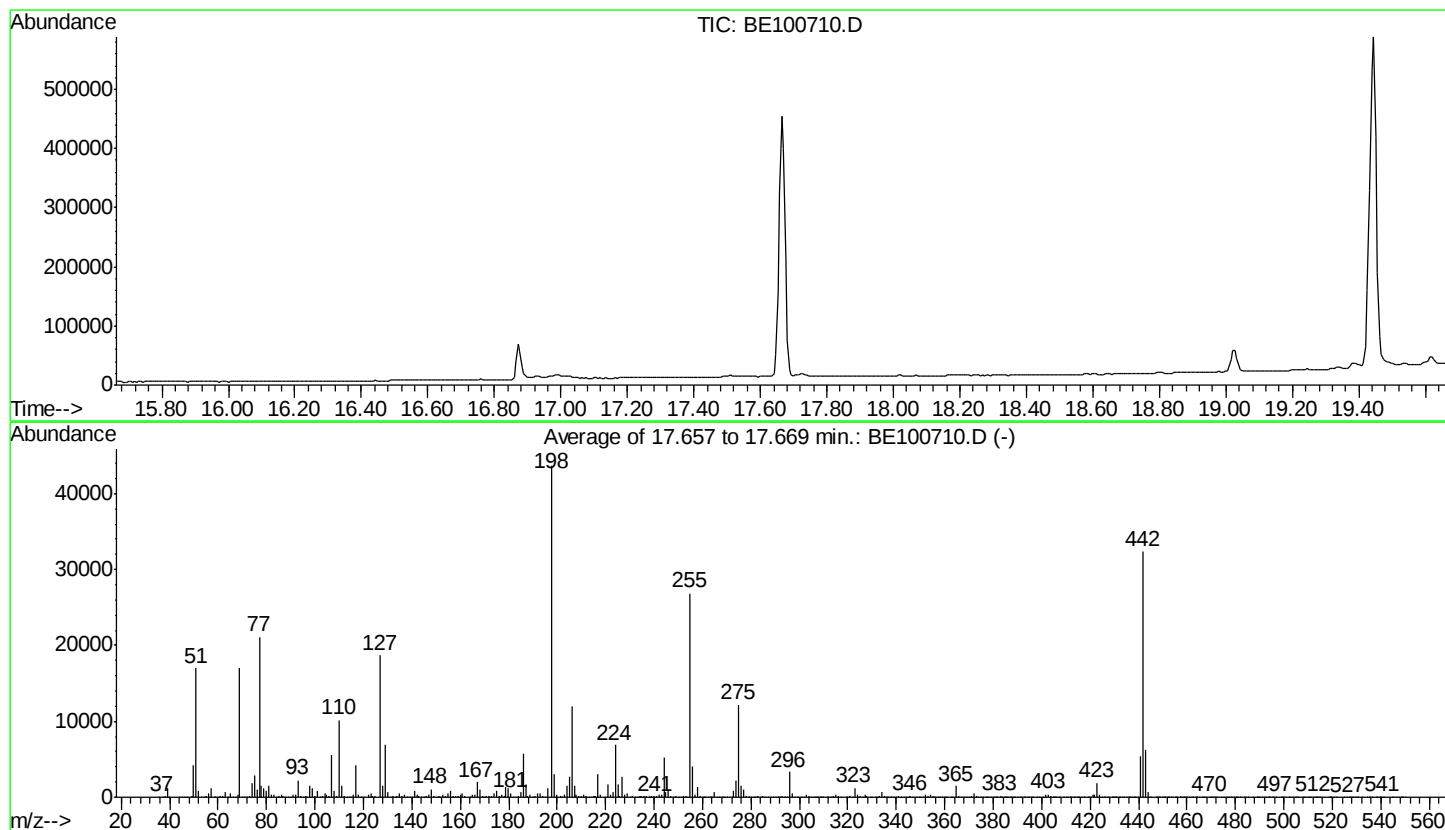

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	16982	PASS
68	69	0.00	2	1.8	301	PASS
69	198	0.00	100	39.1	17103	PASS
70	69	0.00	2	0.5	84	PASS
127	198	10	80	42.8	18686	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	43694	PASS
199	198	5	9	6.8	2984	PASS
275	198	10	60	27.9	12184	PASS
365	198	1	100	3.3	1463	PASS
441	198	0.01	100	12.2	5341	PASS
442	198	50	100	74.1	32356	PASS
443	442	15	24	19.5	6313	PASS