
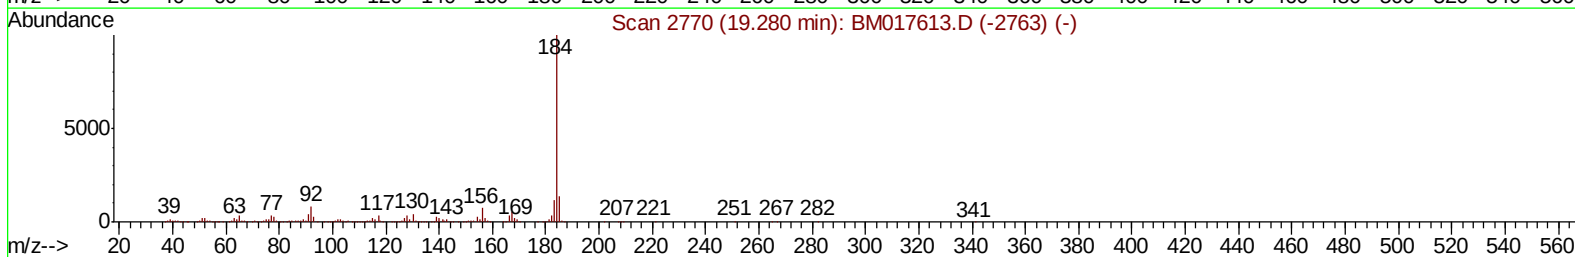
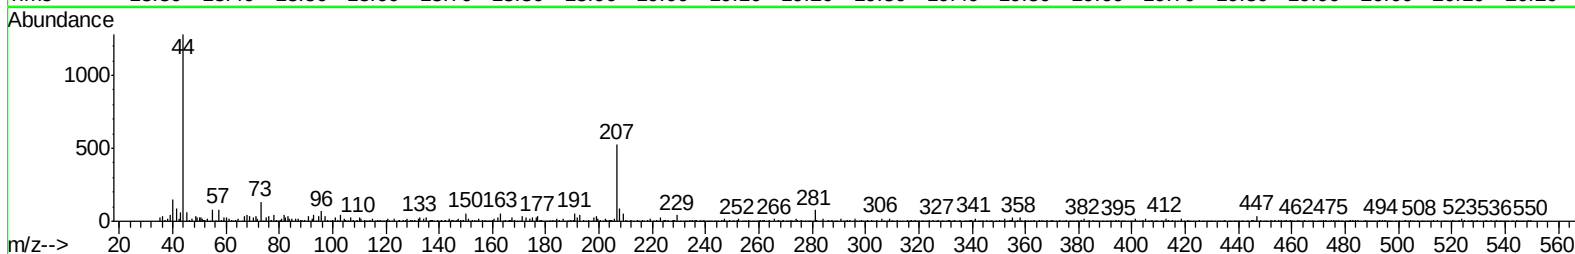


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111218\
Data File : BE098182.D
Acq On : 12 Nov 2018 9:17
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 13 08:09:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 12 18:37:25 2018
Response via : Initial Calibration

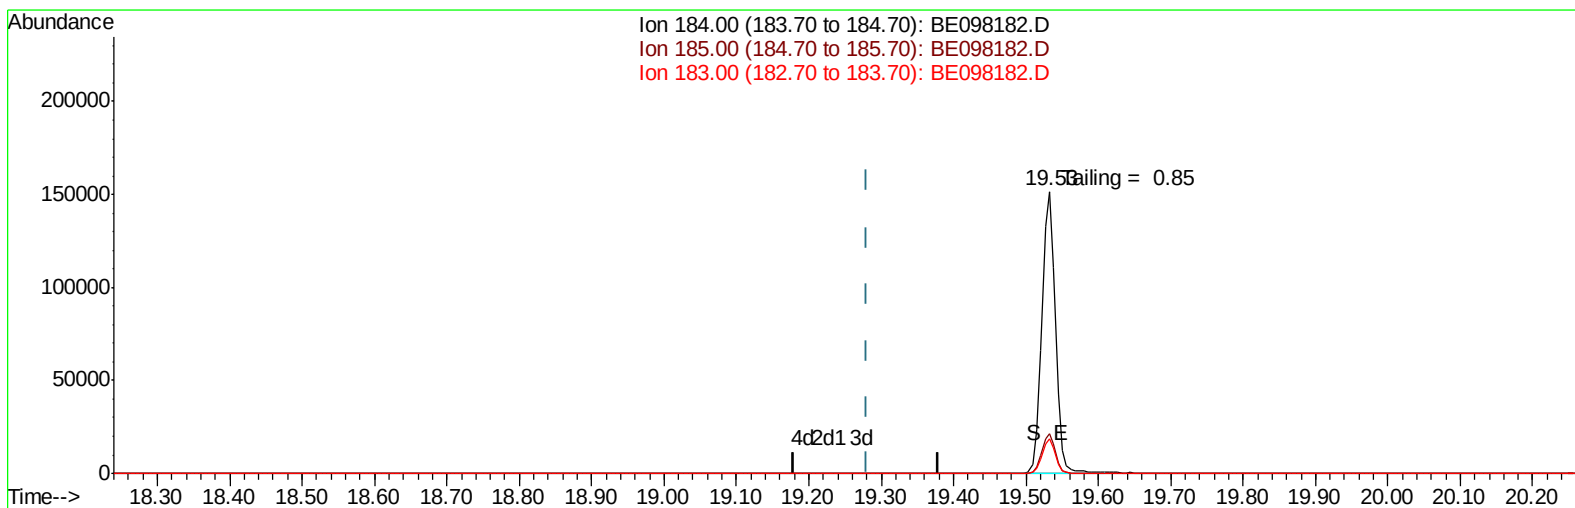

TIC: BE098182.D

(77) Benzidine




19.245min (-0.035) 13.65ng

response 8

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	56.25#
183.00	11.90	62.50#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111218\
 Data File : BE098182.D
 Acq On : 12 Nov 2018 9:17
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 13 08:09:22 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 12 18:37:25 2018
 Response via : Initial Calibration

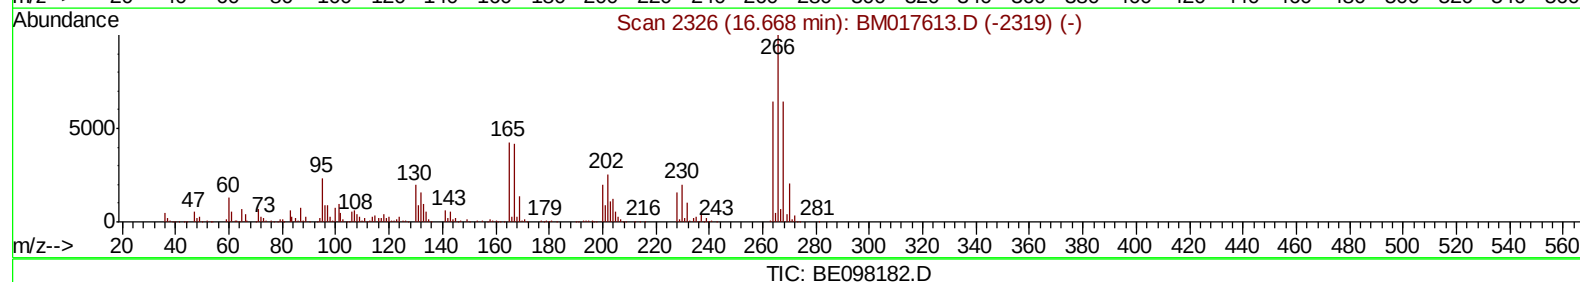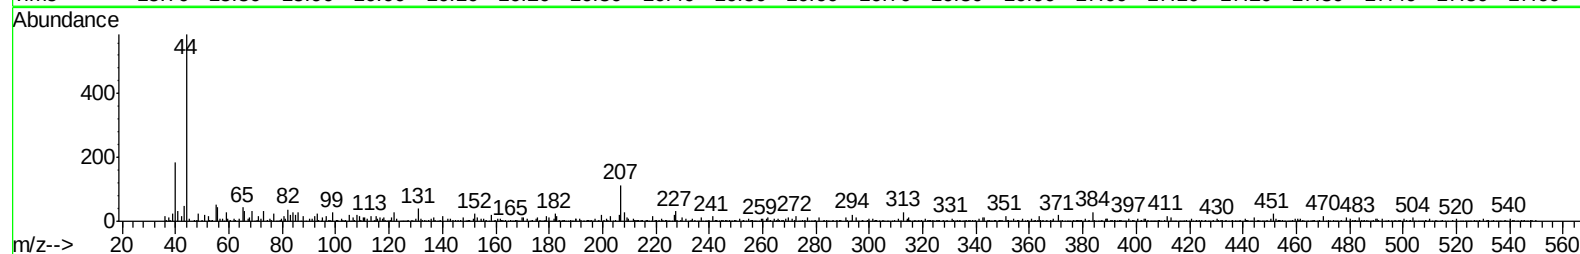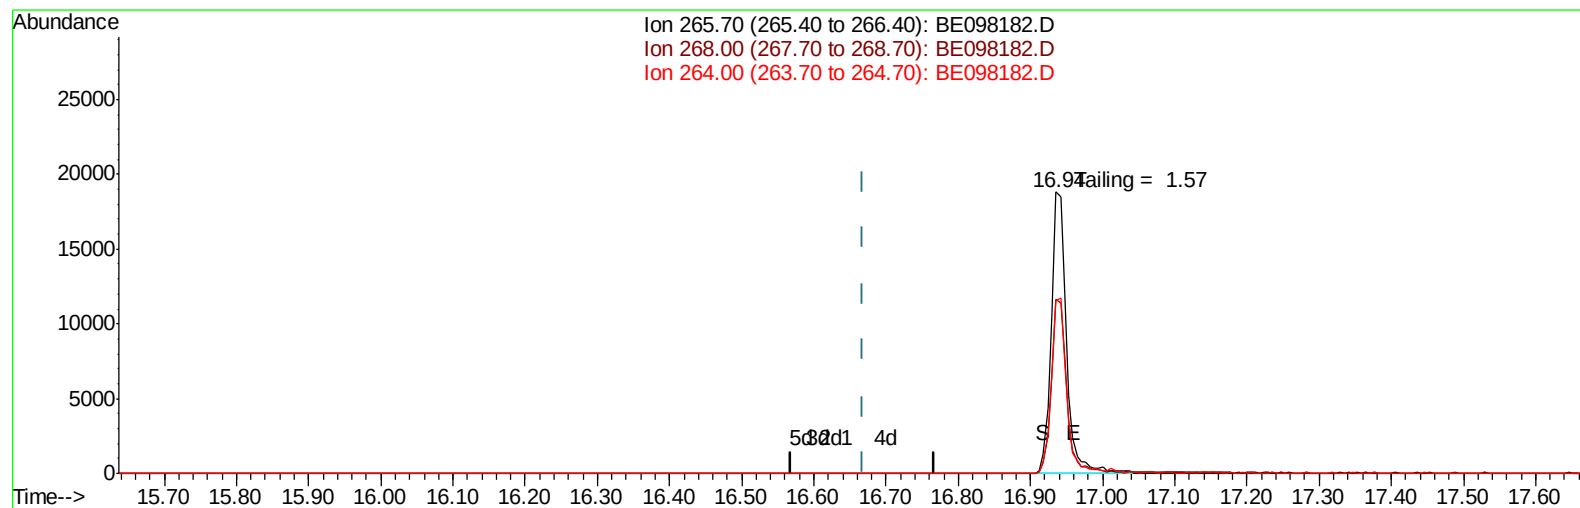

TIC: BE098182.D

(70) Pentachlorophenol (C)

16.648min (-0.021) 75.56ng

response 12

Ion	Exp%	Act%
265.70	100	100
268.00	64.60	25.00#
264.00	64.10	75.00
0.00	0.00	0.00