


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE111218\
 Data File : BE098182.D
 Acq On : 12 Nov 2018 9:17
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE111218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 12 13:32:15 2018

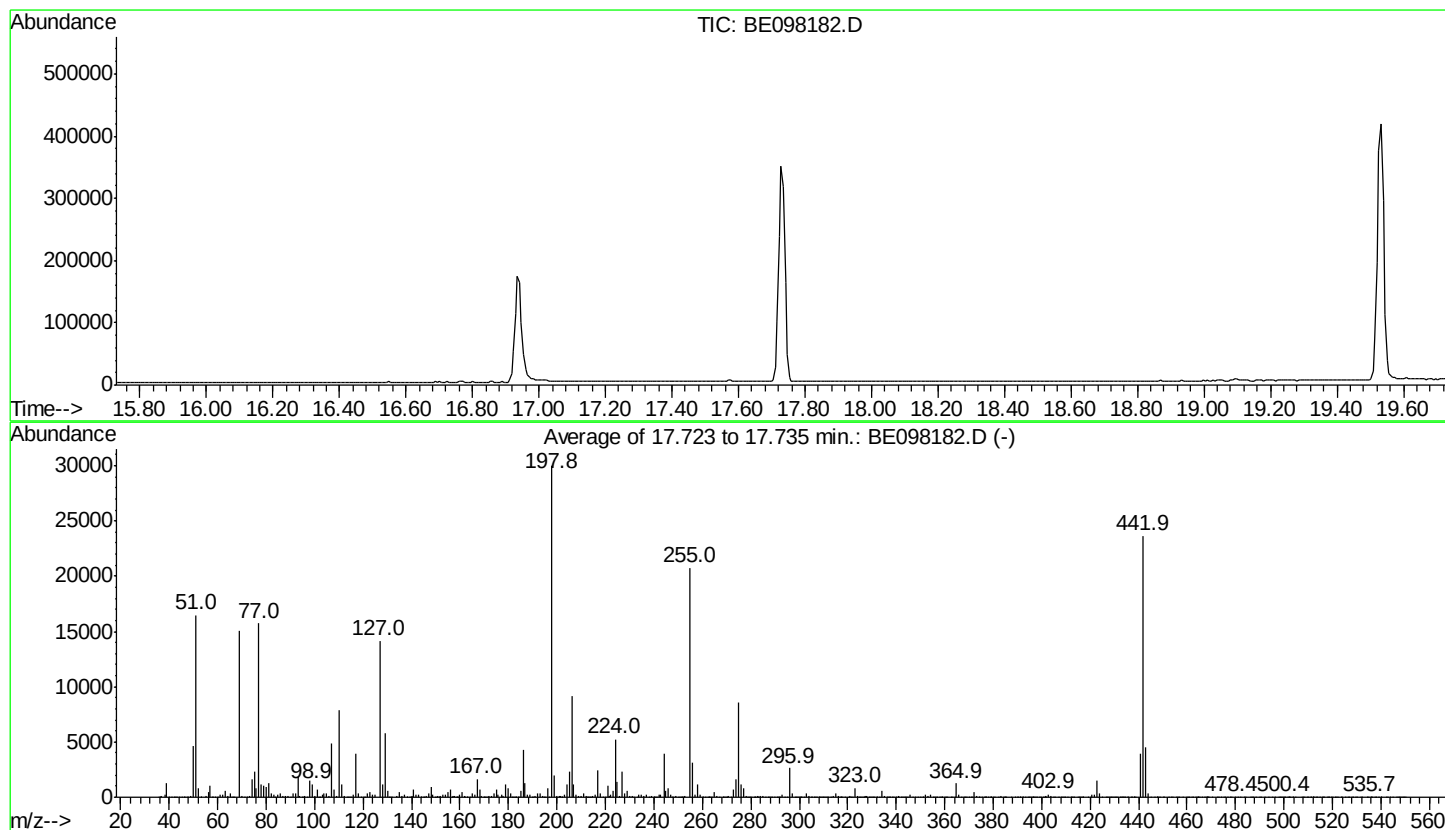

AutoFind: Scans 2576, 2577, 2578; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.0	16493	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	50.2	15056	PASS
70	69	0.00	2	0.5	75	PASS
127	198	10	80	47.1	14139	PASS
197	198	0.00	2	0.2	55	PASS
198	198	100	100	100.0	30007	PASS
199	198	5	9	6.7	2002	PASS
275	198	10	60	28.5	8552	PASS
365	198	1	100	4.2	1260	PASS
441	198	0.01	100	13.0	3888	PASS
442	198	50	100	78.9	23689	PASS
443	442	15	24	19.3	4563	PASS