
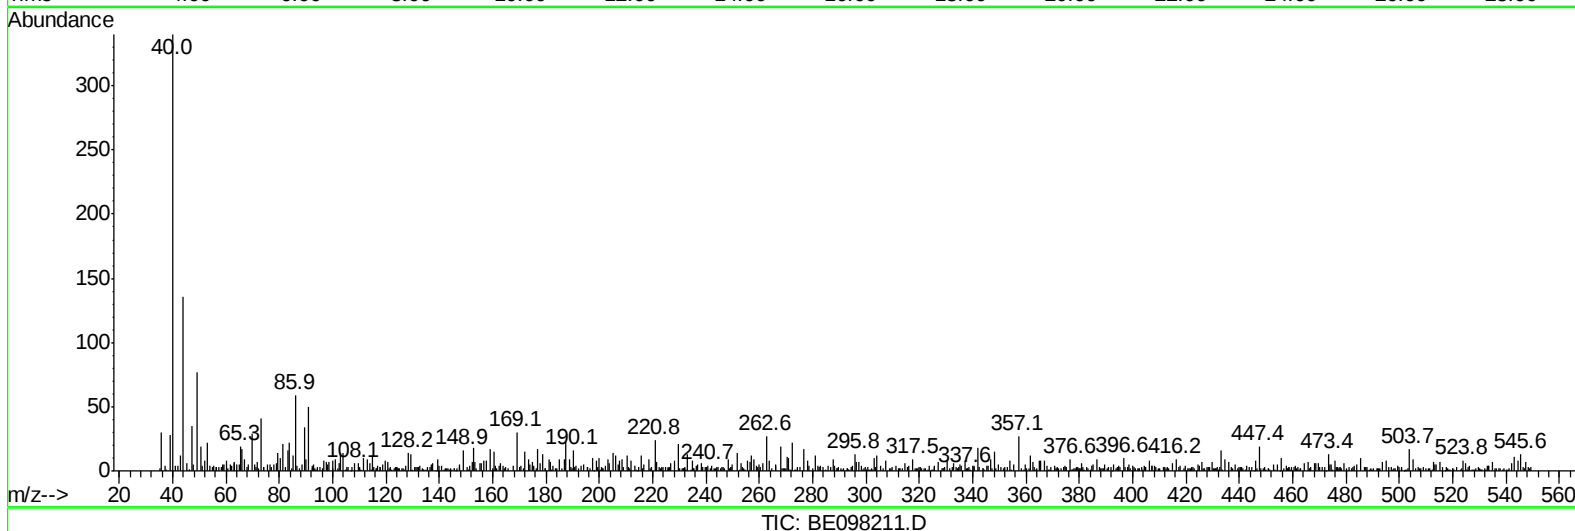


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE111318\
Data File : BE098211.D
Acq On : 13 Nov 2018 16:22
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 00:52:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 12:43:10 2018
Response via : Initial Calibration

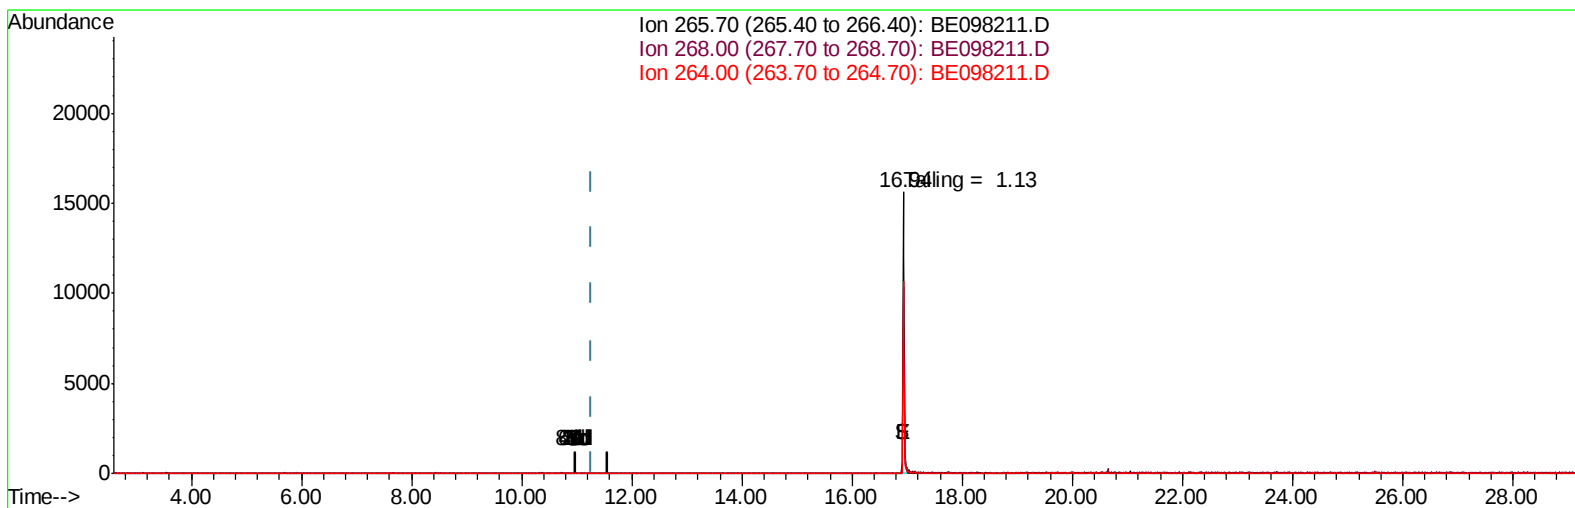

(70) Pentachlorophenol (C)



10.978min (-0.309) 43.86ng

response 6

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	233.33#
264.00	63.20	111.11#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE111318\
Data File : BE098211.D
Acq On : 13 Nov 2018 16:22
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 00:52:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 12:43:10 2018
Response via : Initial Calibration

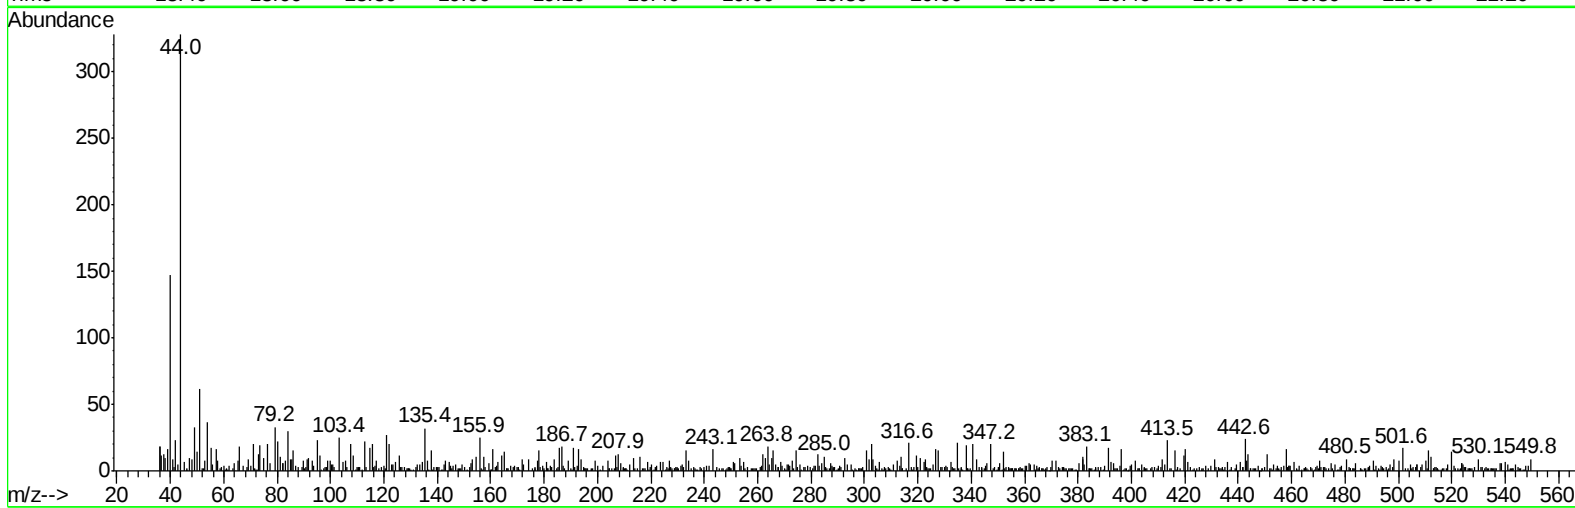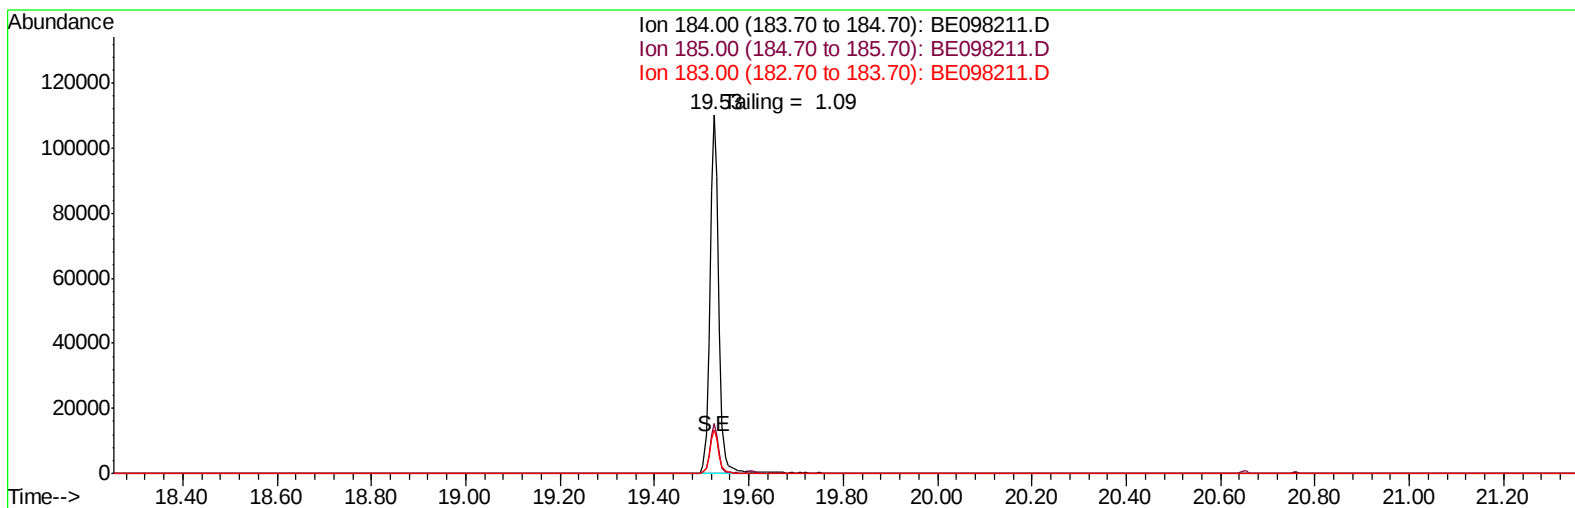

TIC: BE098211.D

(77) Benzidine

12.464min (-0.357) 22.73ng

response 5

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	27.27#
183.00	11.80	27.27#
0.00	0.00	0.00