


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE111318\
 Data File : BE098207.D
 Acq On : 13 Nov 2018 9:52
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE111218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 12 13:32:15 2018

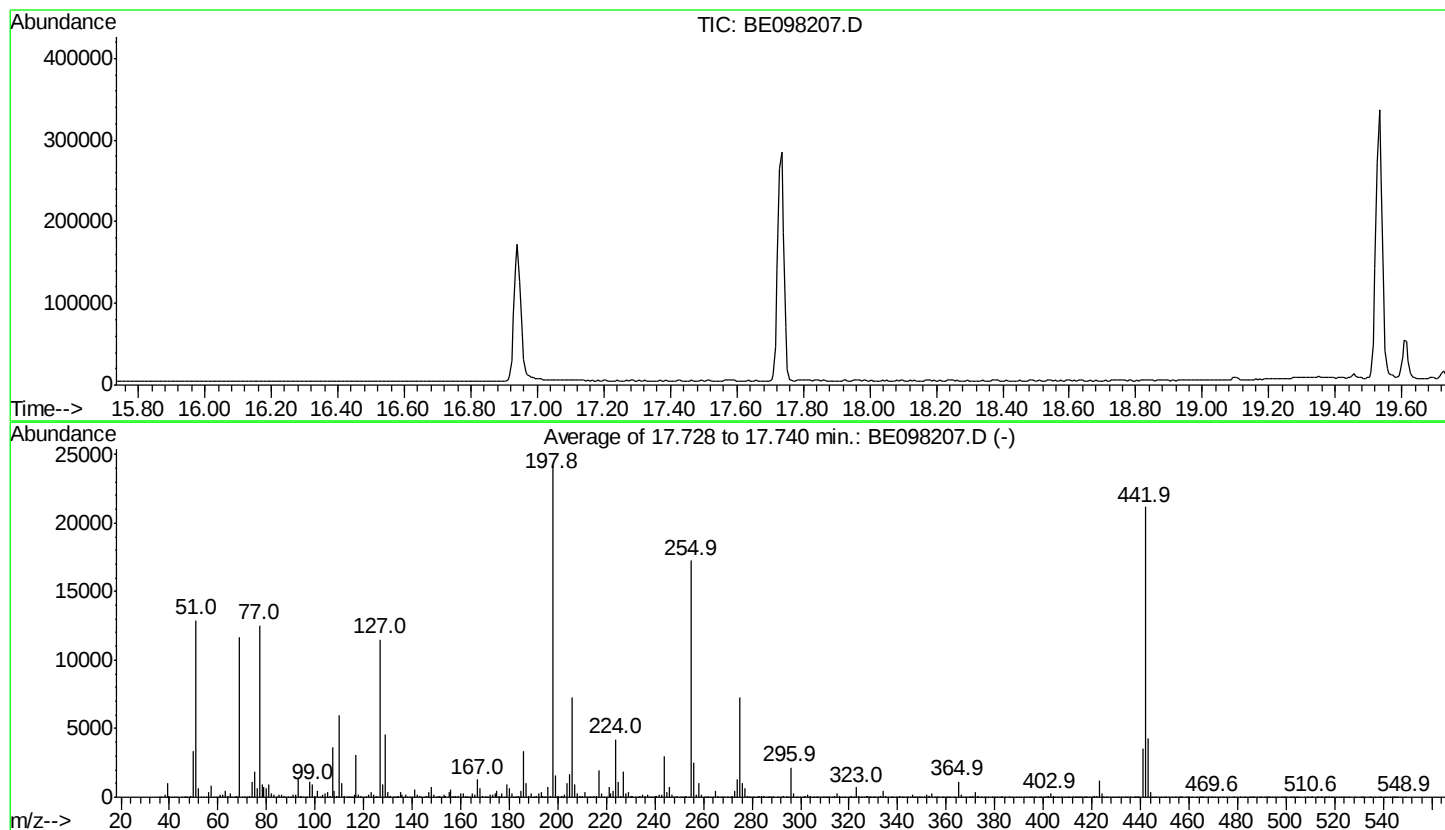

AutoFind: Scans 2577, 2578, 2579; Background Corrected with Scan 2568

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.5	12931	PASS
68	69	0.00	2	1.0	114	PASS
69	198	0.00	100	48.4	11712	PASS
70	69	0.00	2	0.1	15	PASS
127	198	10	80	47.6	11514	PASS
197	198	0.00	2	0.3	79	PASS
198	198	100	100	100.0	24184	PASS
199	198	5	9	6.6	1602	PASS
275	198	10	60	30.0	7262	PASS
365	198	1	100	4.7	1137	PASS
441	198	0.01	100	14.8	3582	PASS
442	198	50	100	87.6	21188	PASS
443	442	15	24	20.2	4282	PASS