
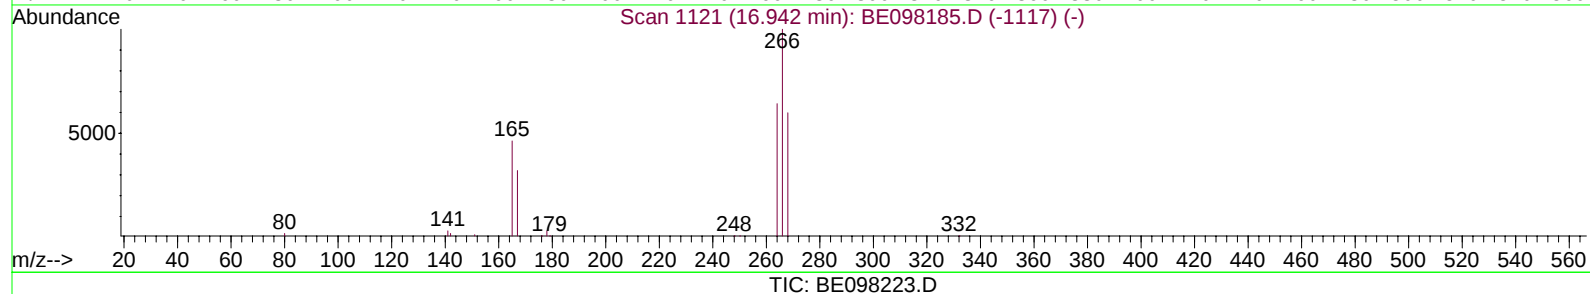
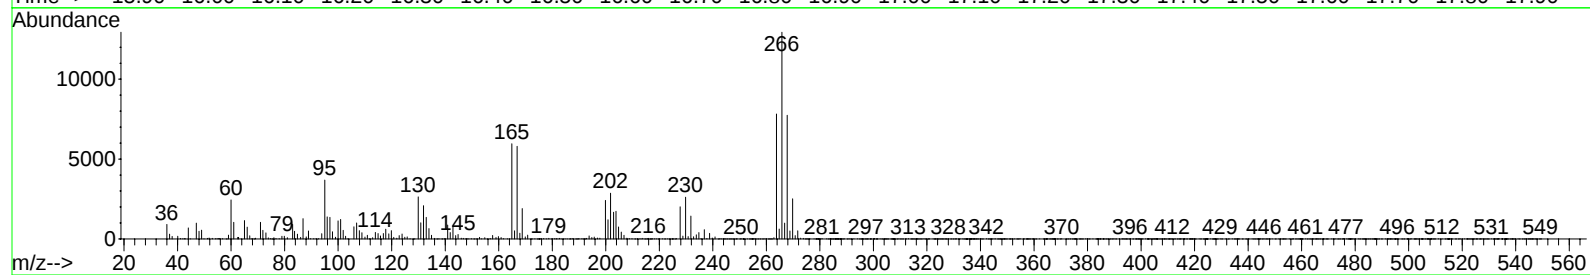


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE111418\
Data File : BE098223.D
Acq On : 14 Nov 2018 13:45
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 17:18:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 12 13:32:15 2018
Response via : Initial Calibration

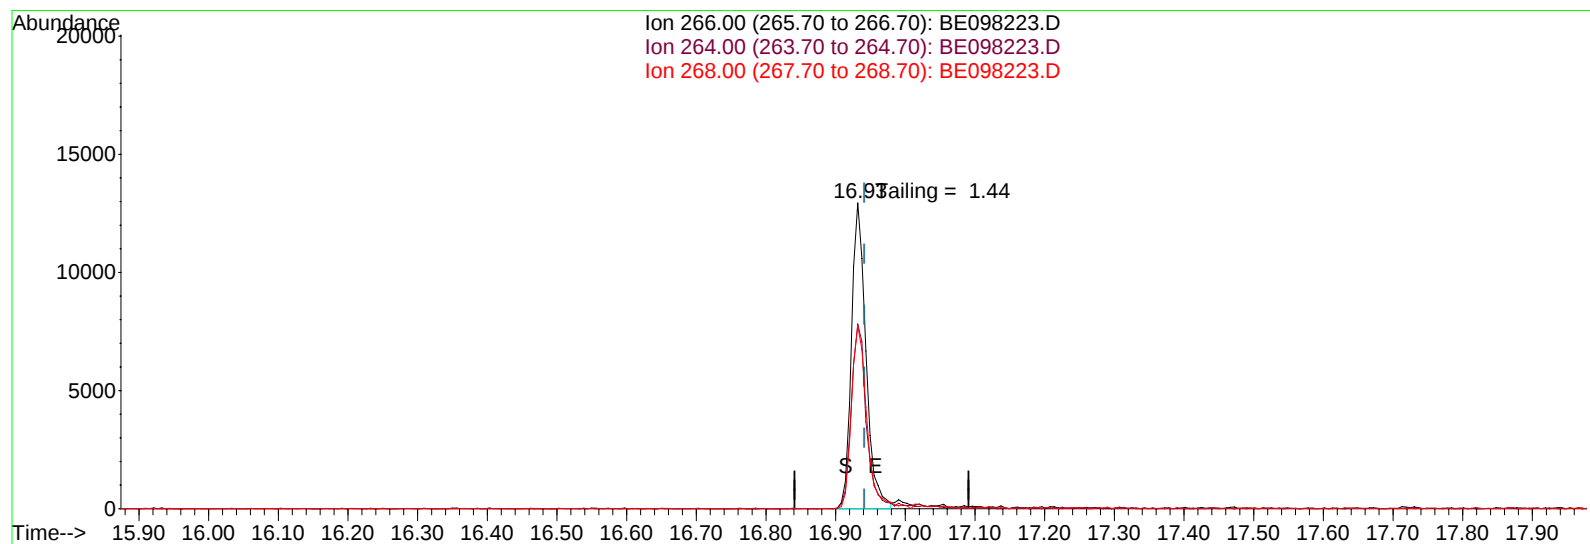

(22) Pentachlorophenol

16.932min (-0.009) 4559.47ng

response 18674

Ion	Exp%	Act%
266.00	100	100
264.00	72.00	60.47
268.00	71.00	59.84
0.00	0.00	0.00