


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE111418\
Data File : BE098223.D
Acq On : 14 Nov 2018 13:45
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE111218.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Nov 12 13:32:15 2018

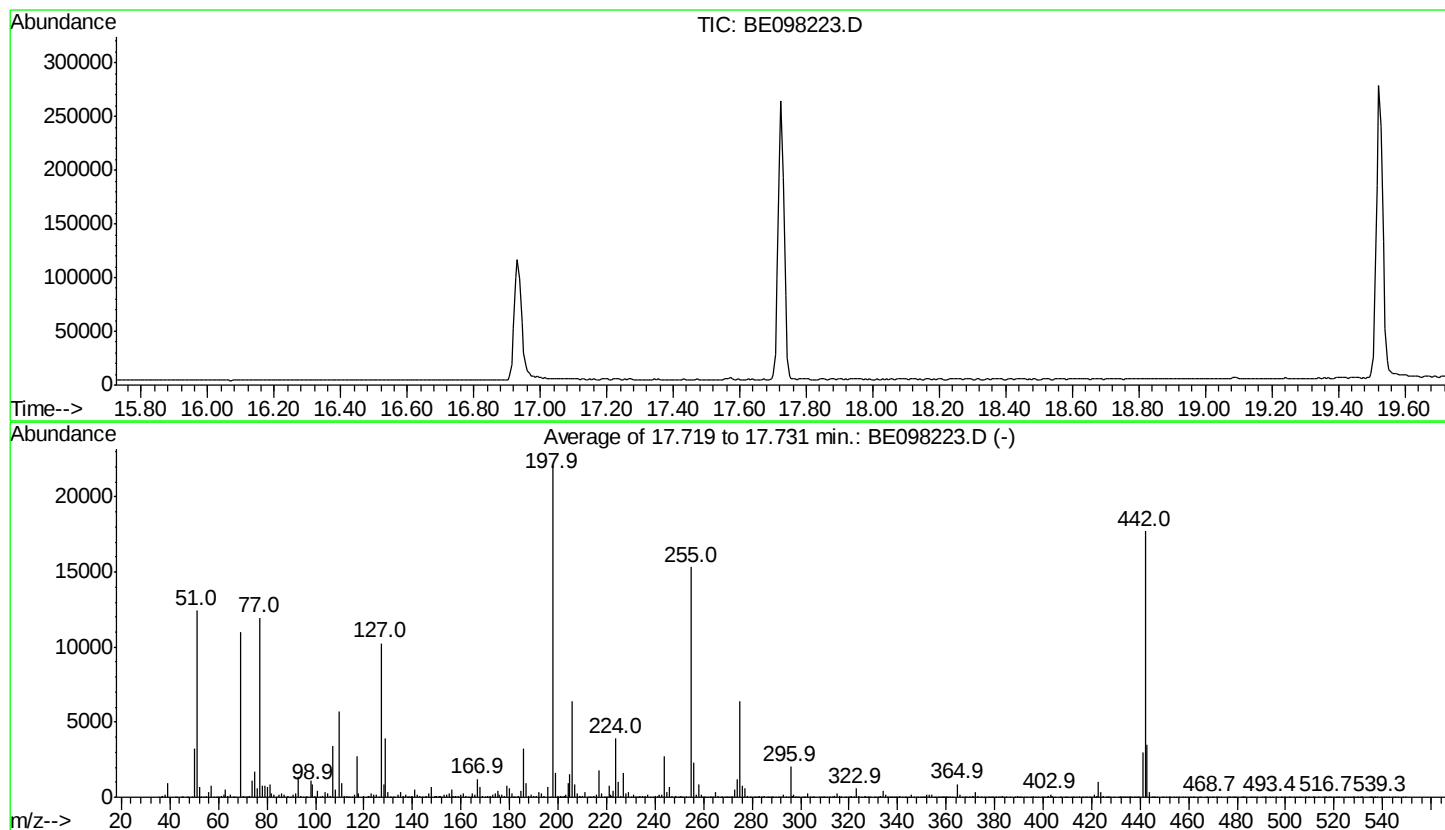

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.3	12434	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	49.7	10977	PASS
70	69	0.00	2	0.7	72	PASS
127	198	10	80	46.4	10250	PASS
197	198	0.00	2	0.2	42	PASS
198	198	100	100	100.0	22088	PASS
199	198	5	9	7.2	1599	PASS
275	198	10	60	28.8	6359	PASS
365	198	1	100	3.9	858	PASS
441	198	0.01	100	13.6	3007	PASS
442	198	50	100	80.2	17718	PASS
443	442	15	24	19.7	3499	PASS