
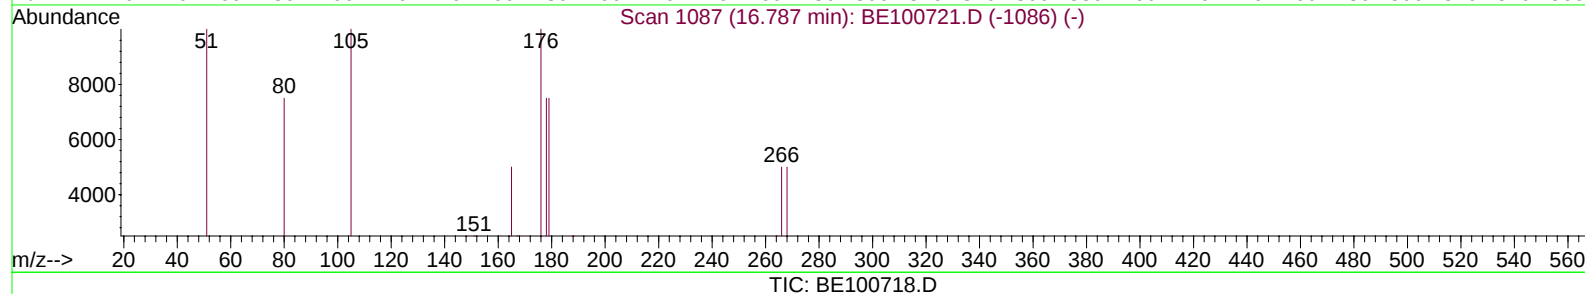
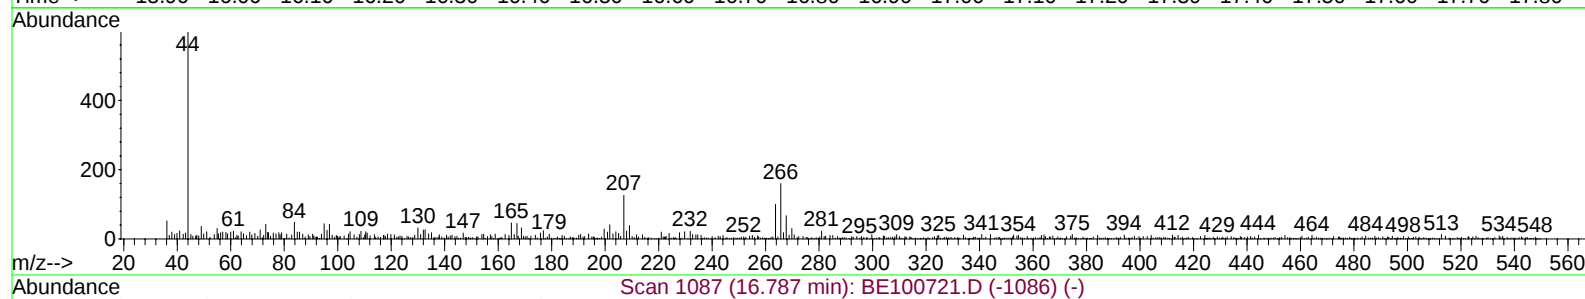


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE111419\
Data File : BE100718.D
Acq On : 14 Nov 2019 12:52
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 18:05:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE111419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 14 16:59:41 2019
Response via : Initial Calibration

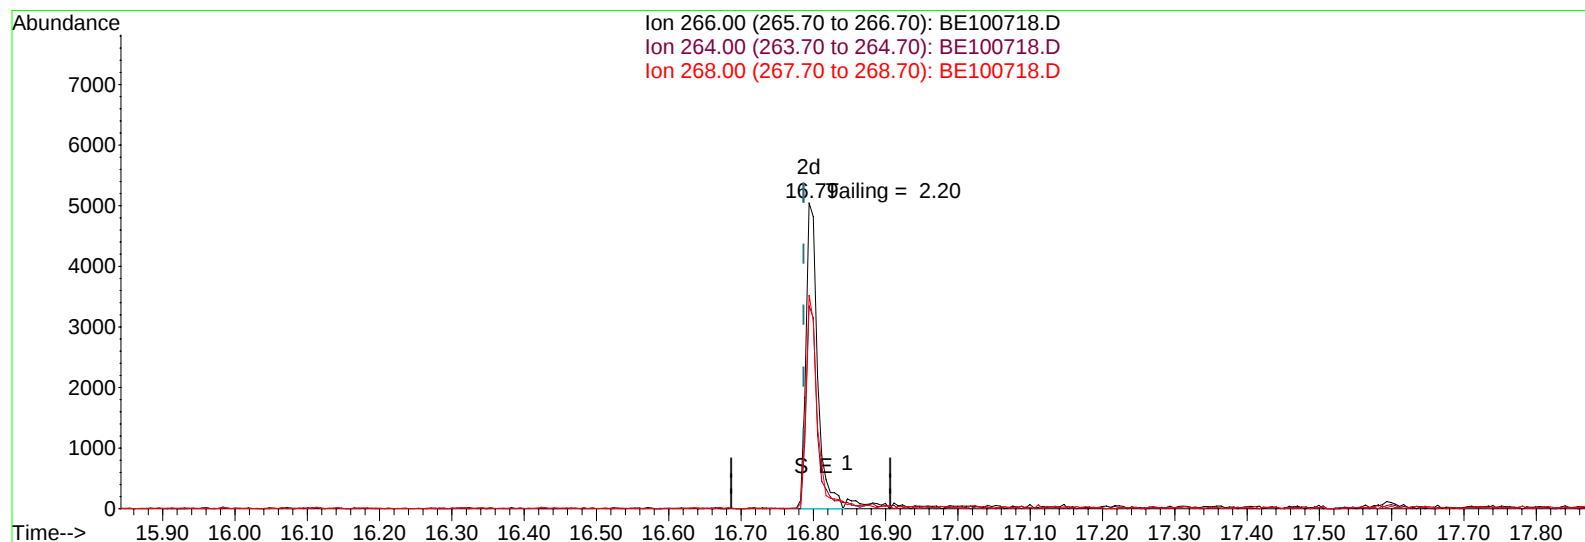

(22) Pentachlorophenol

16.847min (+0.060) 144.42ng

response 203

Ion	Exp%	Act%
266.00	100	100
264.00	93.80	59.55#
268.00	106.30	37.64#
0.00	0.00	0.00