


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE111419\
 Data File : BE100718.D
 Acq On : 14 Nov 2019 12:52
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE111419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 15 15:55:40 2019

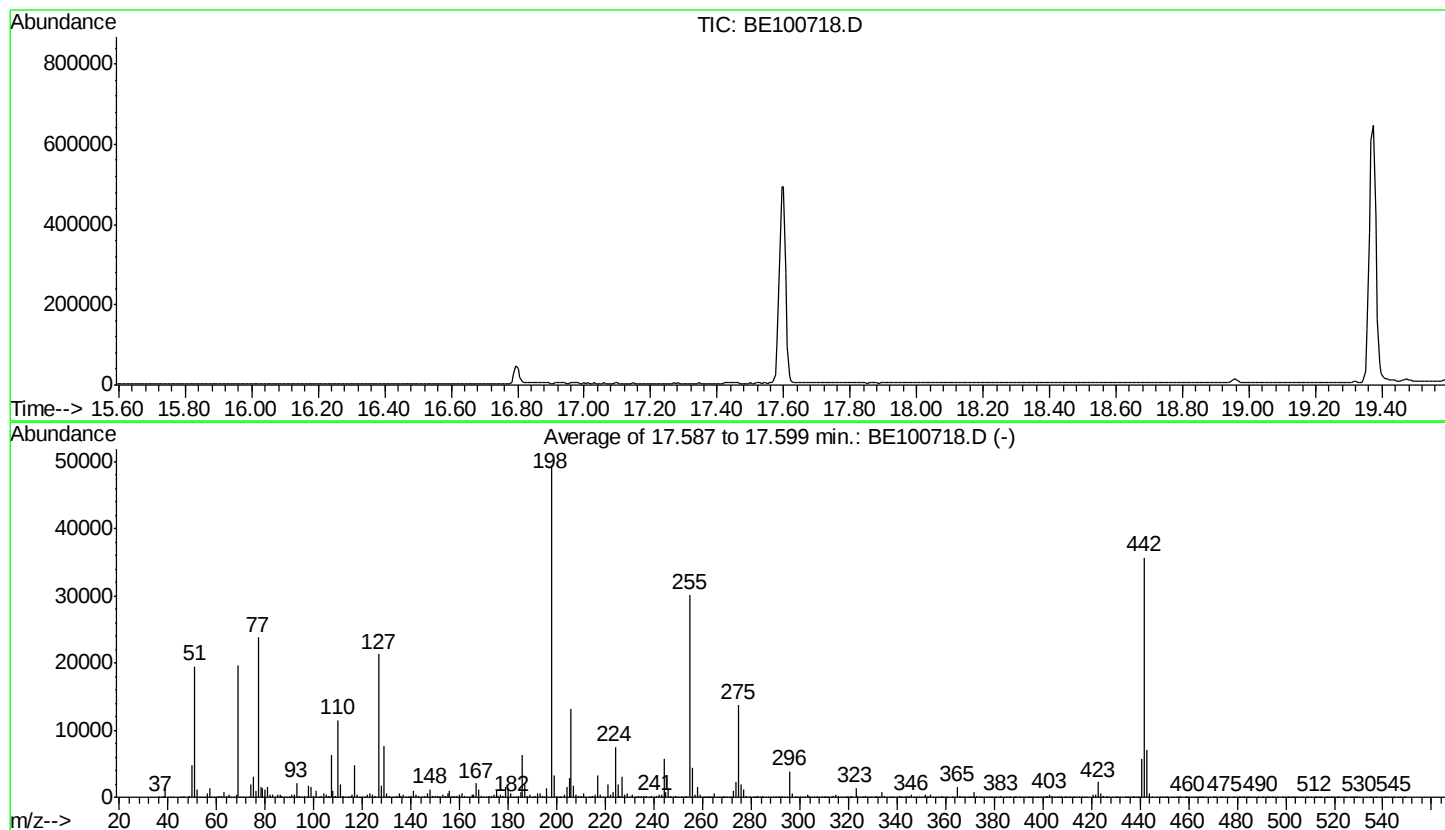

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2542

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	19505	PASS
68	69	0.00	2	1.7	335	PASS
69	198	0.00	100	39.8	19663	PASS
70	69	0.00	2	0.5	101	PASS
127	198	10	80	43.1	21276	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49351	PASS
199	198	5	9	6.7	3291	PASS
275	198	10	60	27.8	13730	PASS
365	198	1	100	3.2	1587	PASS
441	198	0.01	100	11.5	5679	PASS
442	198	50	100	72.3	35695	PASS
443	442	15	24	19.9	7098	PASS