

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE111519\
 Data File : BE100743.D
 Acq On : 15 Nov 2019 18:46
 Operator : JU
 Sample : K5728-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 EXT-034-SW093-110619-4

Manual Integrations
 APPROVED

mohammad
 11/18/2019 3:05:39 PM

Quant Time: Nov 15 23:19:40 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE111419.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Nov 15 15:55:40 2019

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	3481	0.40	ng	0.00
7) Naphthalene-d8	10.55	136	14950	0.40	ng	0.00
13) Acenaphthene-d10	14.40	164	9786	0.40	ng	-0.01
19) Phenanthrene-d10	17.13	188	21604	0.40	ng	0.00
27) Chrysene-d12	21.29	240	22757	0.40	ng	0.00
34) Perylene-d12	23.73	264	25215	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.36	112	2868	0.28	ng	0.00
5) Phenol-d6	6.94	99	4537	0.32	ng	0.00
8) Nitrobenzene-d5	8.91	82	3059	0.24	ng	0.00
11) 2-Methylnaphthalene-d10	12.15	152	5943	0.25	ng	0.00
14) 2,4,6-Tribromophenol	15.89	330	386	0.50	ng	0.00
15) 2-Fluorobiphenyl	13.03	172	7892	0.22	ng	0.00
25) Fluoranthene-d10	19.16	212	61472	0.22	ng	0.00
29) Terphenyl-d14	19.75	244	11361	0.21	ng	0.00
Target Compounds						Qvalue
9) Naphthalene	10.60	128	8573	0.055	ng	98
12) 2-Methylnaphthalene	12.22	142	1501	0.057	ng	97
16) Acenaphthylene	14.12	152	11084	0.280	ng	97
17) Acenaphthene	14.47	154	713	0.027	ng	# 90
18) Fluorene	15.43	166	2922	0.082	ng	# 80
23) Phenanthrene	17.17	178	75356	1.280	ng	99
24) Anthracene	17.25	178	6784	0.129	ng	97
26) Fluoranthene	19.18	202	114190	1.452	ng	98
28) Pyrene	19.55	202	184661	2.919	ng	97
30) Benzo(a)anthracene	21.28	228	86547m	1.185	ng	
31) Chrysene	21.33	228	101847	1.374	ng	97
32) Bis(2-ethylhexyl)phthalate	21.22	149	30473	0.235	ng	98
33) Indeno(1,2,3-cd)pyrene	26.29	276	41904	0.482	ng	97
35) Benzo(b)fluoranthene	22.99	252	86686m	1.178	ng	
36) Benzo(k)fluoranthene	23.03	252	22347m	0.290	ng	
37) Benzo(a)pyrene	23.62	252	68622	1.001	ng	100
38) Dibenzo(a,h)anthracene	26.30	278	13059	0.183	ng	# 87
39) Benzo(a,h,i)perylene	27.08	276	49518	0.706	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE111519\
Data File : BE100743.D
Acq On : 15 Nov 2019 18:46
Operator : JU
Sample : K5728-09
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
EXT-034-SW093-110619-4

Manual Integrations
APPROVED

mohammad
11/18/2019 3:05:39 PM

Quant Time: Nov 15 23:19:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE111419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 15 15:55:40 2019
Response via : Initial Calibration

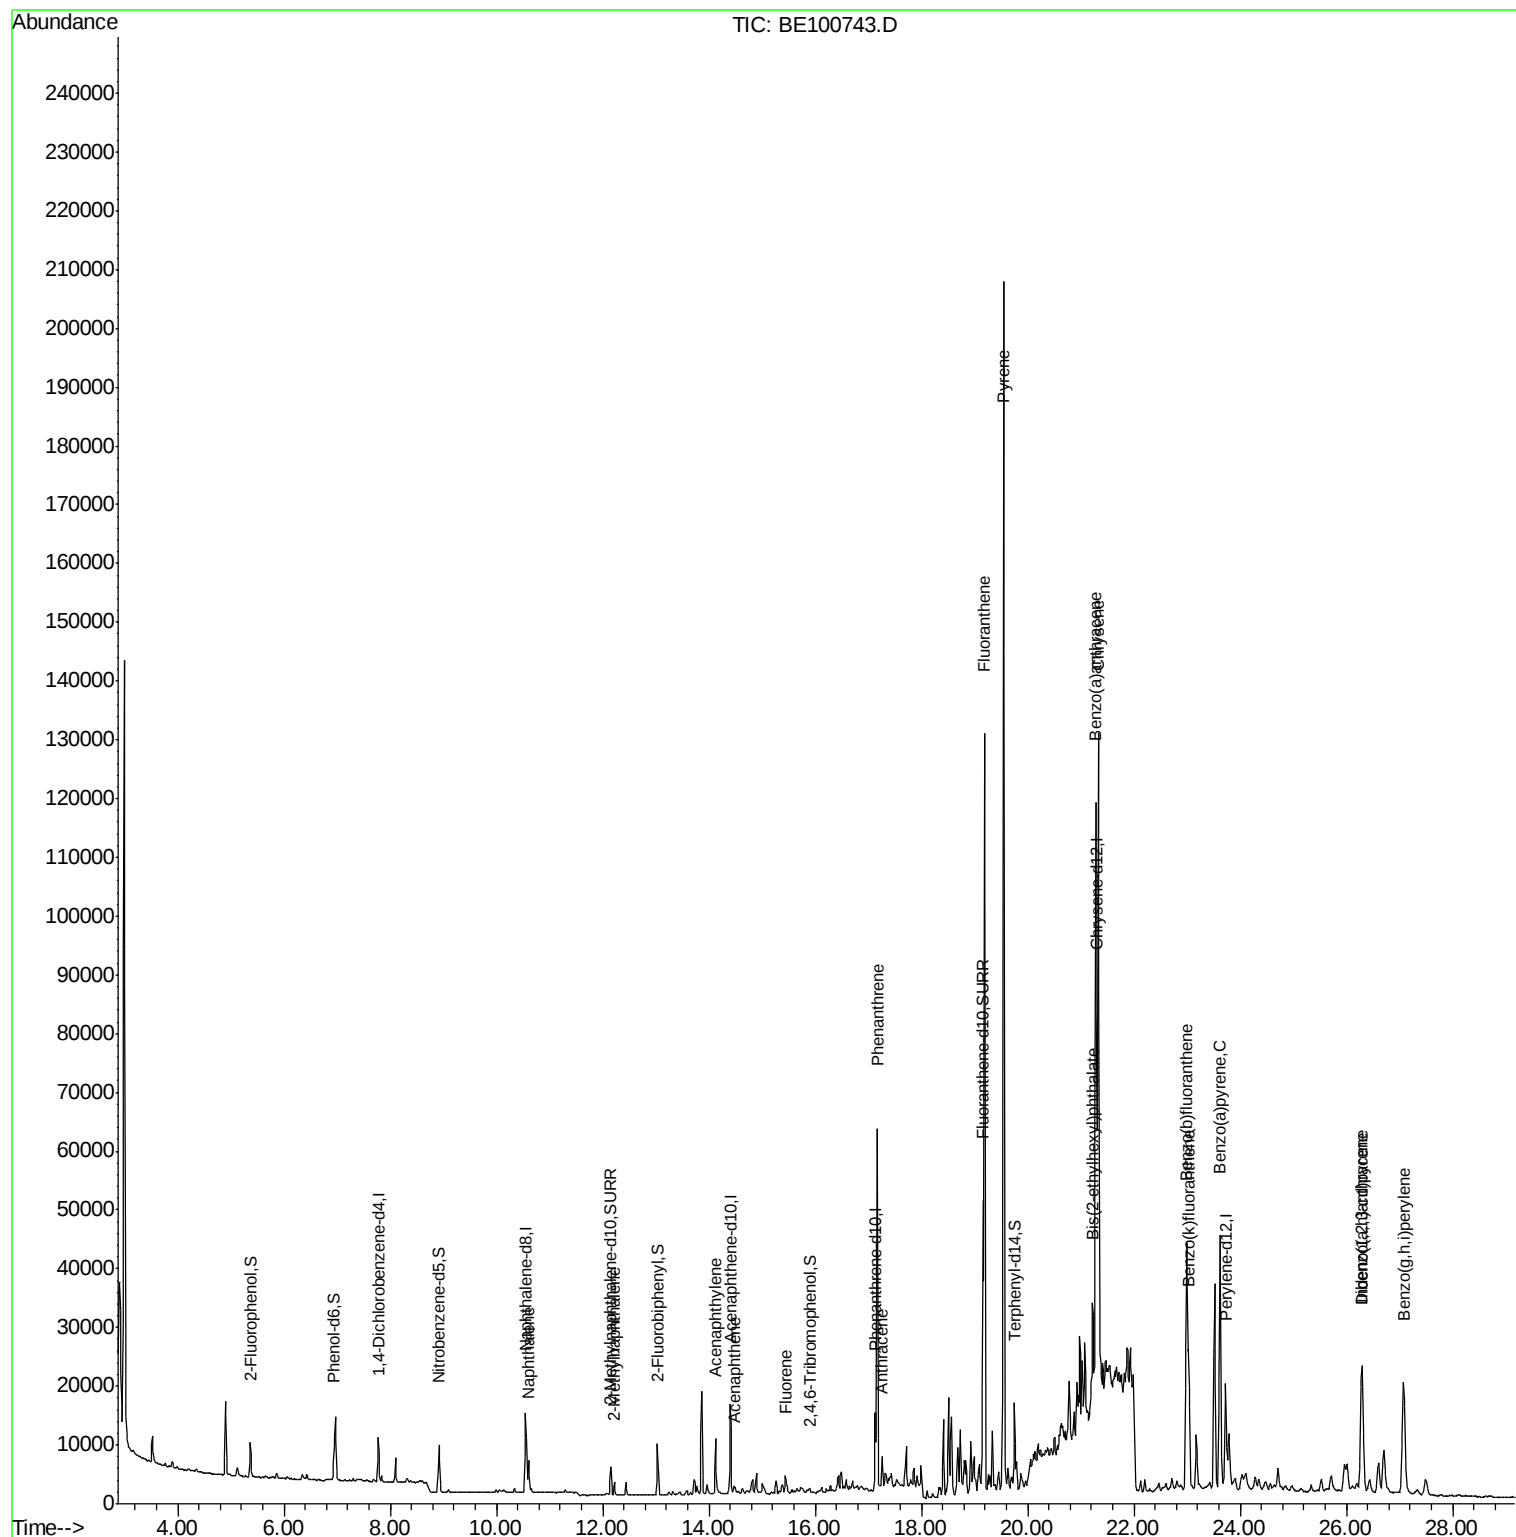



#1


1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.77 min Scan# 426
Delta R.T. -0.00 min
Lab File: BE100743.D
Acq: 15 Nov 2019 18:46

Instrument :
BNA_E
ClientSampleId :
EXT-034-SW093-110619-4

Tot Ion	Ratio	Lower	Upper
152	100		
150	156.7	123.4	185.0
115	68.3	52.1	78.1

Manual Integrations
APPROVED

mohammad
11/18/2019 3:05:39 PM



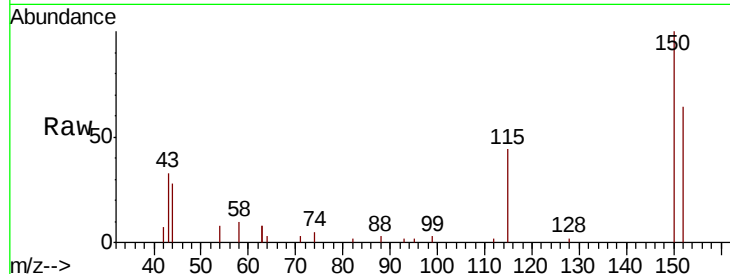


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

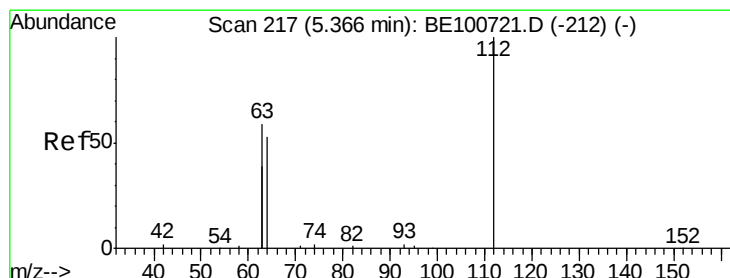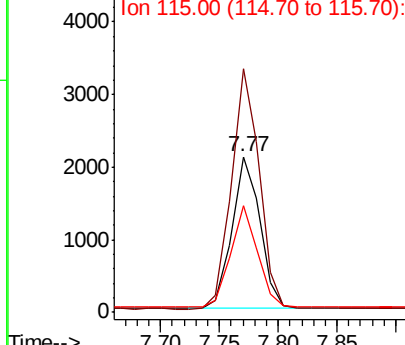

#4

2-Fluorophenol
Concen: 0.282 ng
RT: 5.36 min Scan# 217
Delta R.T. -0.00 min
Lab File: BE100743.D
Acq: 15 Nov 2019 18:46

Tgt Ion	Ratio	Lower	Upper
112	100		
64	72.2	58.3	87.5
63	145.0	115.4	173.2


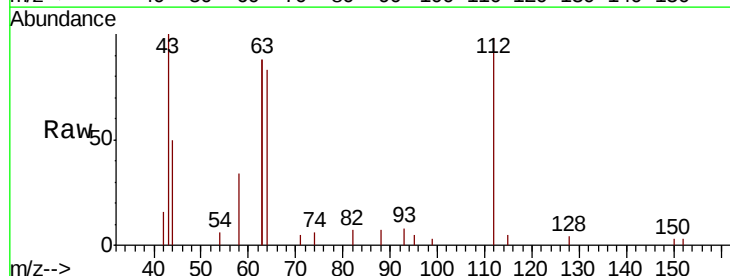



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE1

Ion 63.00 (62.70 to 63.70): BE1

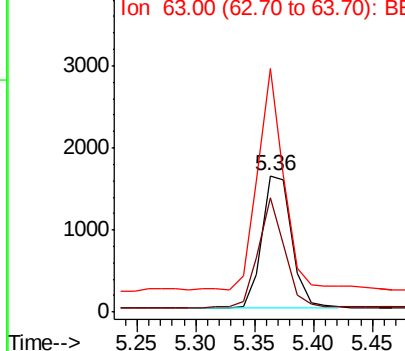



#5

Phenol-d6

Concen: 0.316 ng

RT: 6.94 min Scan# 354

Delta R.T. -0.00 min

Lab File: BE100743.D

Acq: 15 Nov 2019 18:46

Instrument :

BNA_E


ClientSampleId :

EXT-034-SW093-110619-4




Tot Ion:	99	Resp:	4537
Ion	Ratio	Lower	Upper
99	100		
42	31.6	17.8	26.6#
71	34.3	27.3	40.9

Manual Integrations
APPROVED

mohammad
11/18/2019 3:05:39 PM

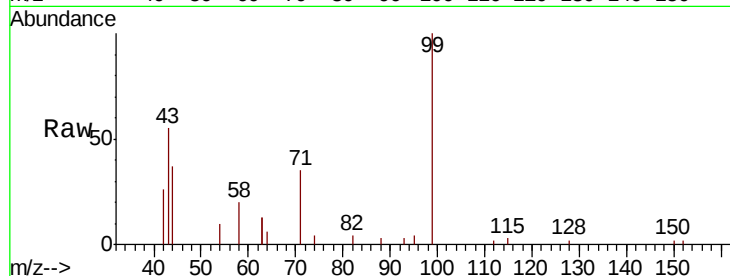

Abundance Ion 99.00 (98.70 to 99.70): BE1
Ion 42.00 (41.70 to 42.70): BE1
Ion 71.00 (70.70 to 71.70): BE1

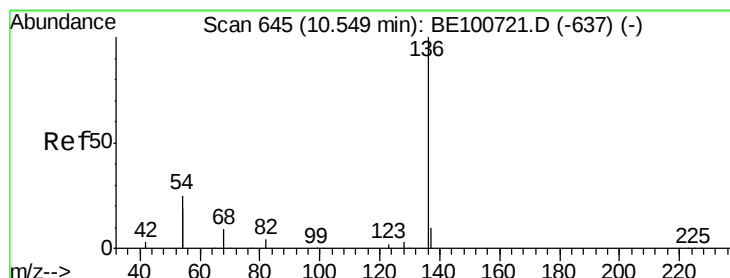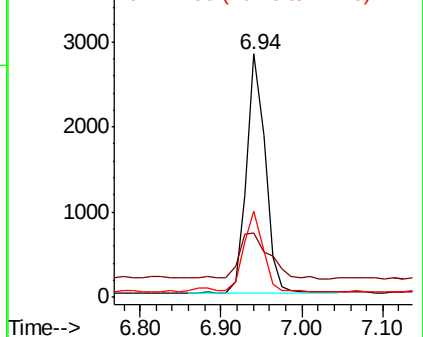

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.55 min Scan# 645




Delta R.T. -0.00 min


Lab File: BE100743.D

Acq: 15 Nov 2019 18:46

Tgt Ion:	136	Resp:	14950
Ion	Ratio	Lower	Upper
136	100		
137	11.6	9.1	13.7
54	46.3	39.0	58.6
68	9.1	7.8	11.8

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BE1
Ion 68.00 (67.70 to 68.70): BE1

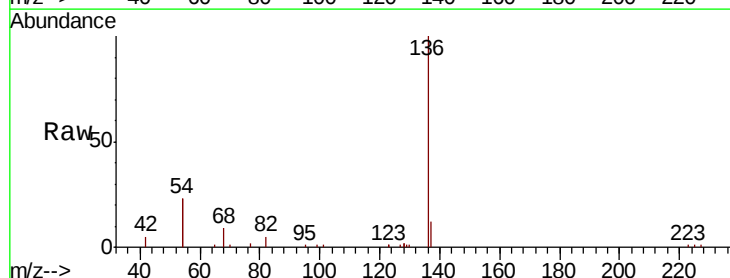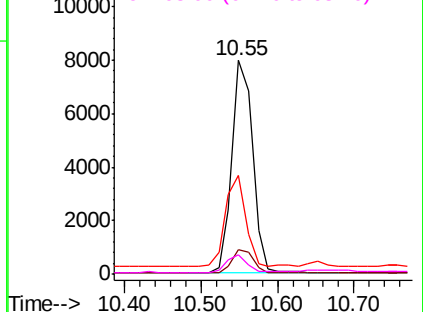



#8

Nitrobenzene-d5

Concen: 0.241 ng

RT: 8.91 min Scan# 519

Delta R.T. -0.00 min

Lab File: BE100743.D

Acq: 15 Nov 2019 18:46

Instrument :

BNA_E


ClientSampleId :

EXT-034-SW093-110619-4




Tot Ion:	82	Resp:	3059
Ion	Ratio	Lower	Upper
82	100		
128	123.2	99.6	149.4
54	241.6	183.8	275.8

Manual Integrations
APPROVED

mohammad
11/18/2019 3:05:39 PM

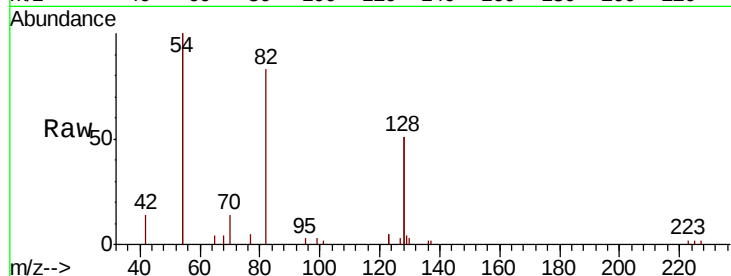

Abundance Ion 82.00 (81.70 to 82.70): BE1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BE1

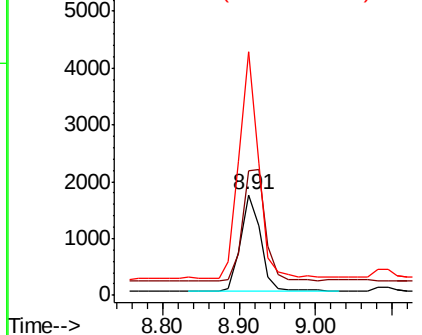

#9

Naphthalene

Concen: 0.055 ng

RT: 10.60 min Scan# 649




Delta R.T. -0.00 min


Lab File: BE100743.D

Acq: 15 Nov 2019 18:46

Tgt Ion:	128	Resp:	8573
Ion	Ratio	Lower	Upper
128	100		
129	3.6	2.4	3.6
127	3.9	2.7	4.1

Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E

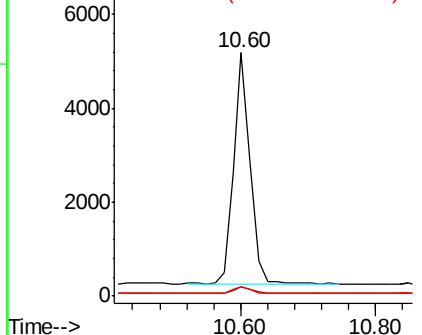

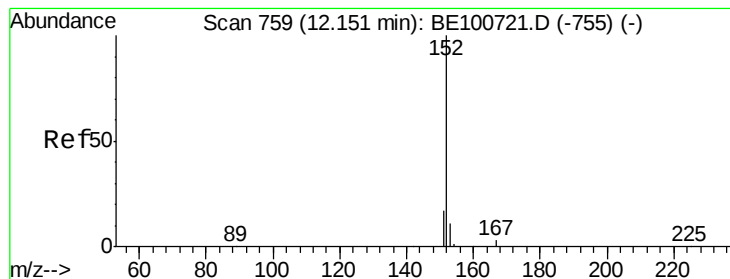





#11
 2-Methylnaphthalene-d10
 Concen: 0.249 ng
 RT: 12.15 min Scan# 759
 Delta R.T. 0.00 min
 Lab File: BE100743.D
 Acq: 15 Nov 2019 18:46

Instrument :
 BNA_E
 ClientSampleId :
 EXT-034-SW093-110619-4

Tot Ion	Ratio	Lower	Upper
152	100		
151	19.2	14.2	21.4




Manual Integrations
 APPROVED


mohammad
 11/18/2019 3:05:39 PM

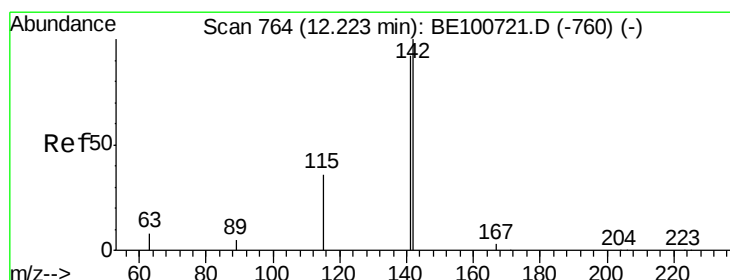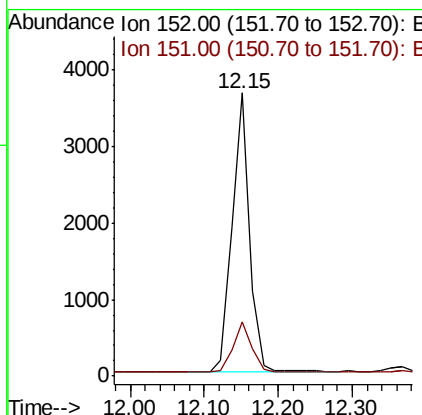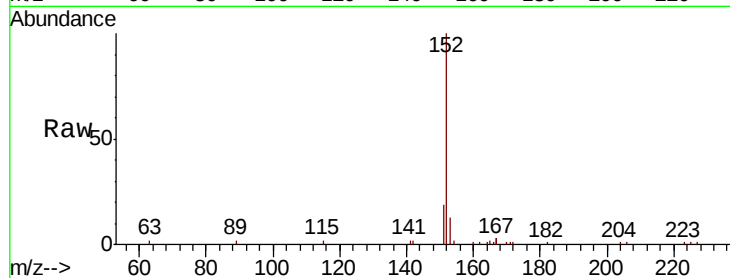

#12
 2-Methylnaphthalene
 Concen: 0.057 ng
 RT: 12.22 min Scan# 764
 Delta R.T. 0.00 min
 Lab File: BE100743.D
 Acq: 15 Nov 2019 18:46

Tgt Ion	Ratio	Lower	Upper
142	100		
141	90.3	73.3	109.9
115	40.7	29.9	44.9

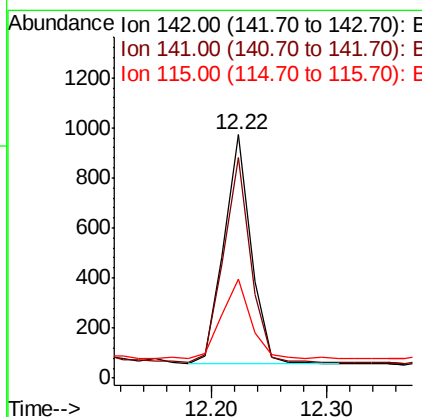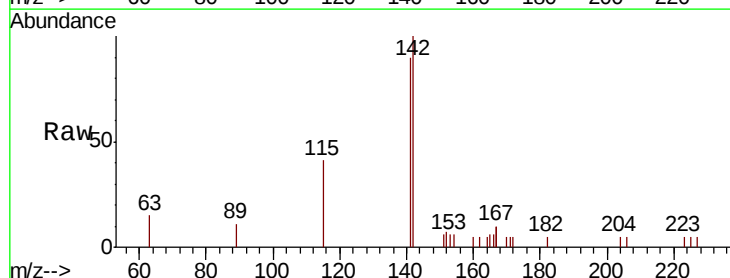




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.40 min Scan# 915
Delta R.T. -0.01 min
Lab File: BE100743.D
Acq: 15 Nov 2019 18:46

Instrument :
BNA_E
ClientSampleId :
EXT-034-SW093-110619-4

Tot Ion	Ratio	Lower	Upper
164	100		
162	100.0	77.8	116.8
160	46.7	35.3	52.9

Manual Integrations
APPROVED

mohammad
11/18/2019 3:05:39 PM



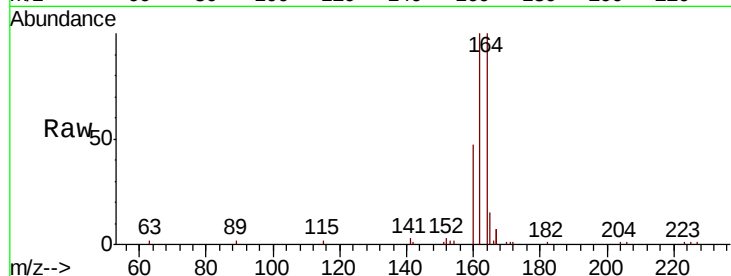


Abundance

Ion 164.00 (163.70 to 164.70): E


Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

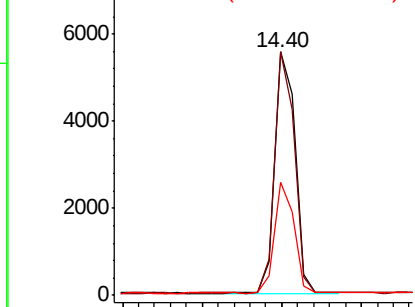

#14
2,4,6-Tribromophenol
Concen: 0.503 ng
RT: 15.89 min Scan# 1020
Delta R.T. 0.00 min
Lab File: BE100743.D
Acq: 15 Nov 2019 18:46

Tgt Ion	Ratio	Lower	Upper
330	100		
332	97.2	85.0	127.6
141	82.6	28.2	42.2#






Abundance

Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

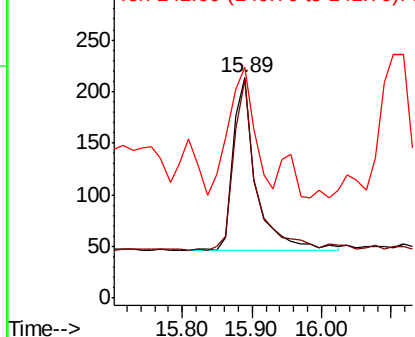







#15
2-Fluorobiphenyl
Concen: 0.220 ng
RT: 13.03 min Scan# 820
Delta R.T. 0.00 min
Lab File: BE100743.D
Acq: 15 Nov 2019 18:46

Instrument :
BNA_E
ClientSampleId :
EXT-034-SW093-110619-4

Tot Ion	Ratio	Lower	Upper
172	100		
171	33.9	28.1	42.1
170	23.7	19.8	29.6




Manual Integrations
APPROVED


mohammad
11/18/2019 3:05:39 PM

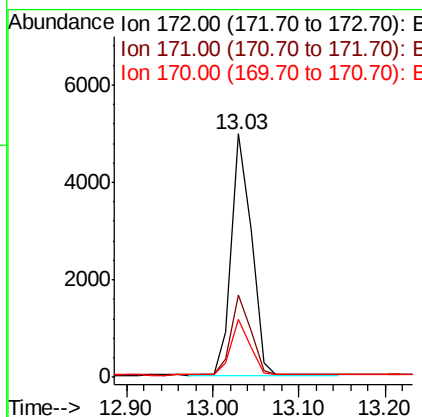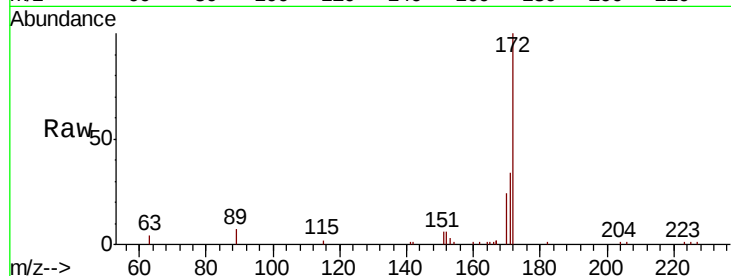

#16
Acenaphthylene
Concen: 0.280 ng
RT: 14.12 min Scan# 896
Delta R.T. 0.00 min
Lab File: BE100743.D
Acq: 15 Nov 2019 18:46

Tgt Ion	Ratio	Lower	Upper
152	100		
151	20.2	14.9	22.3
153	14.2	10.7	16.1

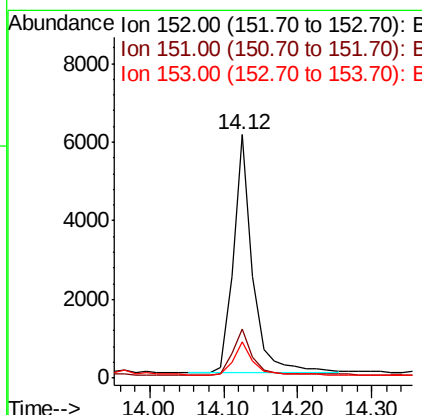




#17
Acenaphthene
Concen: 0.027 ng
RT: 14.47 min Scan# 920
Delta R.T. 0.00 min
Lab File: BE100743.D
Acq: 15 Nov 2019 18:46

Instrument :
BNA_E
ClientSampleId :
EXT-034-SW093-110619-4

Tot Ion	Ratio	Lower	Upper
154	100		
153	121.7	91.9	137.9
152	68.6	44.8	67.2#

Manual Integrations
APPROVED

mohammad
11/18/2019 3:05:39 PM



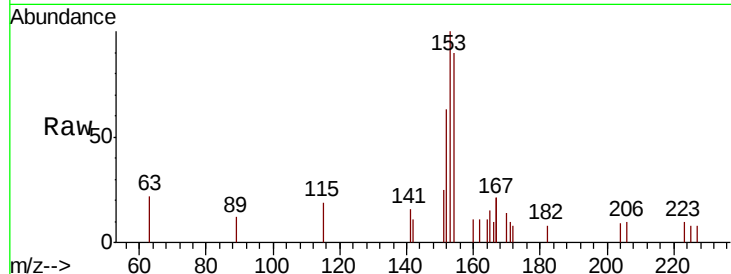


Abundance

Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

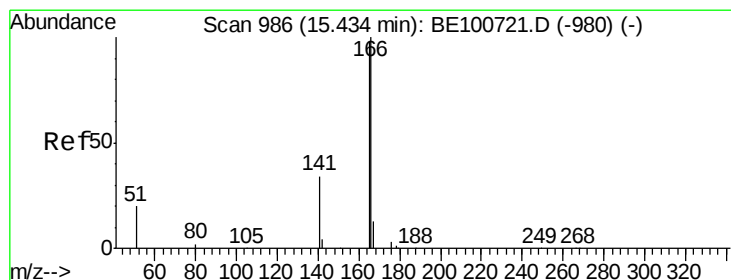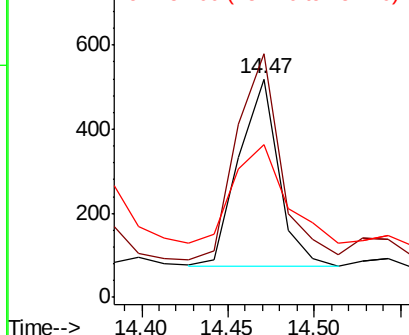

#18
Fluorene
Concen: 0.082 ng
RT: 15.43 min Scan# 986
Delta R.T. -0.00 min
Lab File: BE100743.D
Acq: 15 Nov 2019 18:46




Tgt Ion	Ratio	Lower	Upper
166	100		
165	119.4	78.2	117.4#
167	17.1	10.6	16.0#


Abundance

Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

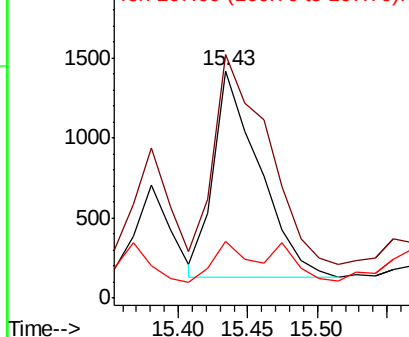



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.13 min Scan# 1113

Delta R.T. -0.00 min

Lab File: BE100743.D

Acq: 15 Nov 2019 18:46

Instrument :

BNA_E





ClientSampleId :

EXT-034-SW093-110619-4

Tot Ion:	188	Resp:	21604
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	5.8	5.4	8.0

Manual Integrations
APPROVED

mohammad
11/18/2019 3:05:39 PM

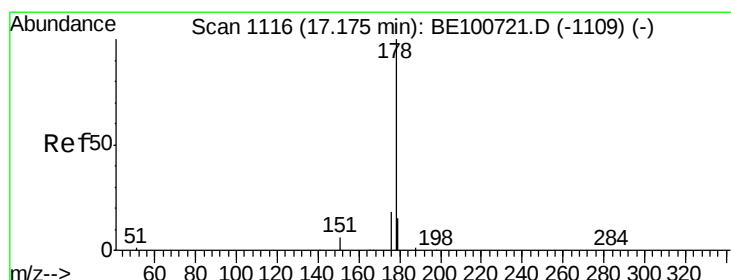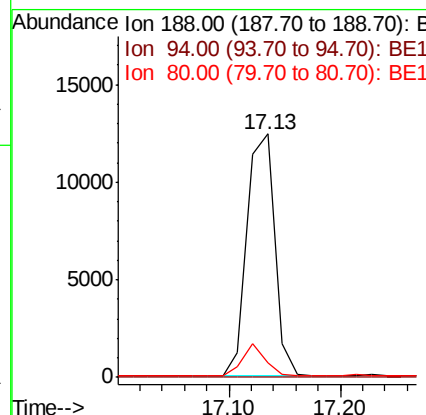

#23

Phenanthrene

Concen: 1.280 ng




RT: 17.17 min Scan# 1116


Delta R.T. -0.00 min

Lab File: BE100743.D

Acq: 15 Nov 2019 18:46

Tgt Ion:	178	Resp:	75356
Ion Ratio	Lower	Upper	
178	100		
176	19.2	15.0	22.4
179	15.7	12.6	18.8

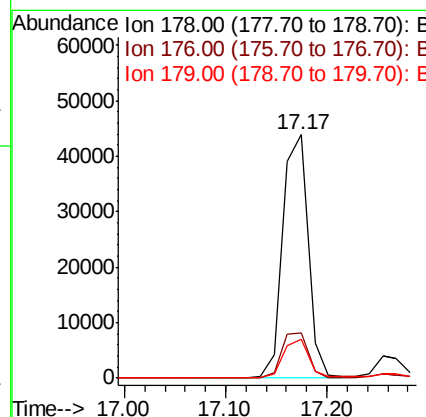







#24
 Anthracene
 Concen: 0.129 ng
 RT: 17.25 min Scan# 1122
 Delta R.T. -0.00 min
 Lab File: BE100743.D
 Acq: 15 Nov 2019 18:46

Instrument :
 BNA_E
 ClientSampleId :
 EXT-034-SW093-110619-4

Tot Ion	Ratio	Lower	Upper
178	100		
176	18.6	14.6	21.8
179	13.8	12.6	18.8




Manual Integrations
 APPROVED


mohammad
 11/18/2019 3:05:39 PM

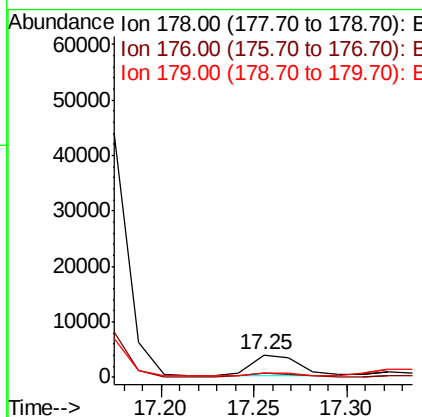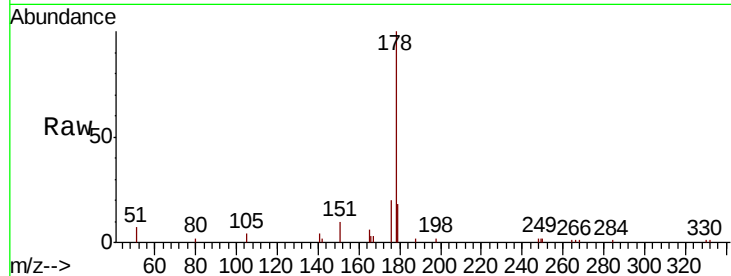

#25
 Fluoranthene-d10
 Concen: 0.215 ng
 RT: 19.16 min Scan# 1373
 Delta R.T. -0.00 min
 Lab File: BE100743.D
 Acq: 15 Nov 2019 18:46

Tgt Ion	Ratio	Lower	Upper
212	100		
106	2.7	2.2	3.4
104	1.8	1.2	1.8#

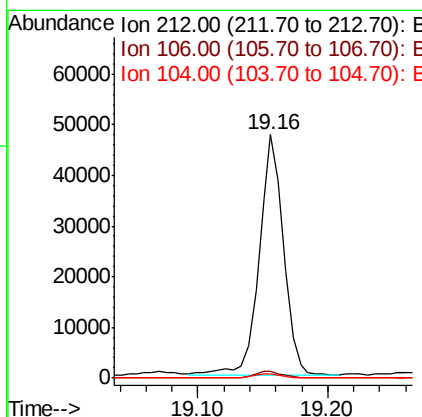

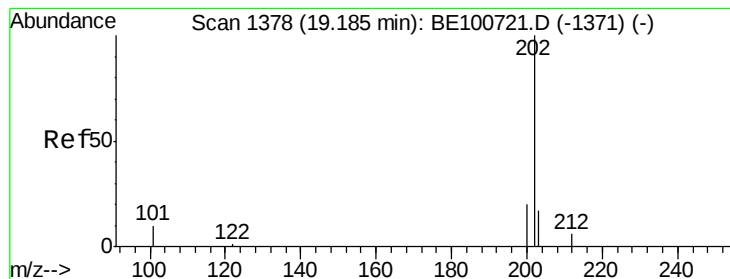

#26

Fluoranthene

Concen: 1.452 ng

RT: 19.18 min Scan# 1378

Delta R.T. -0.00 min

Lab File: BE100743.D

Acq: 15 Nov 2019 18:46

Instrument :

BNA_E





ClientSampleId :

EXT-034-SW093-110619-4

Tot Ion:	202	Resp:	114190
Ion Ratio	Lower	Upper	
202	100		
101	10.4	8.6	12.8
203	18.0	13.6	20.4

Manual Integrations
APPROVED

mohammad
11/18/2019 3:05:39 PM

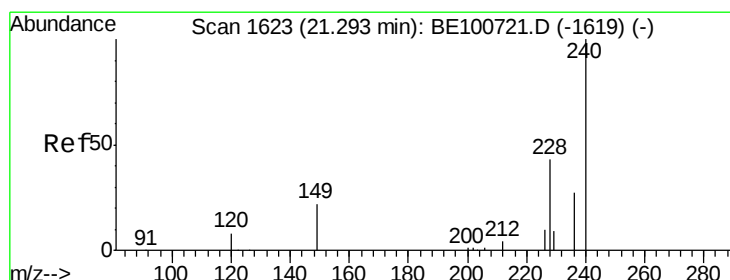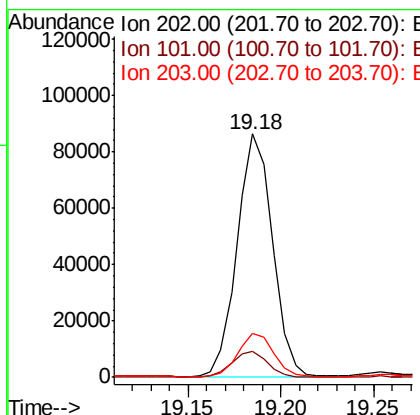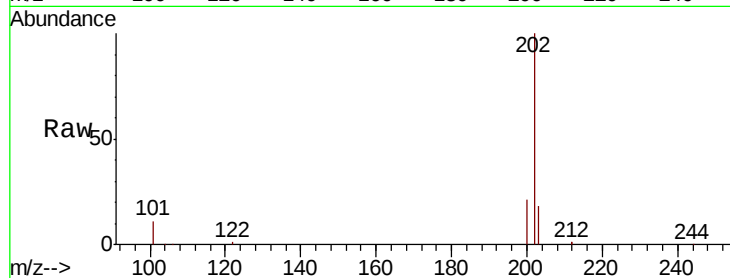

#27

Chrysene-d12

Concen: 0.400 ng




RT: 21.29 min Scan# 1624


Delta R.T. 0.00 min

Lab File: BE100743.D

Acq: 15 Nov 2019 18:46

Tgt Ion:	240	Resp:	22757
Ion Ratio	Lower	Upper	
240	100		
120	9.4	7.4	11.0
236	28.7	21.8	32.6

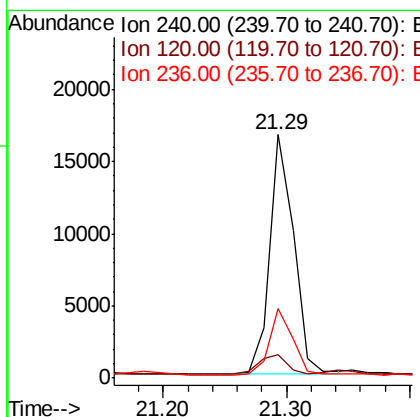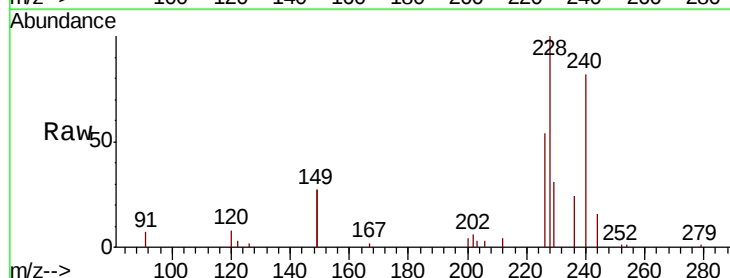




#28
Pvrene
Concen: 2.919 ng
RT: 19.55 min Scan# 1441
Delta R.T. -0.00 min
Lab File: BE100743.D
Acq: 15 Nov 2019 18:46

Instrument :
BNA_E
ClientSampleId :
EXT-034-SW093-110619-4

Tot Ion	Ratio	Resp	Lower	Upper
202	100	184661		
200	21.2		17.0	25.4
203	20.3		14.0	21.0

Manual Integrations
APPROVED

mohammad
11/18/2019 3:05:39 PM






Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

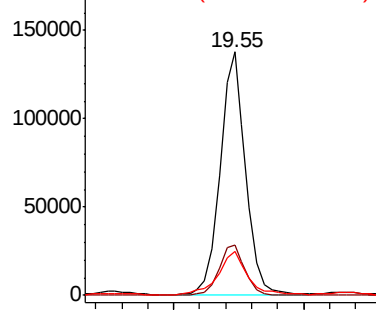

#29
Terphenyl-d14
Concen: 0.209 ng
RT: 19.75 min Scan# 1477
Delta R.T. -0.00 min
Lab File: BE100743.D
Acq: 15 Nov 2019 18:46




Tgt Ion	Ratio	Resp	Lower	Upper
244	100	11361		
212	35.6		24.3	36.5
122	10.7		7.6	11.4


Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

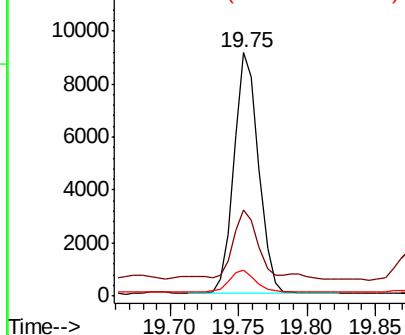



#30

Benzo(a)anthracene

Concen: 1.185 ng m

RT: 21.28 min Scan# 1623

Delta R.T. 0.00 min

Lab File: BE100743.D

Acq: 15 Nov 2019 18:46

Instrument :

BNA_E





ClientSampleId :

EXT-034-SW093-110619-4

Tot Ion	Ion	Ratio	Lower	Upper
228	100			
226	32.2	21.1	31.7	
229	23.4	15.9	23.9	

Manual Integrations
APPROVED

mohammad
11/18/2019 3:05:39 PM

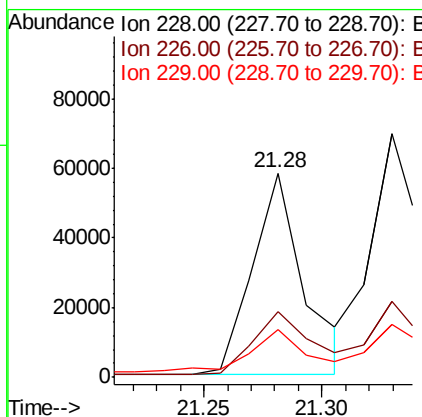

#31

Chrysene

Concen: 1.374 ng




RT: 21.33 min Scan# 1627


Delta R.T. 0.00 min

Lab File: BE100743.D

Acq: 15 Nov 2019 18:46

Tgt Ion	Ion	Ratio	Lower	Upper
228	100			
226	31.4	24.5	36.7	
229	21.8	15.5	23.3	

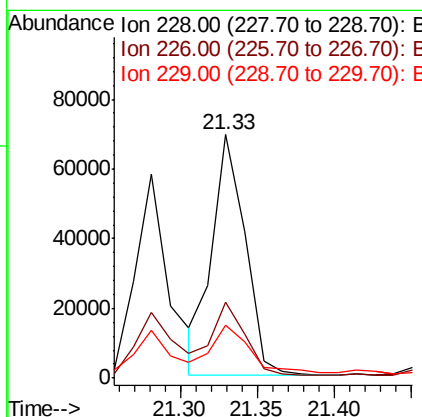



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.235 ng

RT: 21.22 min Scan# 1618

Delta R.T. 0.00 min

Lab File: BE100743.D

Acq: 15 Nov 2019 18:46

Instrument :

BNA_E





ClientSampleId :

EXT-034-SW093-110619-4

Tot Ion:	149	Resp:	30473
Ion Ratio	Lower	Upper	
149	100		
167	5.6	5.2	7.8
279	1.3	0.9	1.3

Manual Integrations
APPROVED

mohammad
11/18/2019 3:05:39 PM

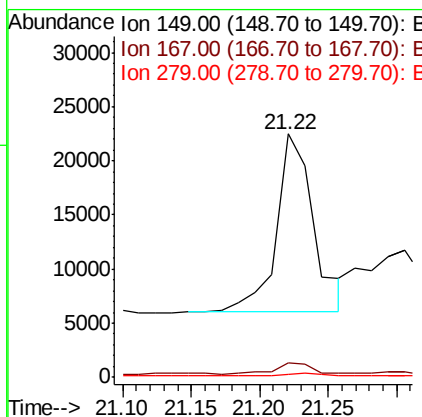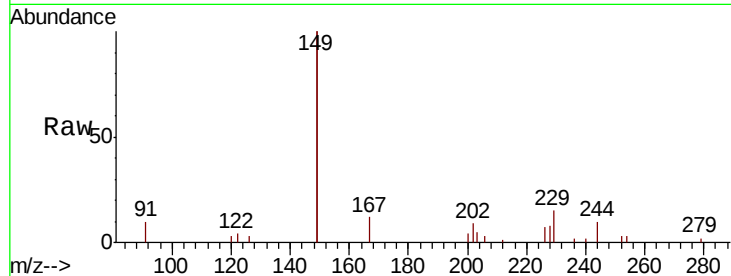

#33

Indeno(1,2,3-cd)pyrene

Concen: 0.482 ng




RT: 26.29 min Scan# 2874


Delta R.T. -0.00 min

Lab File: BE100743.D

Acq: 15 Nov 2019 18:46

Tgt Ion:	276	Resp:	41904
Ion Ratio	Lower	Upper	
276	100		
138	15.9	14.8	22.2
277	24.8	19.6	29.4

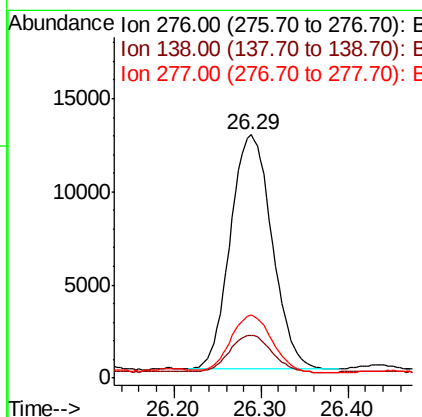

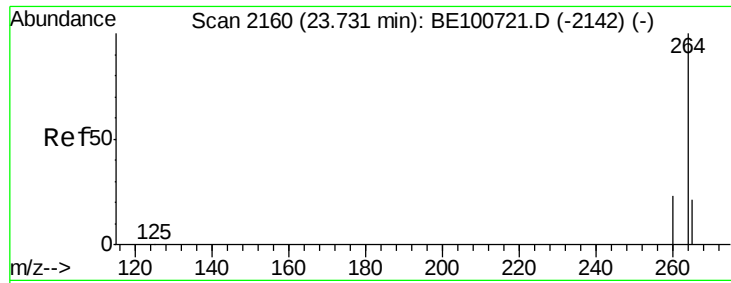





#34
Pervlene-d12
Concen: 0.400 ng
RT: 23.73 min Scan# 2161
Delta R.T. -0.00 min
Lab File: BE100743.D
Acq: 15 Nov 2019 18:46

Instrument :
BNA_E
ClientSampleId :
EXT-034-SW093-110619-4

Tot Ion	Ratio	Lower	Upper
264	100		
260	25.2	19.1	28.7
265	29.3	19.7	29.5




Manual Integrations
APPROVED


mohammad
11/18/2019 3:05:39 PM

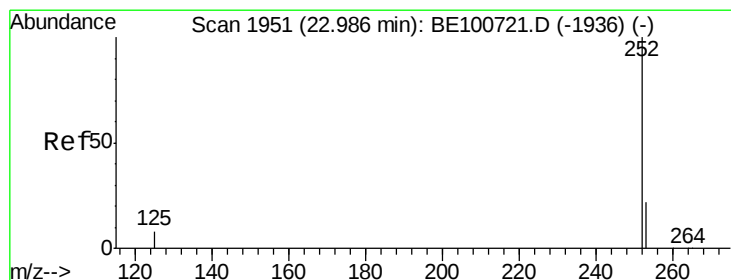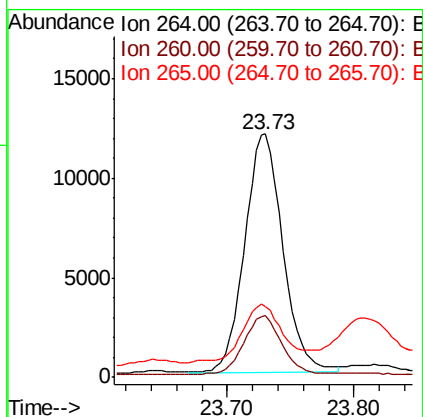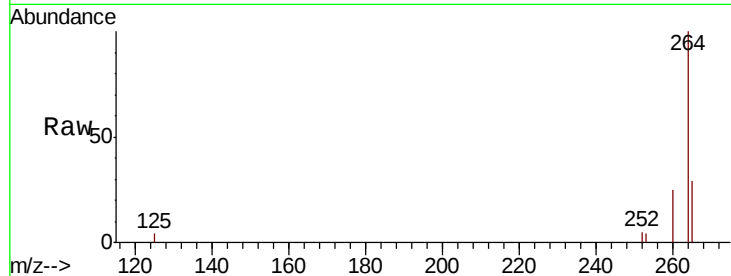

#35
Benzo(b)fluoranthene
Concen: 1.178 ng m
RT: 22.99 min Scan# 1954
Delta R.T. 0.01 min
Lab File: BE100743.D
Acq: 15 Nov 2019 18:46

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.5	18.7	28.1
125	9.4	7.0	10.4

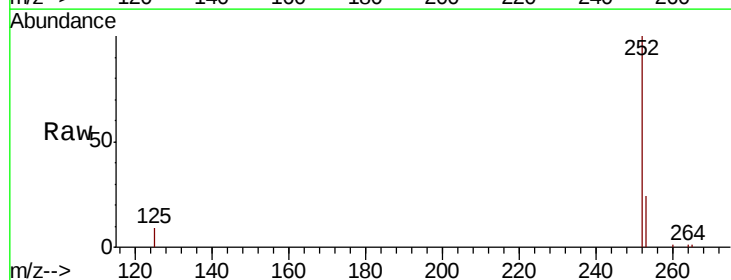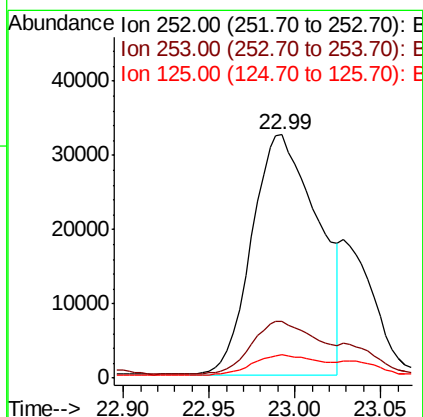

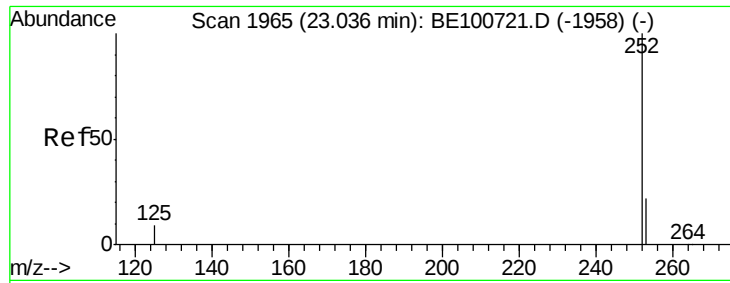





#36
Benzo(k)fluoranthene
Concen: 0.290 ng m
RT: 23.03 min Scan# 1964
Delta R.T. -0.01 min
Lab File: BE100743.D
Acq: 15 Nov 2019 18:46

Instrument :
BNA_E
ClientSampleId :
EXT-034-SW093-110619-4

Tot Ion	Ratio	Lower	Upper
252	100		
253	24.8	18.6	27.8
125	12.0	7.6	11.4




Manual Integrations
APPROVED


mohammad
11/18/2019 3:05:39 PM

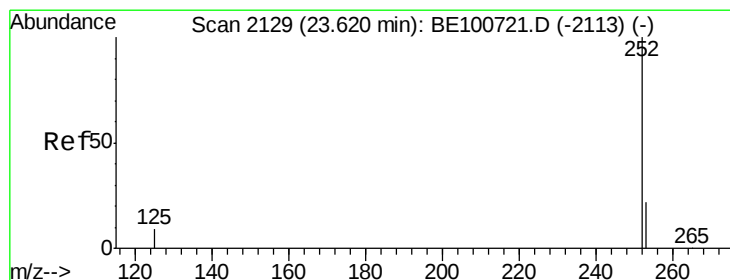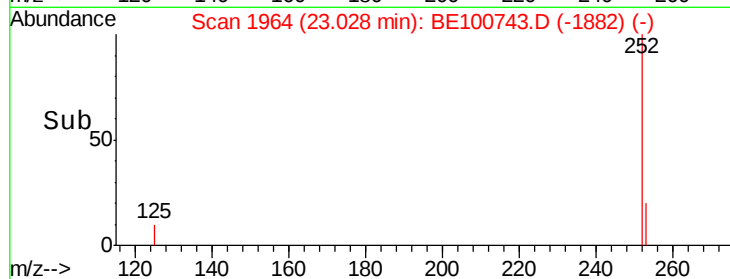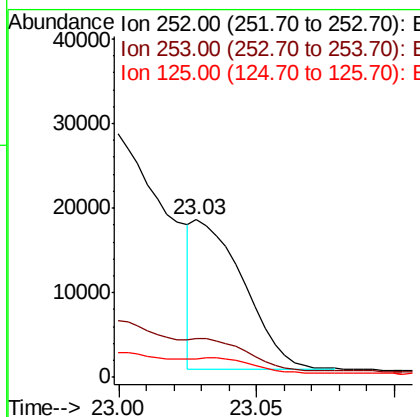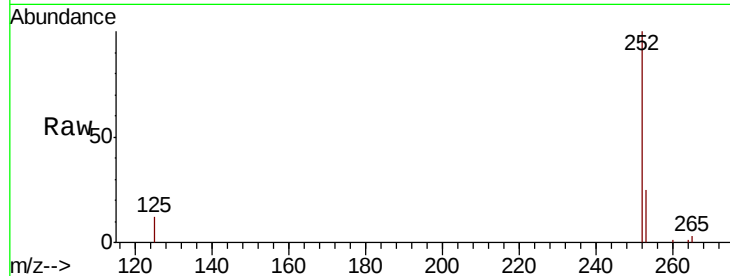

#37
Benzo(a)pyrene
Concen: 1.001 ng
RT: 23.62 min Scan# 2130
Delta R.T. -0.00 min
Lab File: BE100743.D
Acq: 15 Nov 2019 18:46

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.3	18.6	28.0
125	9.5	7.9	11.9

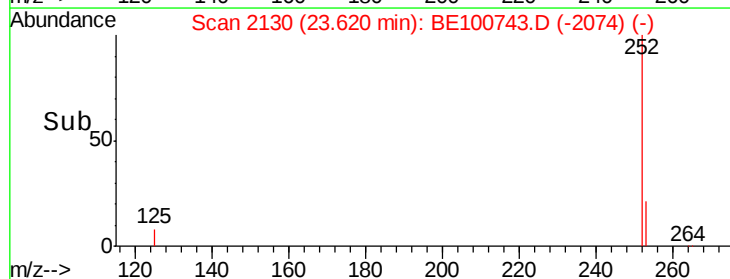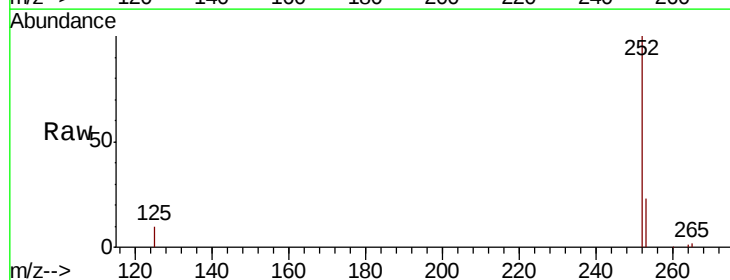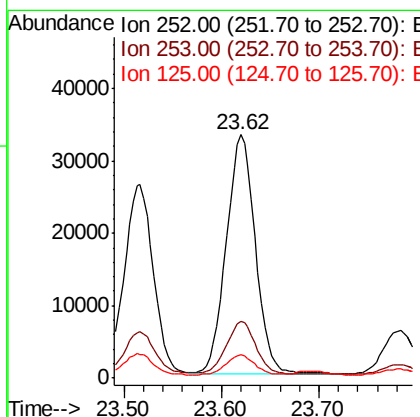







#38
Dibenzo(a,h)anthracene
Concen: 0.183 ng
RT: 26.30 min Scan# 2878
Delta R.T. -0.01 min
Lab File: BE100743.D
Acq: 15 Nov 2019 18:46

Instrument :
BNA_E
ClientSampleId :
EXT-034-SW093-110619-4

Tot Ion	Ratio	Lower	Upper
278	100		
139	17.6	10.3	15.5#
279	32.9	20.6	31.0#

Manual Integrations
APPROVED

mohammad
11/18/2019 3:05:39 PM

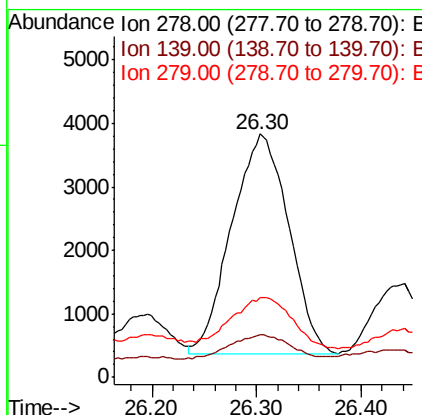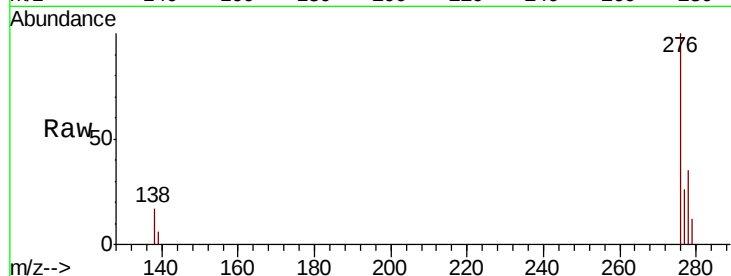

#39
Benzo(g,h,i)perylene
Concen: 0.706 ng
RT: 27.08 min Scan# 3095
Delta R.T. -0.00 min
Lab File: BE100743.D
Acq: 15 Nov 2019 18:46

Tgt Ion	Ratio	Lower	Upper
276	100		
277	24.9	19.8	29.6
138	17.2	13.6	20.4

