


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE111519\
 Data File : BE100728.D
 Acq On : 15 Nov 2019 8:50
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE111419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 15 15:55:40 2019

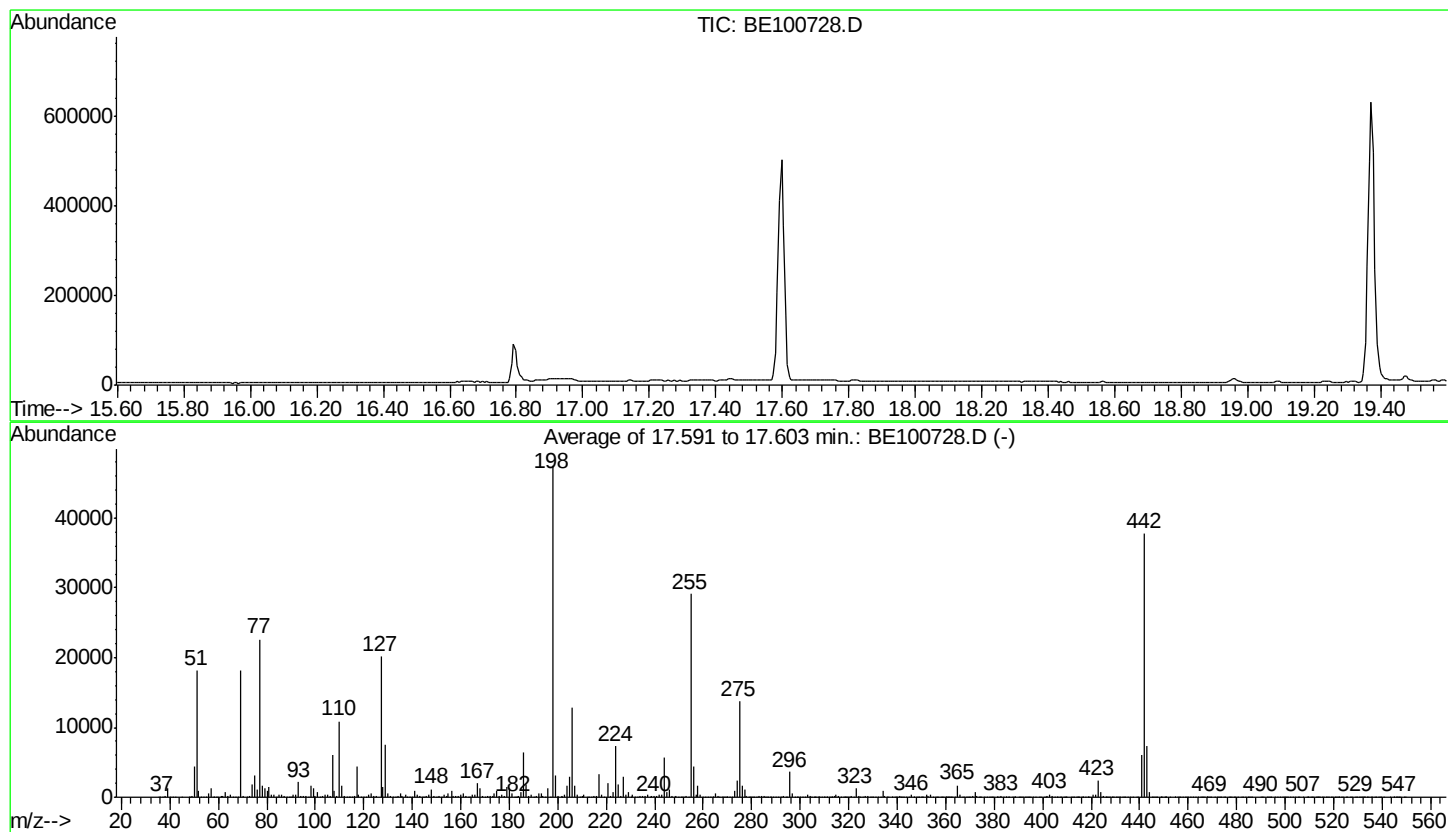

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2545

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	18097	PASS
68	69	0.00	2	0.5	87	PASS
69	198	0.00	100	38.3	18220	PASS
70	69	0.00	2	0.6	104	PASS
127	198	10	80	42.4	20153	PASS
197	198	0.00	2	0.2	89	PASS
198	198	100	100	100.0	47510	PASS
199	198	5	9	6.5	3065	PASS
275	198	10	60	28.9	13736	PASS
365	198	1	100	3.6	1698	PASS
441	198	0.01	100	12.7	6043	PASS
442	198	50	100	79.4	37725	PASS
443	442	15	24	19.4	7306	PASS